
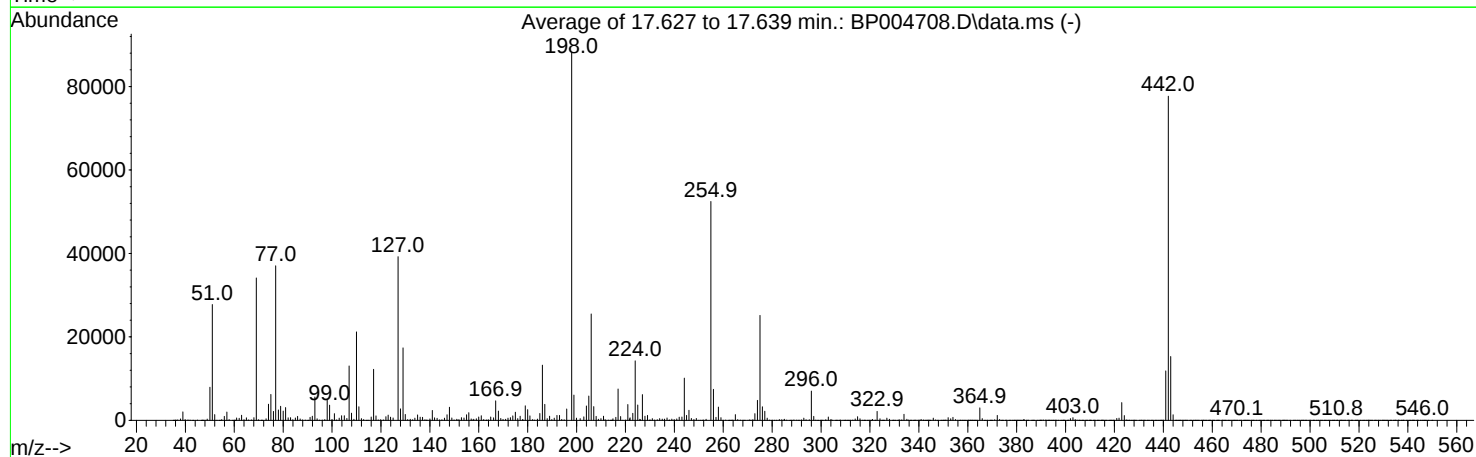


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021121\
 Data File : BP004708.D
 Acq On : 11 Feb 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 05 18:04:48 2021

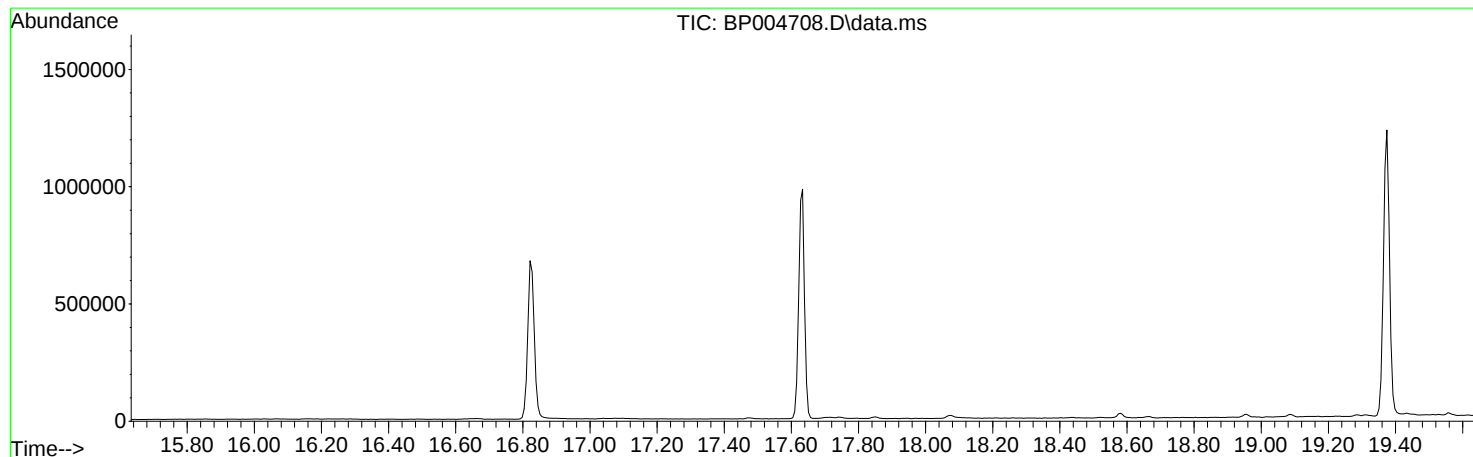

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	27776	PASS
68	69	0.00	2	1.9	643	PASS
69	198	0.00	100	38.7	34121	PASS
70	69	0.00	2	0.5	157	PASS
127	198	10	80	44.5	39224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88160	PASS
199	198	5	9	6.9	6079	PASS
275	198	10	60	28.5	25168	PASS
365	198	1	100	3.4	3007	PASS
441	198	0.01	100	13.4	11837	PASS
442	442	100	100	100.0	77691	PASS
443	442	15	24	19.7	15317	PASS

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/11/2021	BNA_P	<u>BP004708.D</u>
Compound Name	Response	Retention Time
DDT	324914	20.57
DDD	1350	21.14
DDE	564	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1914	326828	0.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021121\
Data File : BP004708.D
Acq On : 11 Feb 2021 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 11 11:17:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 05 18:04:48 2021
Response via : Initial Calibration

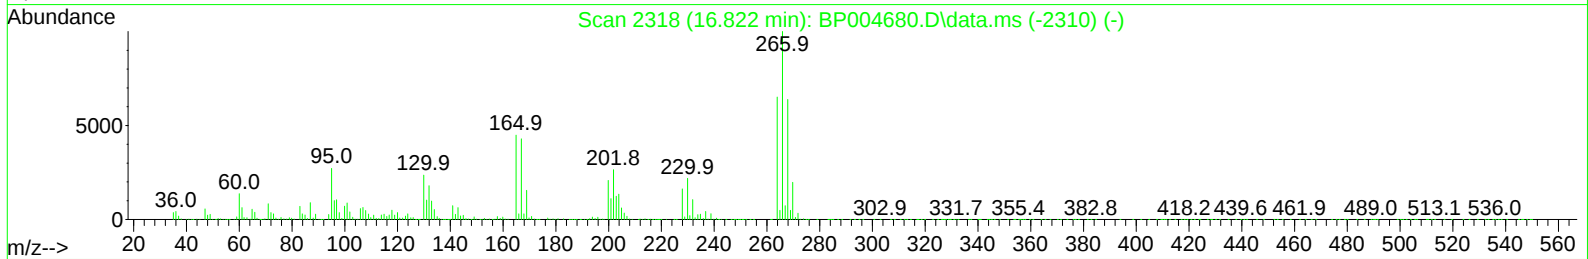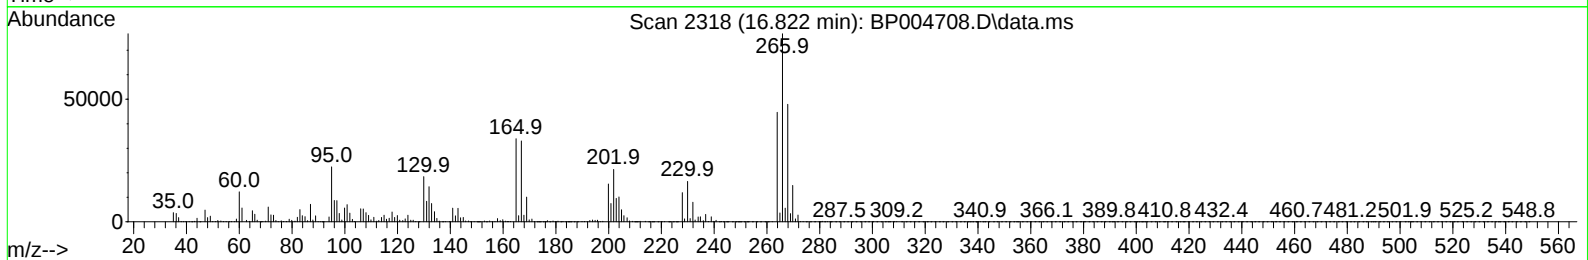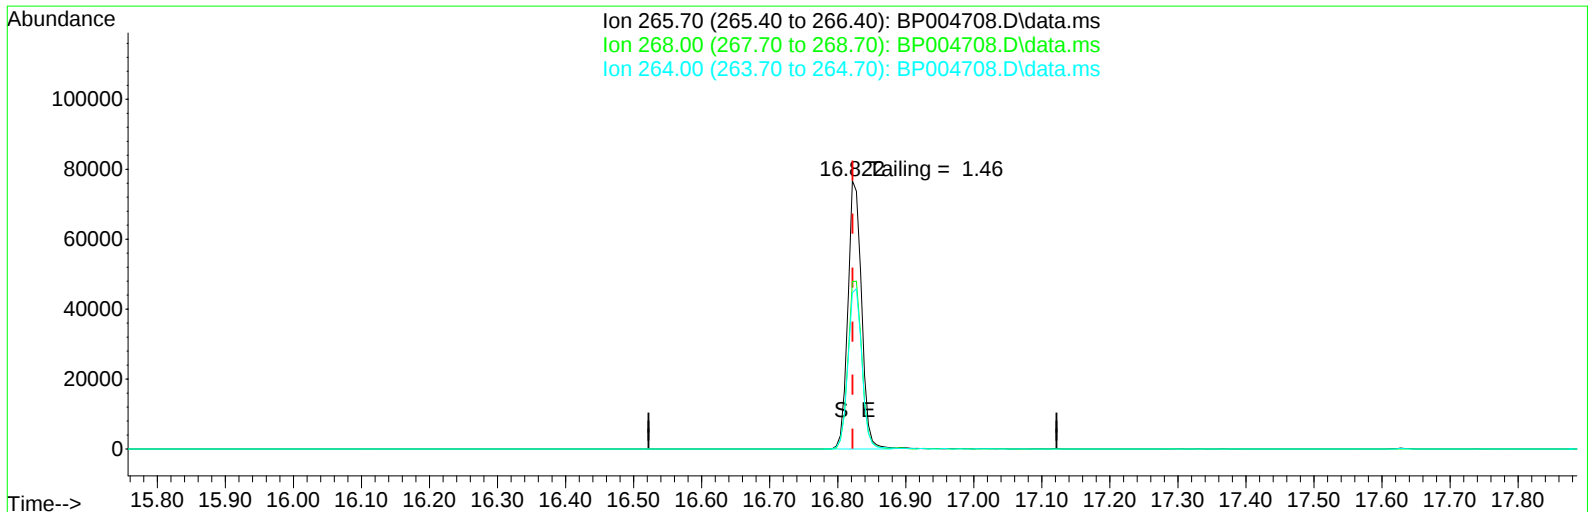

TIC: BP004708.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.000) 110916.21 ng




response 106229

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.45
264.00	63.30	58.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021121\
Data File : BP004708.D
Acq On : 11 Feb 2021 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 11 11:17:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 05 18:04:48 2021
Response via : Initial Calibration

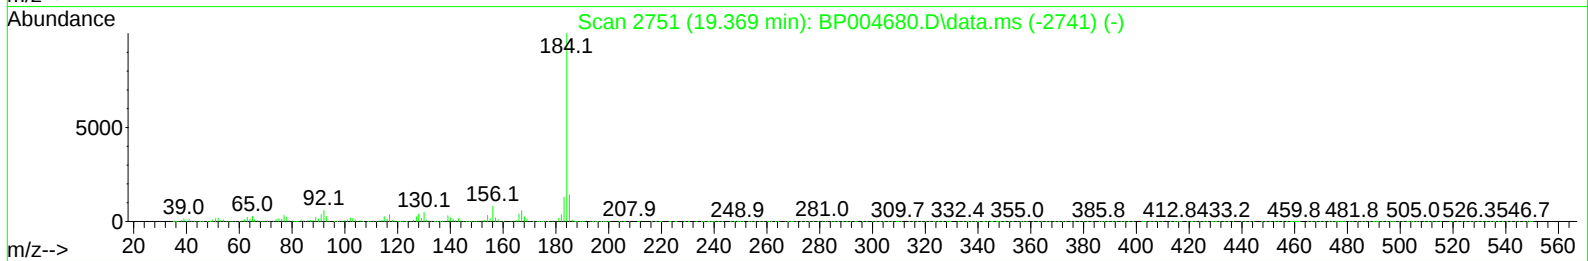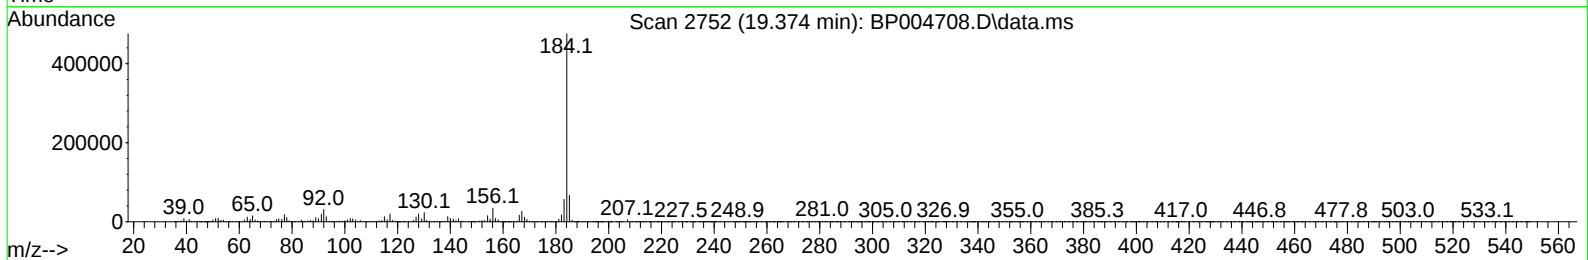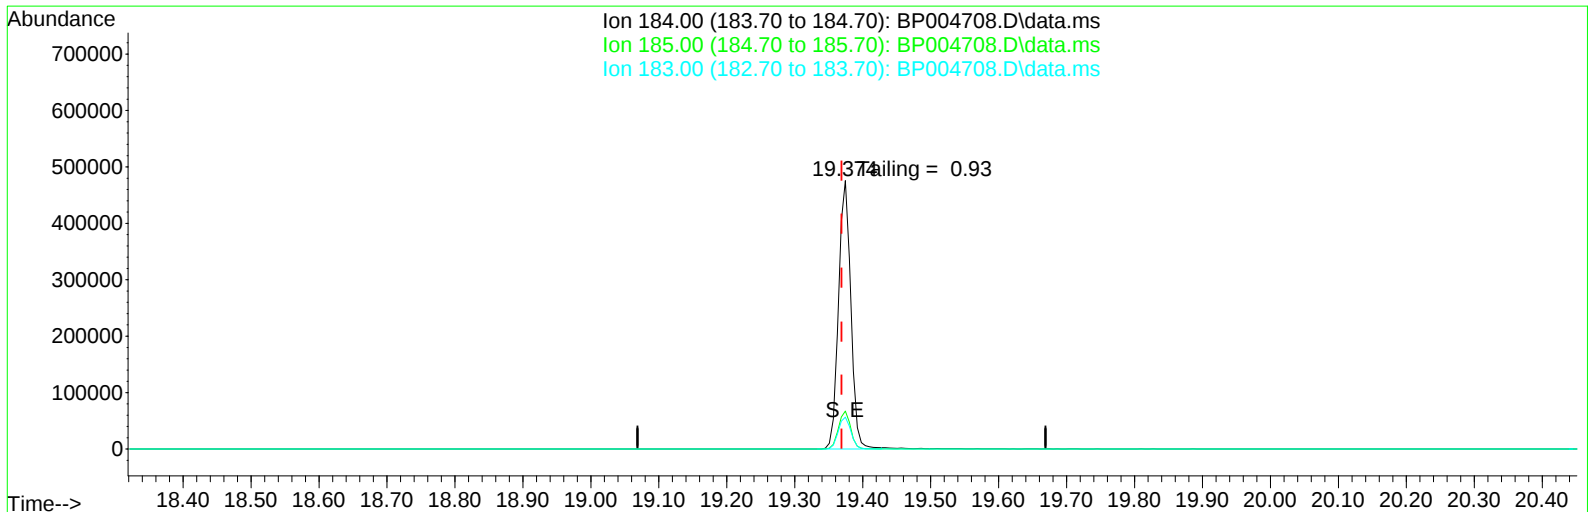

TIC: BP004708.D\data.ms

(77) Benzidine

19.374min (+ 0.005) 6989.26 ng

response 599900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	12.00	11.90
0.00	0.00	0.00