
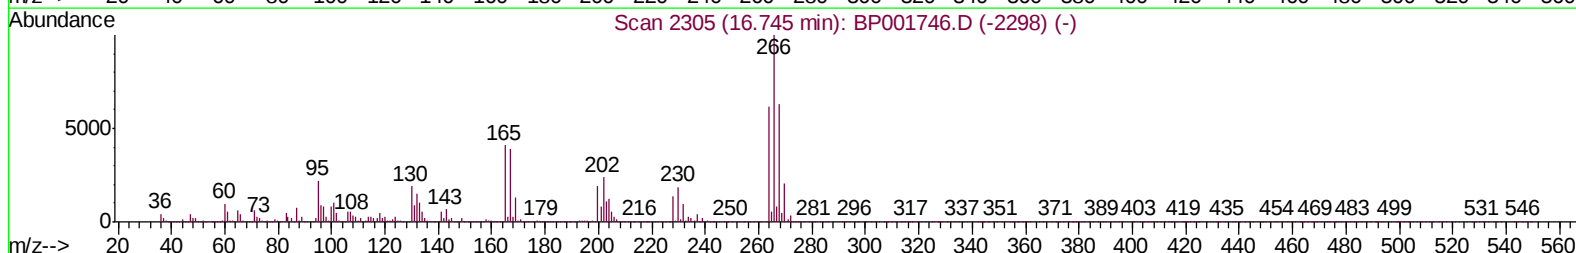
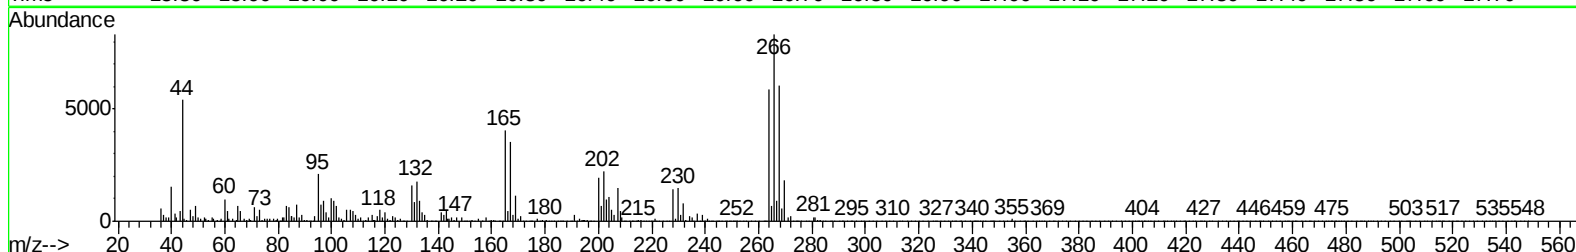


Data File : BP001748.D
Acq On : 14 Feb 2020 16:39
Operator : CG/JU
Sample : K5695-08
Misc : MDL-WATER-01
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Feb 15 04:48:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 15 04:45:21 2020
Response via : Initial Calibration

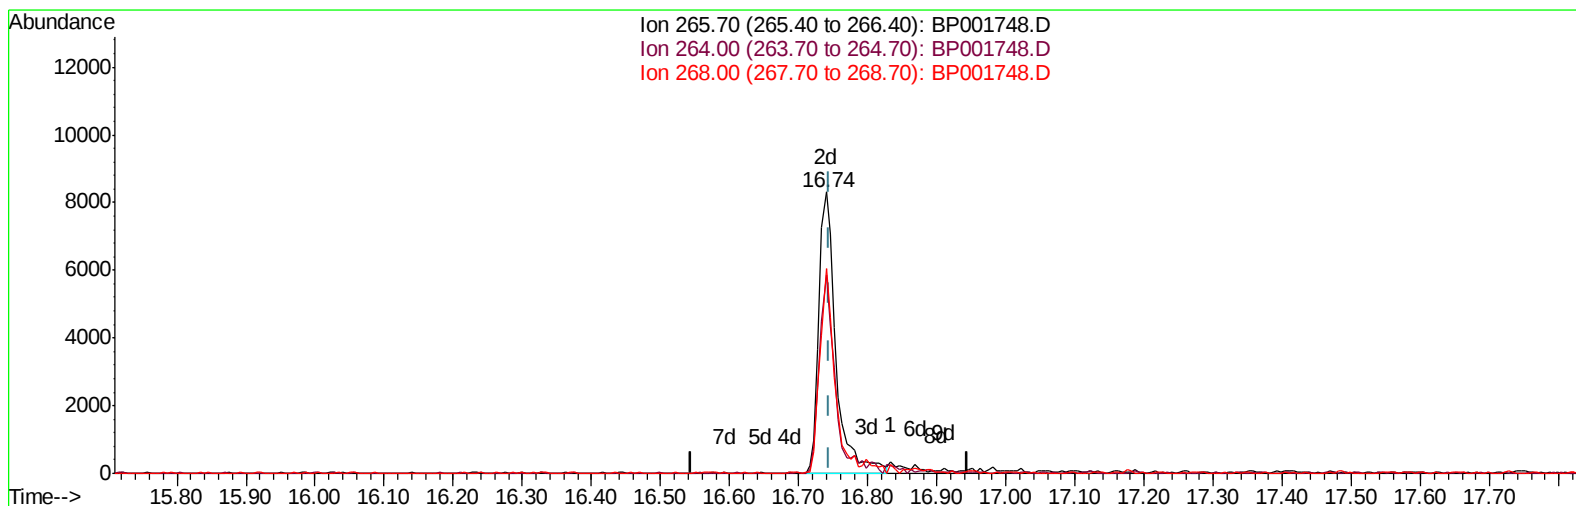

TIC: BP001748.D

(69) Pentachlorophenol (C)

16.739min (-0.005) 1.68ng/ul m

response 14209

Ion	Exp%	Act%
265.70	100	100
264.00	63.70	70.43
268.00	63.50	72.87
0.00	0.00	0.00