
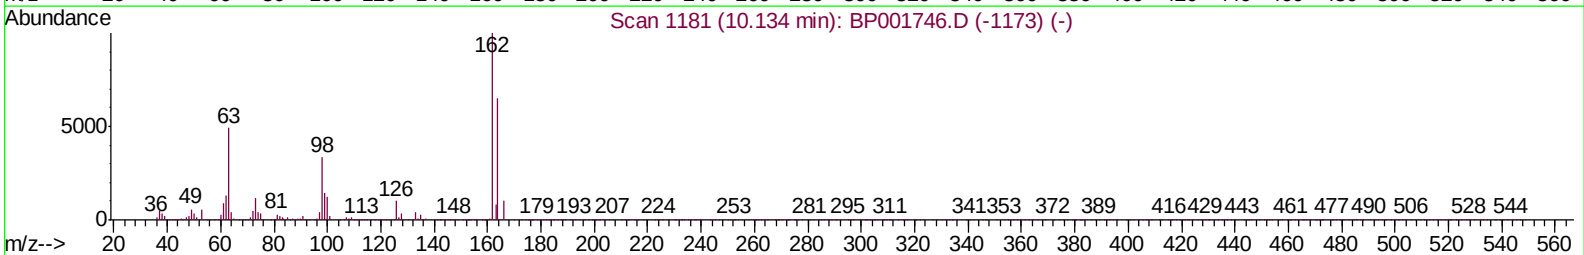
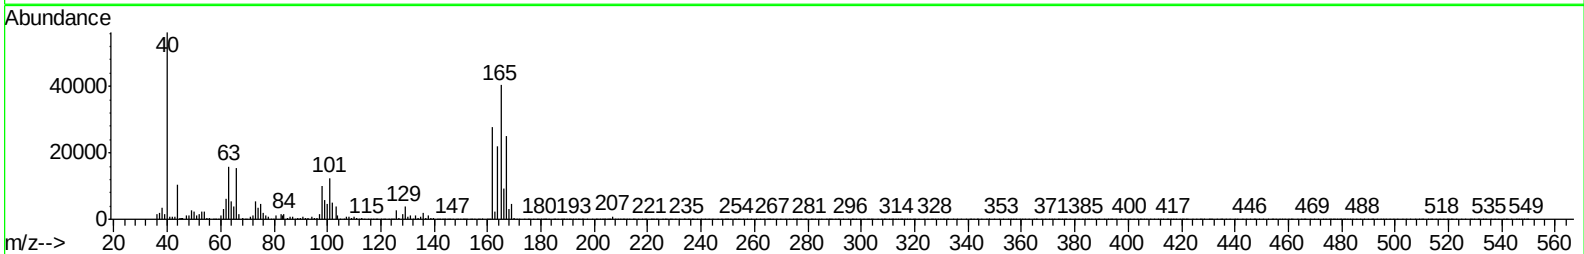


Data File : BP001750.D
Acq On : 14 Feb 2020 17:47
Operator : CG/JU
Sample : K5695-10
Misc : MDL-WATER-03
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 15 04:49:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 15 04:45:21 2020
Response via : Initial Calibration

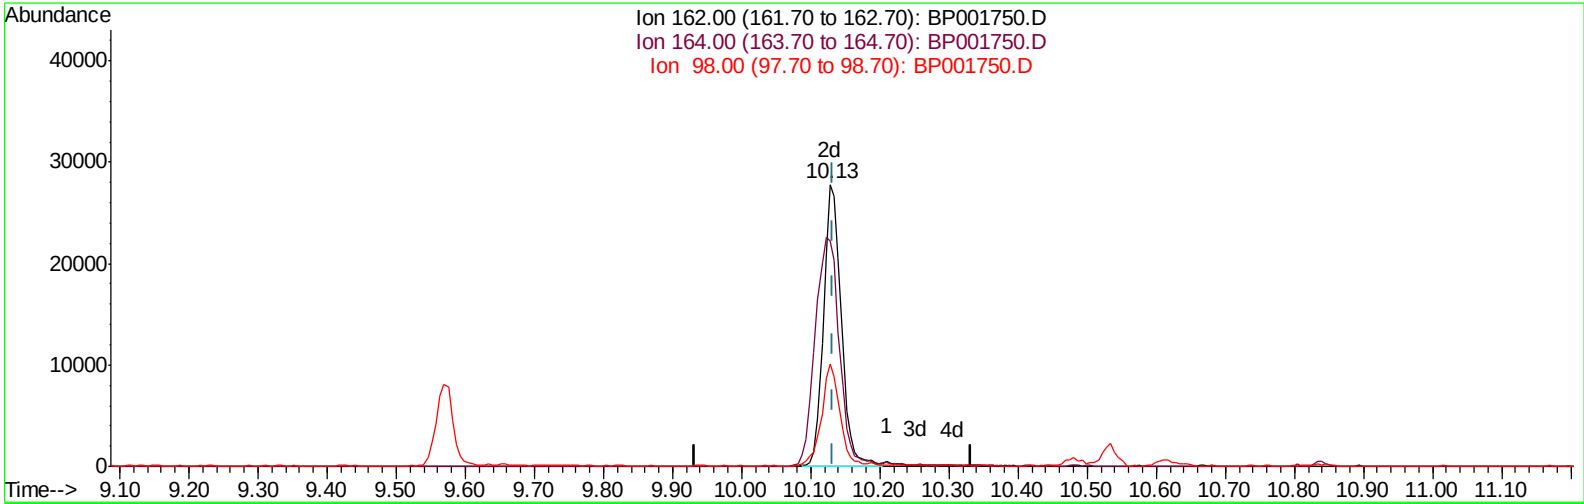

TIC: BP001750.D

(27) 2,4-Dichlorophenol (C)

10.128min (-0.005) 2.87ng/ul m

response 49412

Ion	Exp%	Act%
162.00	100	100
164.00	65.20	79.81#
98.00	33.30	36.20
0.00	0.00	0.00