
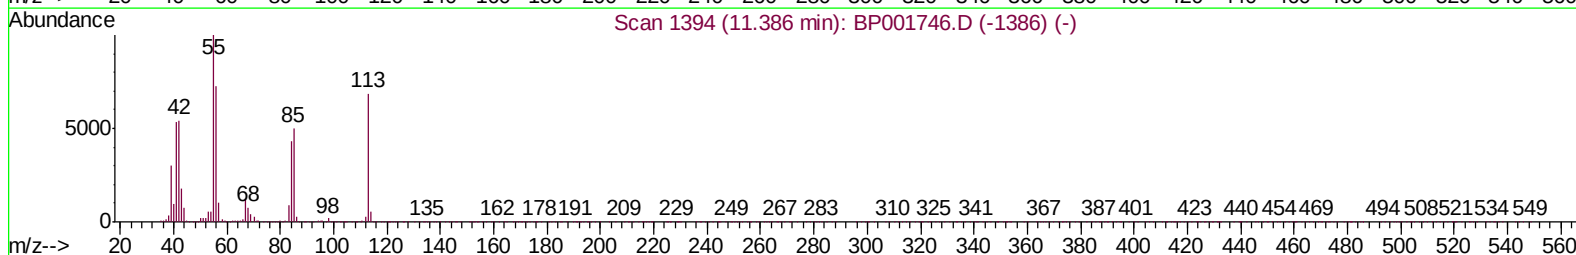
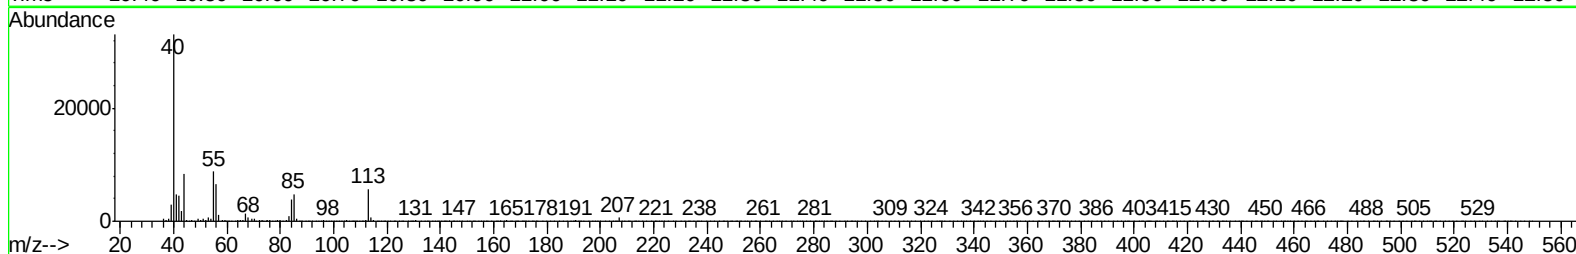


Data File : BP001751.D
Acq On : 14 Feb 2020 18:20
Operator : CG/JU
Sample : K5695-11
Misc : MDL-WATER-04
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 15 04:50:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 15 04:45:21 2020
Response via : Initial Calibration

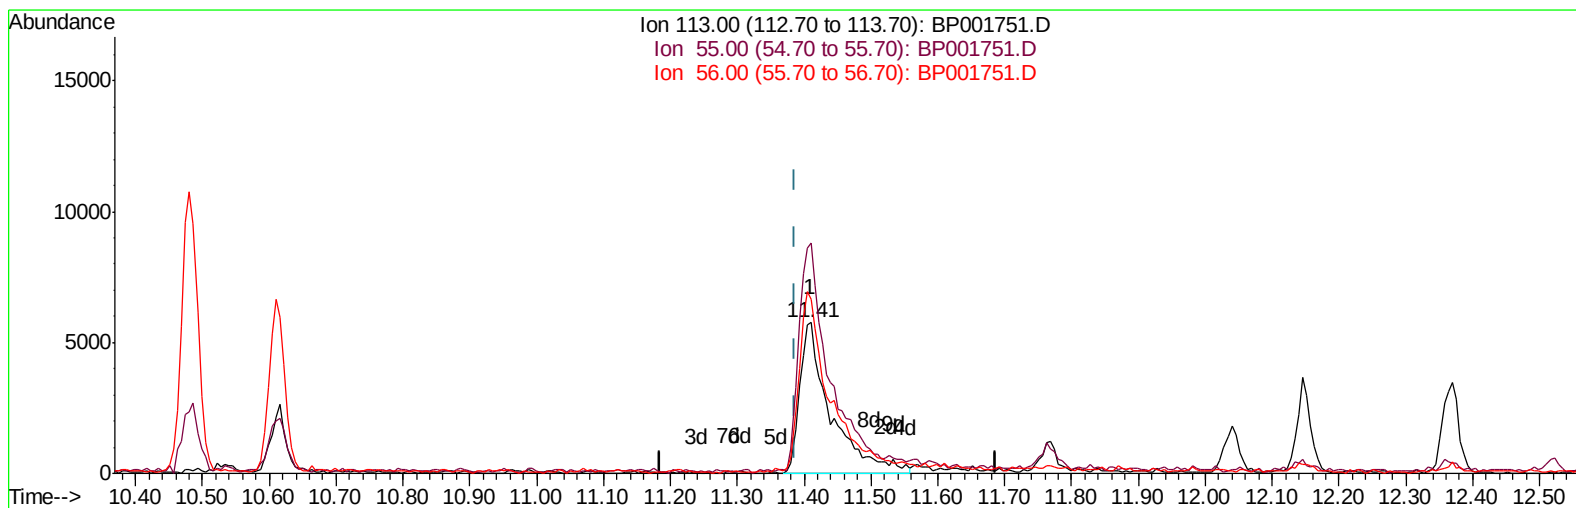

TIC: BP001751.D

(32) Caprolactam

11.410min (+0.024) 2.13ng/ul m

response 18768

Ion	Exp%	Act%
113.00	100	100
55.00	146.60	153.01
56.00	113.40	115.19
0.00	0.00	0.00