

Data File : BP001752.D

Acq On : 14 Feb 2020 18:54

Operator : CG/JU

Sample : K5695-12

Misc : MDL-WATER-05

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Feb 15 04:51:30 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Feb 15 04:45:21 2020

Response via : Initial Calibration

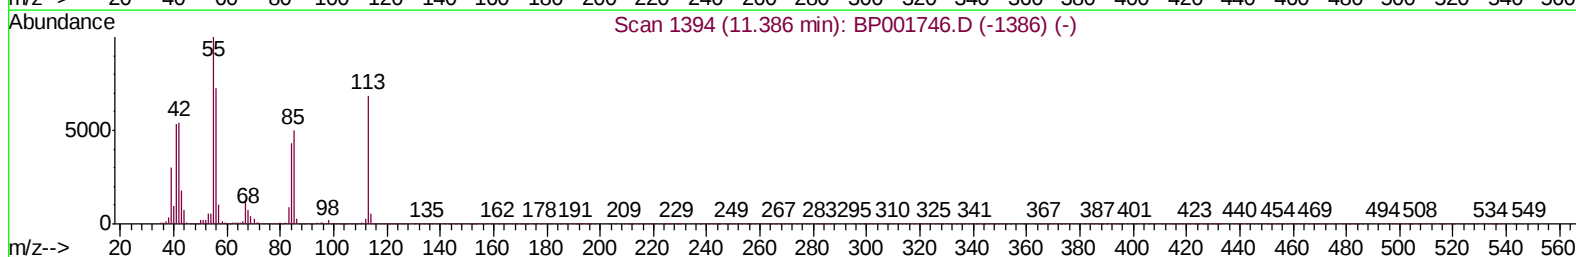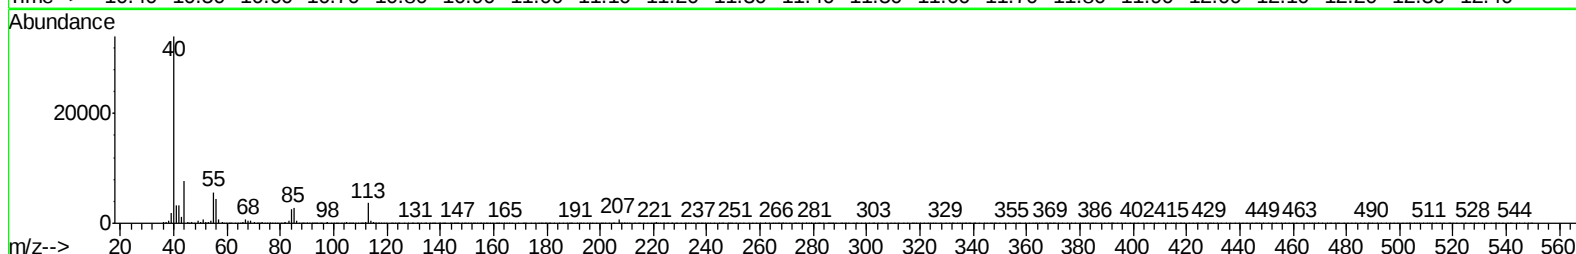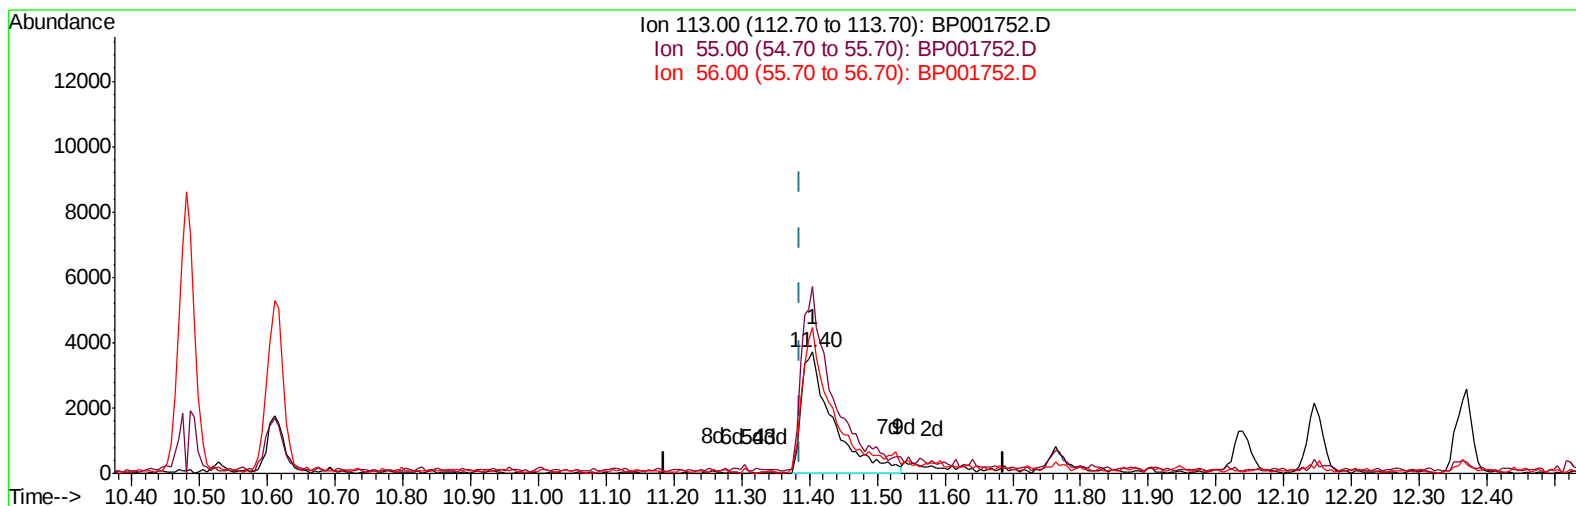

TIC: BP001752.D

(32) Caprolactam

11.405min (+0.018) 1.78ng/ul m

response 12100

Ion	Exp%	Act%
113.00	100	100
55.00	146.60	153.93
56.00	113.40	120.64
0.00	0.00	0.00