
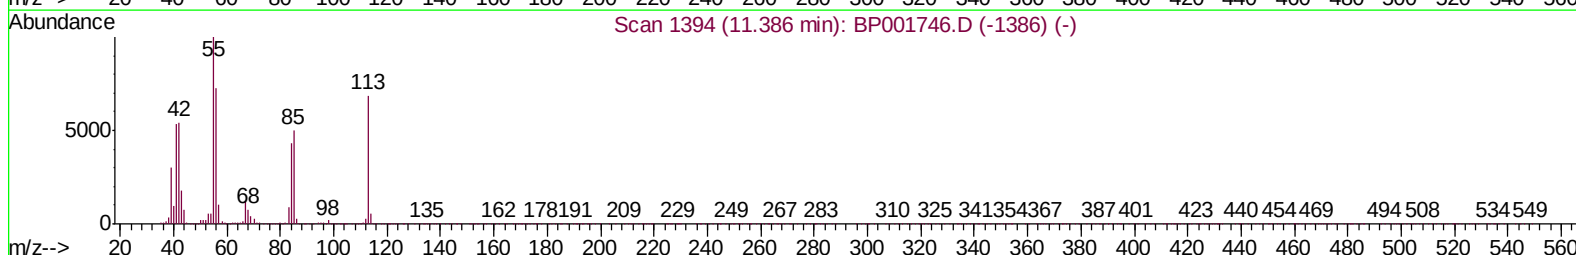
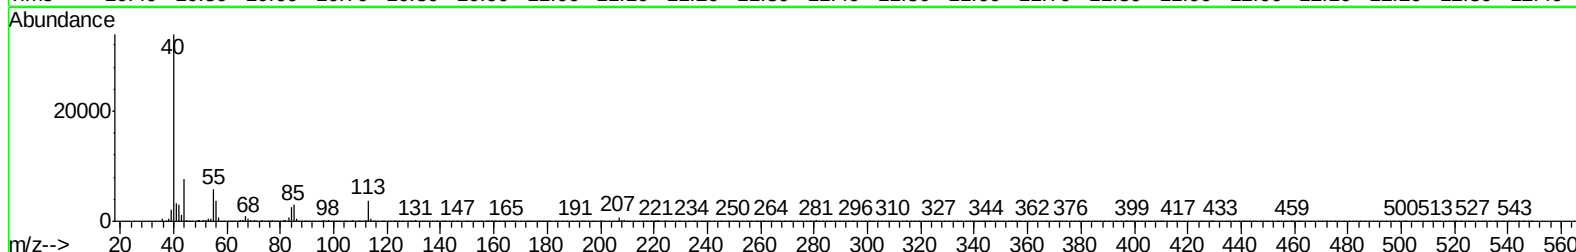


Data File : BP001753.D
Acq On : 14 Feb 2020 19:28
Operator : CG/JU
Sample : K5695-13
Misc : MDL-WATER-06
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 15 04:52:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 15 04:45:21 2020
Response via : Initial Calibration

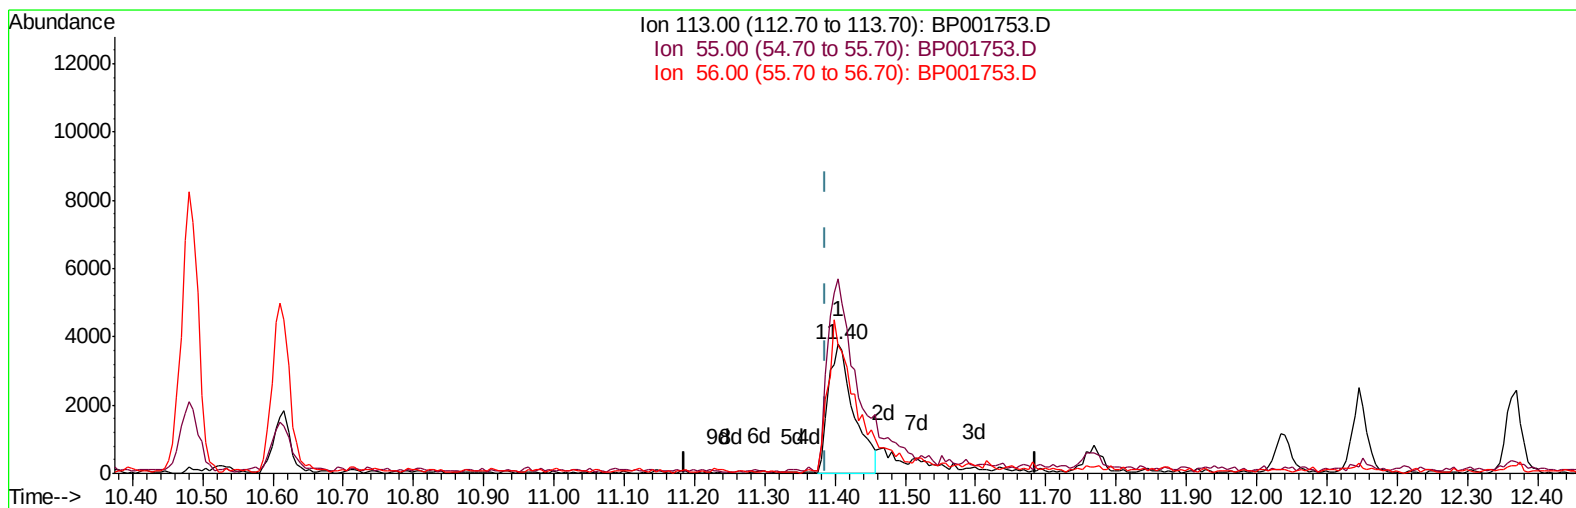

TIC: BP001753.D

(32) Caprolactam

11.404min (+0.018) 1.37ng/ul

response 9517

Ion	Exp%	Act%
113.00	100	100
55.00	146.60	151.18
56.00	113.40	99.05
0.00	0.00	0.00