

Data File : BP001753.D

Acq On : 14 Feb 2020 19:28

Operator : CG/JU

Sample : K5695-13

Misc : MDL-WATER-06

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Feb 15 04:52:19 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Feb 15 04:45:21 2020

Response via : Initial Calibration

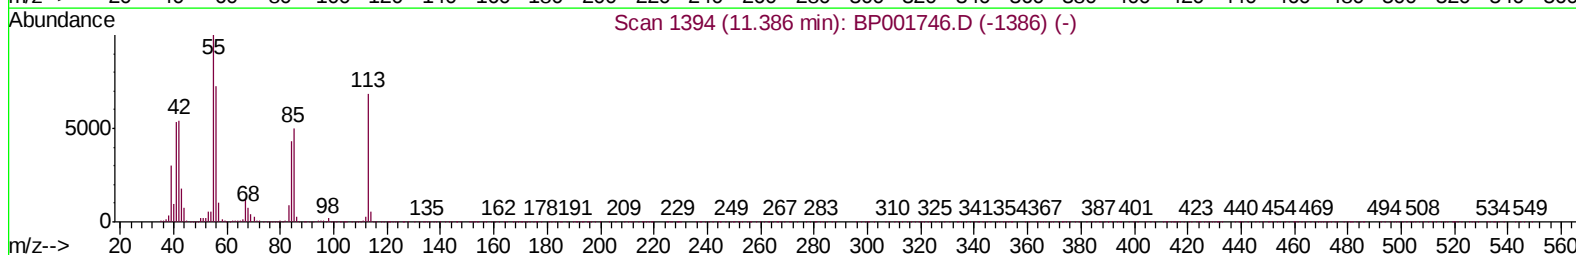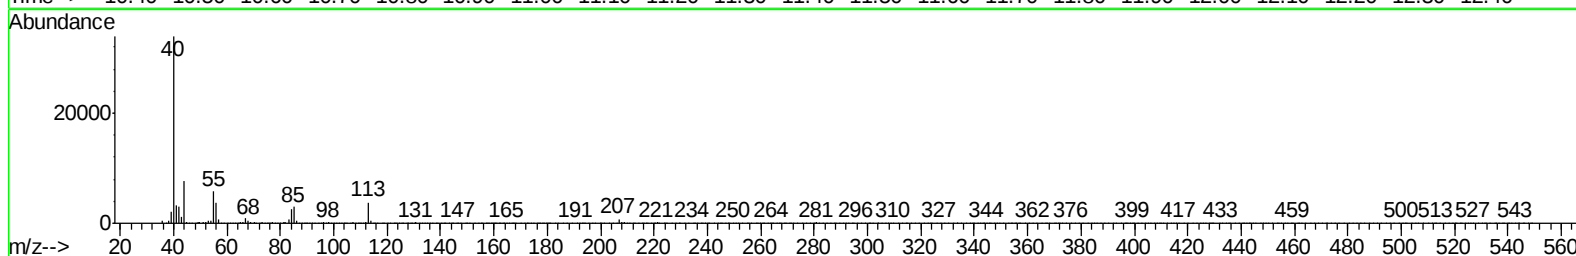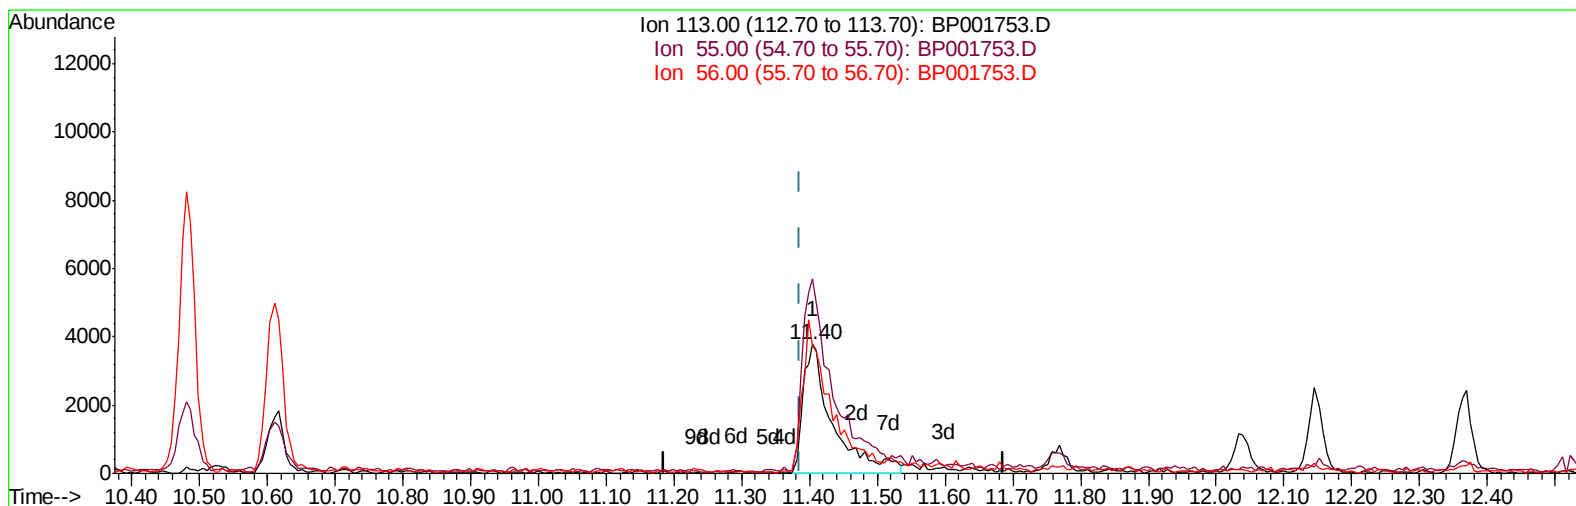

TIC: BP001753.D

(32) Caprolactam

11.404min (+0.018) 1.66ng/ul m

response 11527

Ion	Exp%	Act%
113.00	100	100
55.00	146.60	151.18
56.00	113.40	99.05
0.00	0.00	0.00