
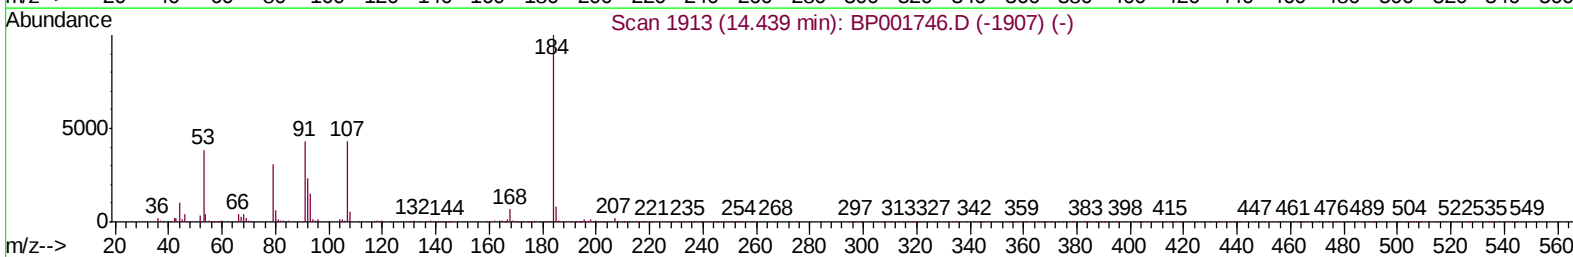
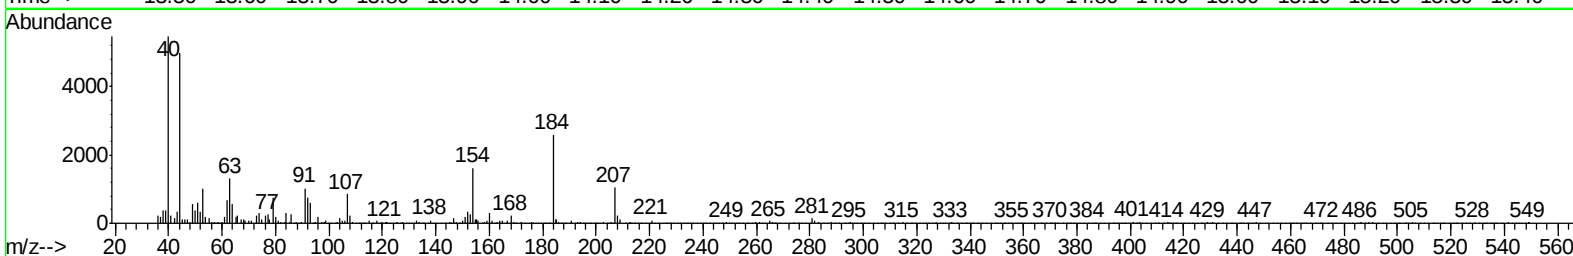


Data File : BP001753.D  
Acq On : 14 Feb 2020 19:28  
Operator : CG/JU  
Sample : K5695-13  
Misc : MDL-WATER-06  
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 15 04:52:19 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 15 04:45:21 2020  
Response via : Initial Calibration

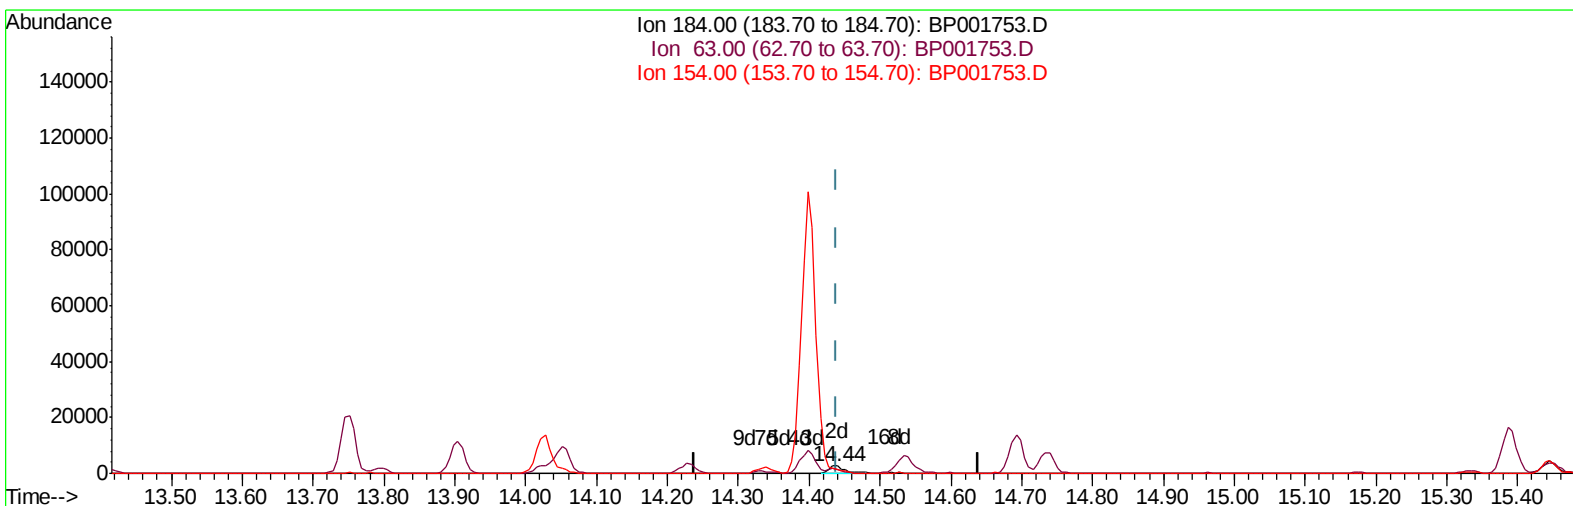

TIC: BP001753.D

(51) 2,4-Dinitrophenol

14.439min (+0.000) 0.90ng/ul m

response 4163

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 63.00  | 63.90 | 49.73# |
| 154.00 | 58.30 | 61.92  |
| 0.00   | 0.00  | 0.00   |