

Data File : BP001753.D

Acq On : 14 Feb 2020 19:28

Operator : CG/JU

Sample : K5695-13

Misc : MDL-WATER-06

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Feb 15 04:52:19 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Feb 15 04:45:21 2020

Response via : Initial Calibration

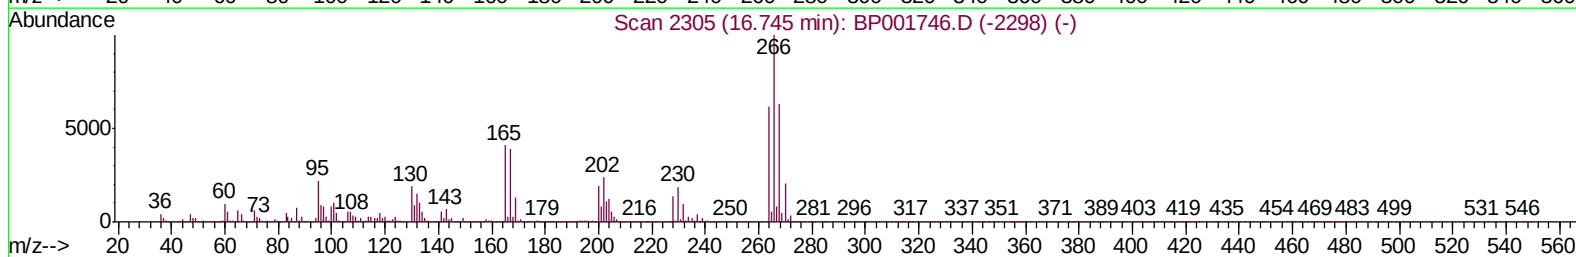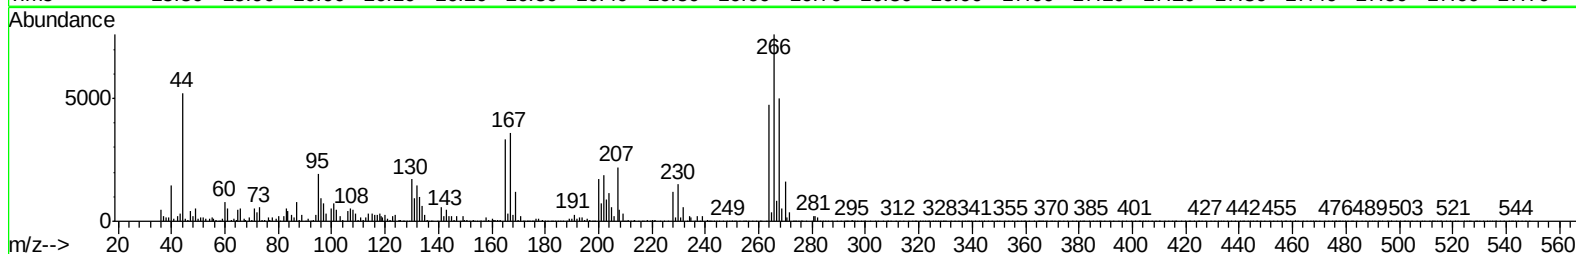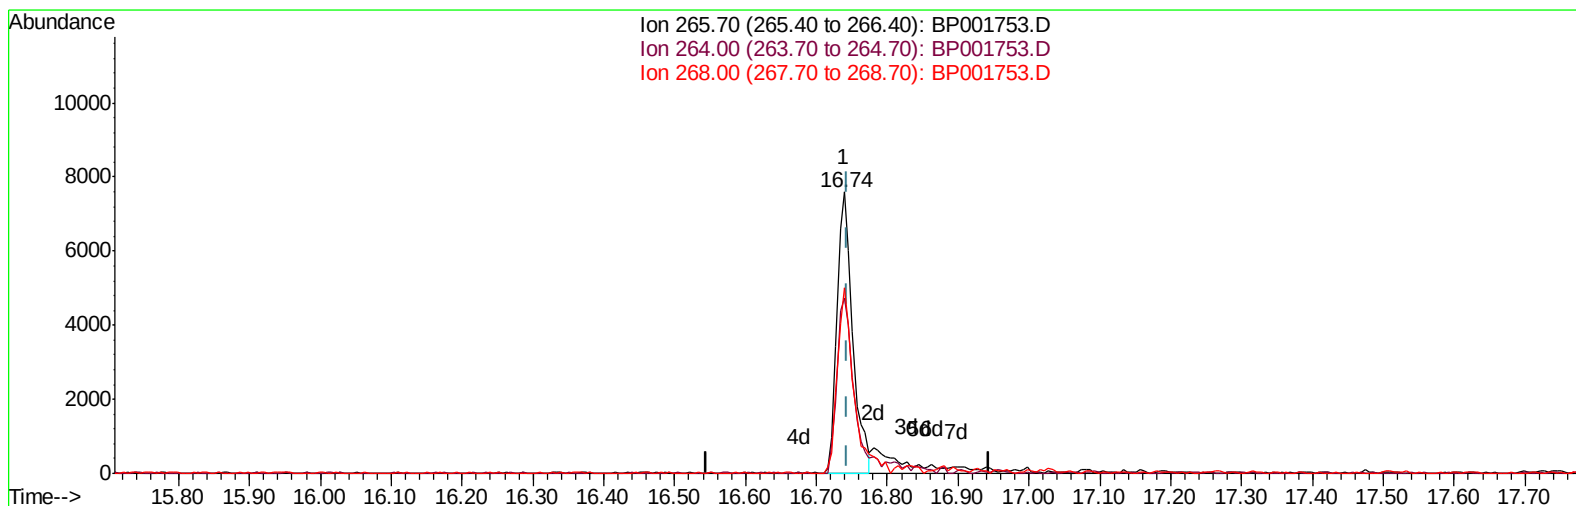

TIC: BP001753.D

(69) Pentachlorophenol (C)

16.739min (-0.006) 0.99ng/ul

response 11744

Ion	Exp%	Act%
265.70	100	100
264.00	63.70	62.39
268.00	63.50	72.53
0.00	0.00	0.00