
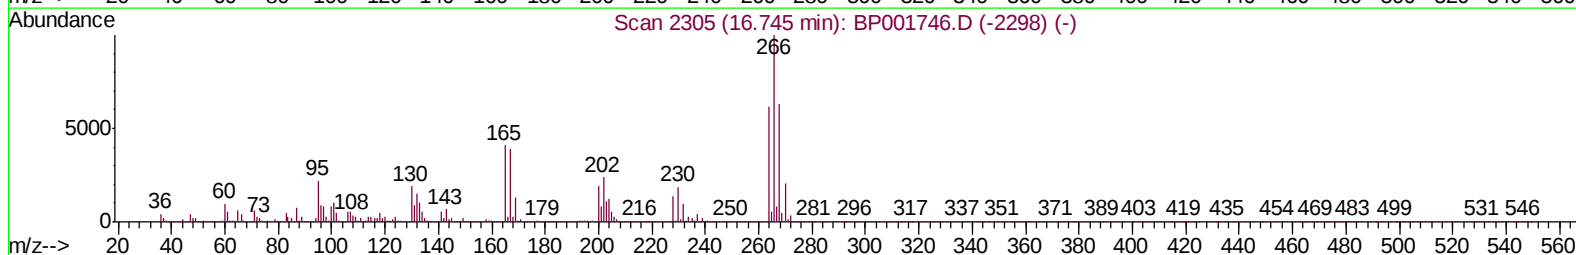
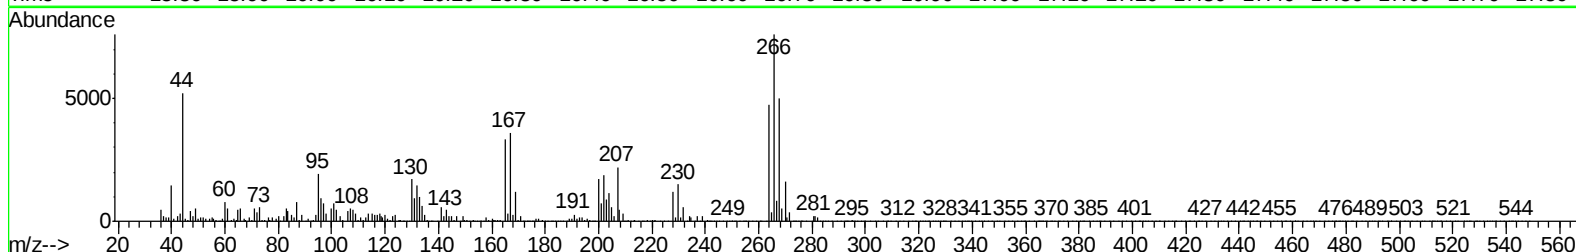


Data File : BP001753.D
Acq On : 14 Feb 2020 19:28
Operator : CG/JU
Sample : K5695-13
Misc : MDL-WATER-06
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 15 04:52:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 15 04:45:21 2020
Response via : Initial Calibration

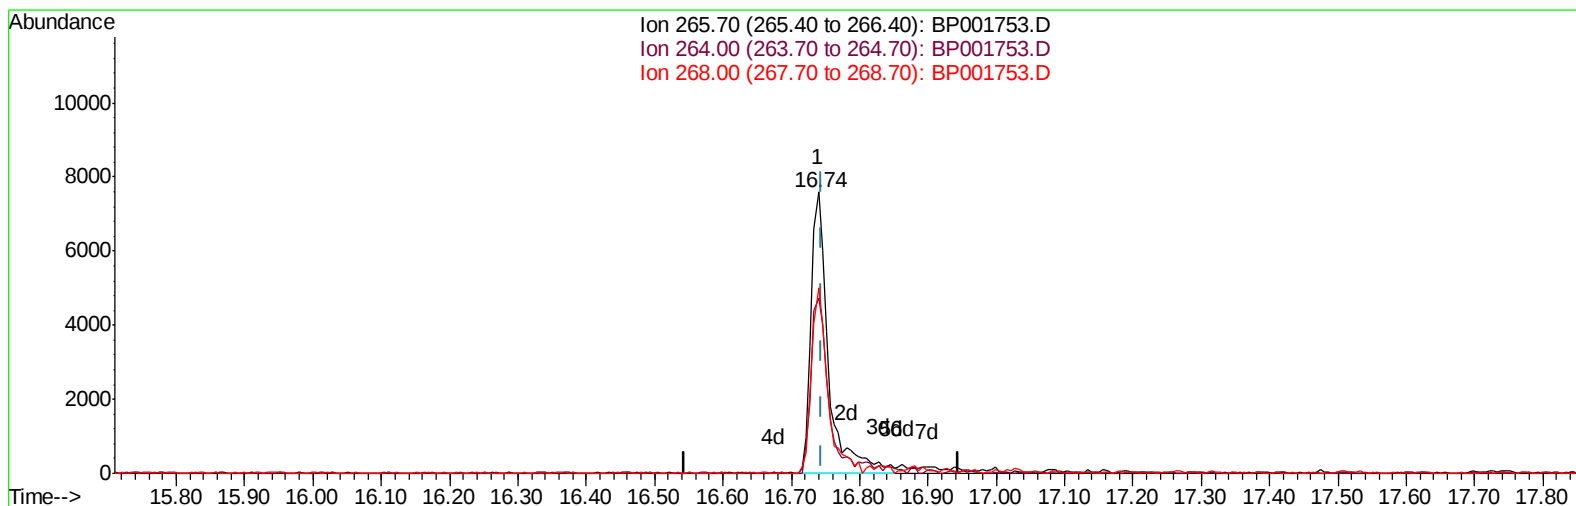

TIC: BP001753.D

(69) Pentachlorophenol (C)

16.739min (-0.006) 1.14ng/ul m

response 13438

Ion	Exp%	Act%
265.70	100	100
264.00	63.70	62.39
268.00	63.50	65.84
0.00	0.00	0.00