

Data File : BP001752.D

Acq On : 14 Feb 2020 18:54

Operator : CG/JU

Sample : K5695-12

Misc : MDL-WATER-05

ALS Vial : 8 Sample Multiplier: 1

Instrument :

BNA\_P

ClientSampleId :

MDL-WATER-05

Manual Integrations  
APPROVED

mohammad  
2/17/2020 3:50:47 PM




Quant Time: Feb 15 04:51:30 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Feb 15 04:45:21 2020

Response via : Initial Calibration

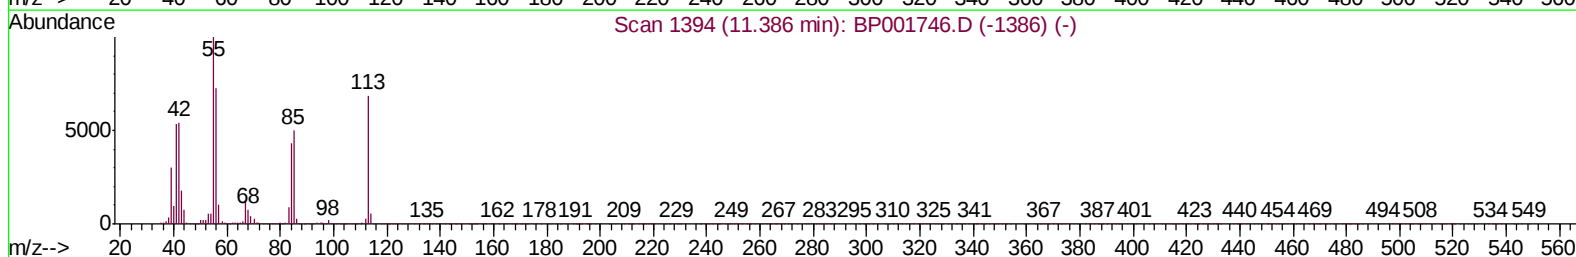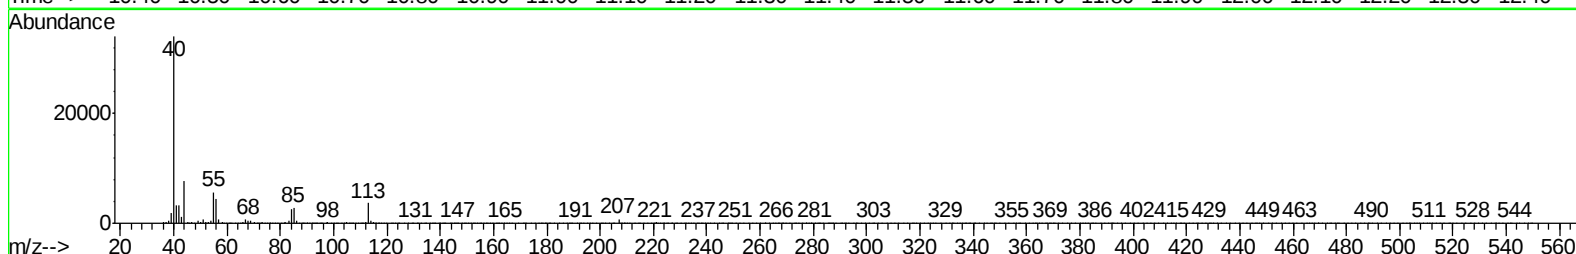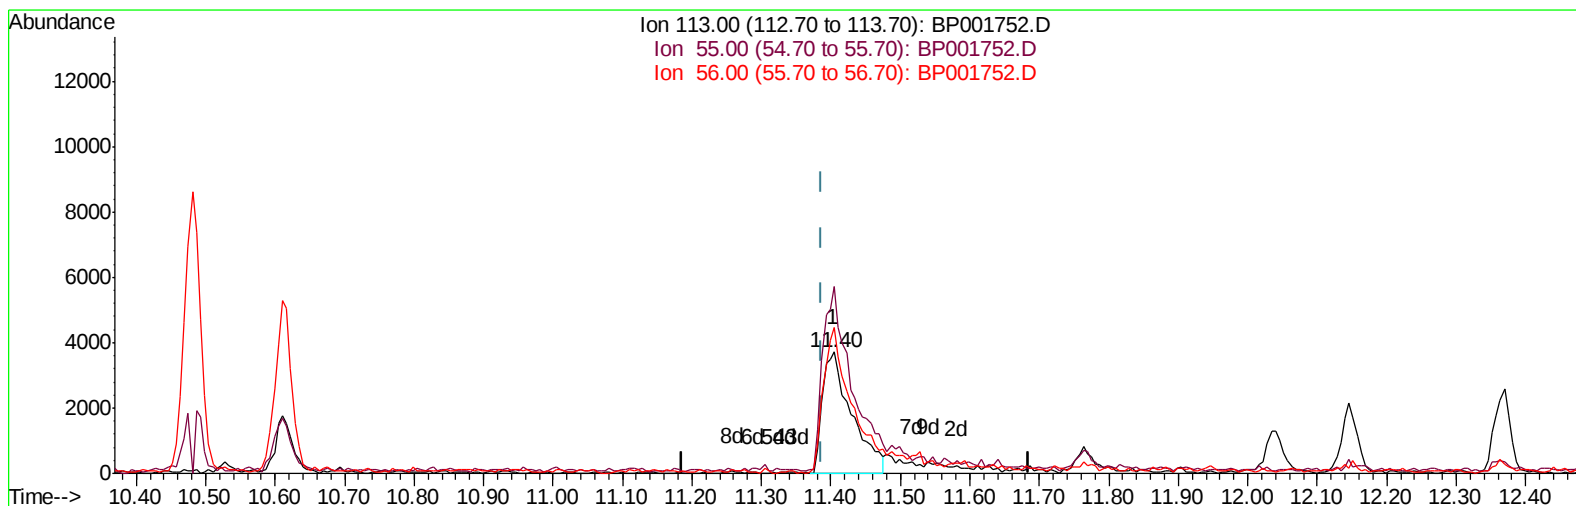

TIC: BP001752.D

(32) Caprolactam

11.405min (+0.018) 1.58ng/ul

response 10777

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 146.60 | 153.93 |
| 56.00  | 113.40 | 120.64 |
| 0.00   | 0.00   | 0.00   |

Data File : BP001752.D

Acq On : 14 Feb 2020 18:54

Operator : CG/JU

Sample : K5695-12

Misc : MDL-WATER-05

ALS Vial : 8 Sample Multiplier: 1

Instrument :

BNA\_P

ClientSampleId :

MDL-WATER-05

Manual Integrations  
APPROVED

mohammad  
2/17/2020 3:50:47 PM




Quant Time: Feb 15 04:51:30 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Feb 15 04:45:21 2020

Response via : Initial Calibration

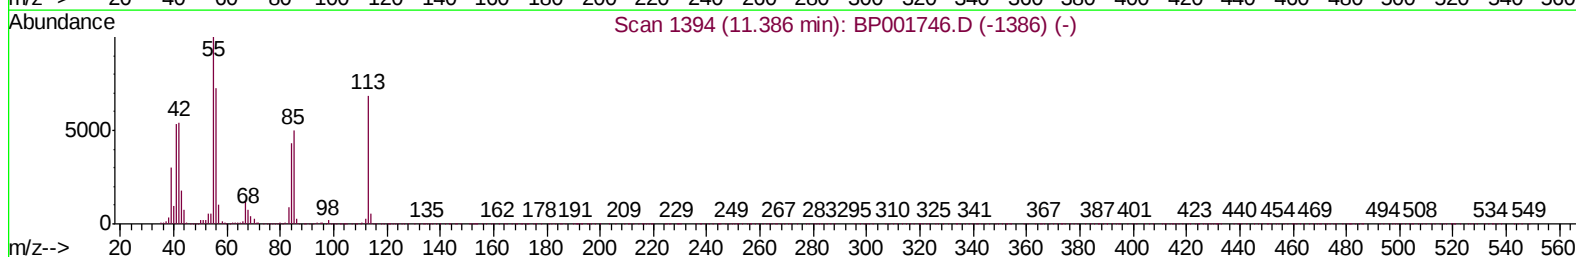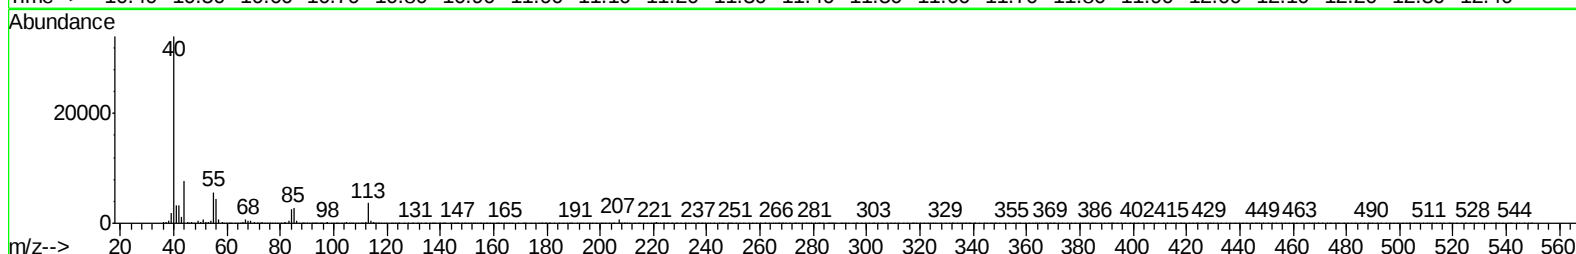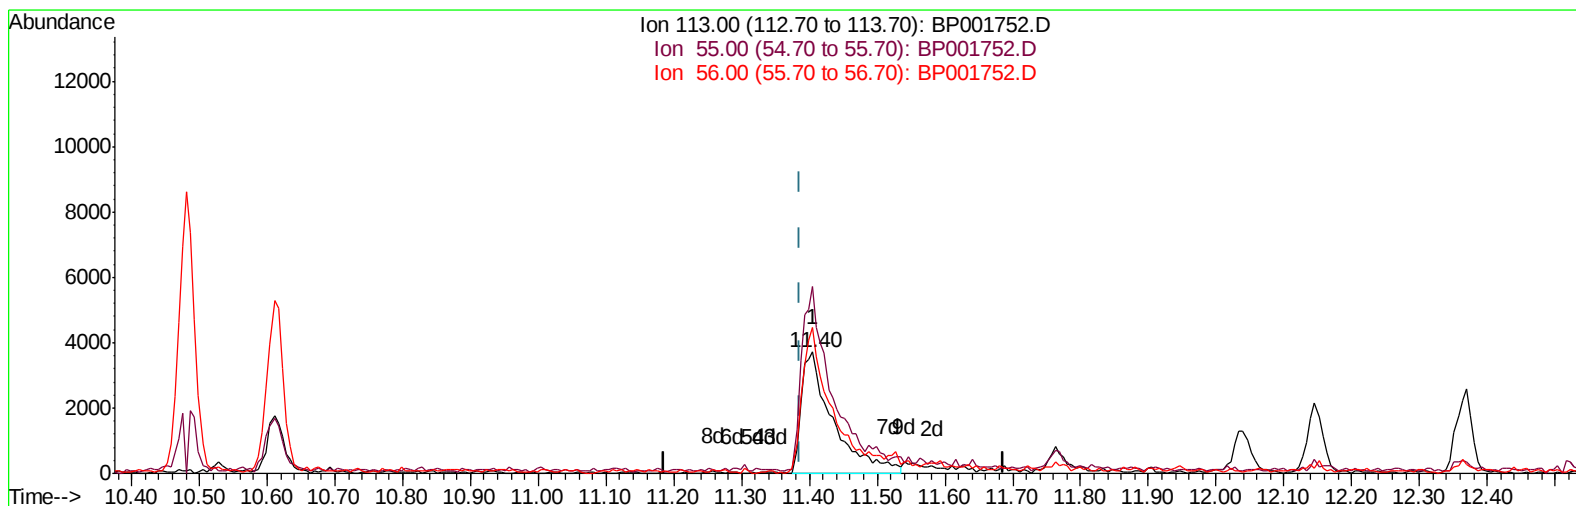

TIC: BP001752.D

(32) Caprolactam

11.405min (+0.018) 1.78ng/ul m

response 12100

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 146.60 | 153.93 |
| 56.00  | 113.40 | 120.64 |
| 0.00   | 0.00   | 0.00   |

Data File : BP001752.D  
Acq On : 14 Feb 2020 18:54  
Operator : CG/JU  
Sample : K5695-12  
Misc : MDL-WATER-05  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
MDL-WATER-05

Manual Integrations  
APPROVED

mohammad  
2/17/2020 3:50:47 PM

Quant Time: Feb 15 05:38:11 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 15 04:45:21 2020  
Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.71  | 152  | 275557   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.48 | 136  | 1272269  | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.33 | 164  | 839925   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.09 | 188  | 1889744  | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.17 | 240  | 2114105  | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.42 | 264  | 2402836  | 20.00 | ng/ul | 0.00     |

#### System Monitoring Compounds

|                                |       |     |         |       |       |      |
|--------------------------------|-------|-----|---------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.24  | 96  | 27621   | 4.79  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 6.88  | 99  | 602624  | 25.83 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.05  | 67  | 418881  | 30.35 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.25  | 132 | 485534  | 28.46 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.41  | 113 | 487739  | 25.49 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 8.85  | 128 | 302013  | 30.86 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 9.57  | 143 | 189724  | 24.71 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 10.10 | 165 | 472280  | 26.23 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 10.61 | 131 | 810083  | 35.72 | ng/ul | 0.00 |
| 44) Dimethylphthalate-d6       | 13.75 | 166 | 1889442 | 31.27 | ng/ul | 0.00 |
| 47) Acenaphthylene-d8          | 14.02 | 160 | 2457010 | 32.20 | ng/ul | 0.00 |
| 52) 4-Nitrophenol-d4           | 14.53 | 143 | 233358  | 20.81 | ng/ul | 0.00 |
| 58) Fluorene-d10               | 15.33 | 176 | 1695398 | 30.96 | ng/ul | 0.00 |
| 63) 4,6-Dinitro-2-methylphenol | 15.45 | 200 | 129423  | 17.00 | ng/ul | 0.00 |
| 71) Anthracene-d10             | 17.19 | 188 | 2699305 | 31.43 | ng/ul | 0.00 |
| 79) Pyrene-d10                 | 19.43 | 212 | 3096647 | 30.89 | ng/ul | 0.00 |
| 90) Benzo(a)pyrene-d12         | 23.27 | 264 | 3498672 | 30.76 | ng/ul | 0.00 |

#### Target Compounds

|                                |       |     |        |              | Qvalue |
|--------------------------------|-------|-----|--------|--------------|--------|
| 2) 1,4-Dioxane                 | 3.28  | 88  | 4117   | 0.649 ng/uL# | 86     |
| 4) Benzaldehyde                | 6.86  | 77  | 54734  | 3.603 ng/ul  | 99     |
| 6) Phenol                      | 6.91  | 94  | 62782  | 2.513 ng/ul  | 97     |
| 8) Bis(2-Chloroethyl)ether     | 7.14  | 93  | 60621  | 3.063 ng/ul  | 97     |
| 10) 2-Chlorophenol             | 7.28  | 128 | 49006  | 2.697 ng/ul  | 97     |
| 11) 2-Methylphenol             | 8.15  | 108 | 42846  | 2.220 ng/ul  | 96     |
| 12) 2,2'-oxybis(1-Chloropropan | 8.24  | 45  | 79251  | 3.122 ng/ul  | 98     |
| 14) Acetophenone               | 8.52  | 105 | 95633  | 3.027 ng/ul  | 98     |
| 15) N-Nitroso-di-n-propylamine | 8.51  | 70  | 43393  | 2.763 ng/ul  | 97     |
| 16) 4-Methylphenol             | 8.47  | 108 | 52249  | 2.455 ng/ul  | 100    |
| 17) Hexachloroethane           | 8.79  | 117 | 23624  | 2.986 ng/ul  | 100    |
| 20) Nitrobenzene               | 8.89  | 77  | 72287  | 3.038 ng/ul  | 99     |
| 21) Isophorone                 | 9.42  | 82  | 118987 | 2.635 ng/ul  | 98     |
| 23) 2-Nitrophenol              | 9.60  | 139 | 20842  | 2.271 ng/ul  | 96     |
| 24) 2,4-Dimethylphenol         | 9.67  | 107 | 52278  | 2.456 ng/ul  | 99     |
| 25) Bis(2-Chloroethoxy)methane | 9.90  | 93  | 82806  | 2.923 ng/ul  | 99     |
| 27) 2,4-Dichlorophenol         | 10.13 | 162 | 49118  | 2.651 ng/ul# | 88     |
| 28) Naphthalene                | 10.53 | 128 | 208785 | 3.038 ng/ul  | 99     |
| 30) 4-Chloroaniline            | 10.63 | 127 | 74606  | 3.233 ng/ul  | 99     |
| 31) Hexachlorobutadiene        | 10.83 | 225 | 39478  | 3.068 ng/ul  | 97     |
| 32) Caprolactam                | 11.40 | 113 | 12100m | 1.776 ng/ul  |        |
| 33) 4-Chloro-3-methylphenol    | 11.76 | 107 | 37514  | 1.966 ng/ul  | 99     |
| 34) 2-Methylnaphthalene        | 12.15 | 142 | 144311 | 2.922 ng/ul  | 99     |

Data File : BP001752.D  
Acq On : 14 Feb 2020 18:54  
Operator : CG/JU  
Sample : K5695-12  
Misc : MDL-WATER-05  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleID :  
MDL-WATER-05

Manual Integrations  
APPROVED

mohammad  
2/17/2020 3:50:47 PM

Quant Time: Feb 15 05:38:11 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 15 04:45:21 2020  
Response via : Initial Calibration

| Internal Standards             | R.T.  | QIon | Response | Conc  | Units  | Dev(Min) |
|--------------------------------|-------|------|----------|-------|--------|----------|
| 35) 1-Methylnaphthalene        | 12.37 | 142  | 153943   | 3.139 | ng/ul  | 98       |
| 37) 1,2,4,5-Tetrachlorobenzene | 12.52 | 216  | 77508    | 2.949 | ng/ul  | 99       |
| 38) Hexachlorocyclopentadiene  | 12.51 | 237  | 34865    | 2.227 | ng/ul  | 98       |
| 39) 2,4,6-Trichlorophenol      | 12.76 | 196  | 22849    | 1.709 | ng/ul  | 96       |
| 40) 2,4,5-Trichlorophenol      | 12.83 | 196  | 22006    | 1.460 | ng/ul  | 95       |
| 41) 1,1'-Biphenyl              | 13.17 | 154  | 195245   | 3.032 | ng/ul  | 99       |
| 42) 2-Chloronaphthalene        | 13.20 | 162  | 154960   | 3.041 | ng/ul  | 100      |
| 43) 2-Nitroaniline             | 13.40 | 65   | 25145    | 1.994 | ng/ul  | 91       |
| 45) Dimethylphthalate          | 13.80 | 163  | 187247   | 2.934 | ng/ul  | 99       |
| 46) 2,6-Dinitrotoluene         | 13.90 | 165  | 27323    | 2.211 | ng/ul  | 89       |
| 48) Acenaphthylene             | 14.05 | 152  | 254474   | 3.091 | ng/ul  | 99       |
| 49) 3-Nitroaniline             | 14.23 | 138  | 24883    | 2.077 | ng/ul# | 91       |
| 50) Acenaphthene               | 14.40 | 153  | 167241   | 3.028 | ng/ul  | 99       |
| 51) 2,4-Dinitrophenol          | 14.45 | 184  | 3896     | 0.871 | ng/ul  | 92       |
| 53) 4-Nitrophenol              | 14.54 | 109  | 19041    | 2.176 | ng/ul  | 85       |
| 54) Dibenzofuran               | 14.73 | 168  | 237522   | 3.051 | ng/ul  | 100      |
| 55) 2,4-Dinitrotoluene         | 14.69 | 165  | 42284    | 2.324 | ng/ul# | 90       |
| 56) 2,3,4,6-Tetrachlorophenol  | 14.96 | 232  | 22022    | 1.718 | ng/ul  | 97       |
| 57) Diethylphthalate           | 15.17 | 149  | 158400   | 2.548 | ng/ul  | 98       |
| 59) Fluorene                   | 15.39 | 166  | 194950   | 3.013 | ng/ul  | 99       |
| 60) 4-Chlorophenyl-phenylether | 15.39 | 204  | 98857    | 3.021 | ng/ul  | 99       |
| 61) 4-Nitroaniline             | 15.39 | 138  | 30307    | 2.085 | ng/ul  | 98       |
| 64) 4,6-Dinitro-2-methylphenol | 15.46 | 198  | 13472    | 1.567 | ng/ul# | 51       |
| 65) N-Nitrosodiphenylamine     | 15.60 | 169  | 145275   | 2.717 | ng/ul  | 99       |
| 66) 4-Bromophenyl-phenylether  | 16.29 | 248  | 54515    | 2.711 | ng/ul  | 98       |
| 67) Hexachlorobenzene          | 16.40 | 284  | 69661    | 2.930 | ng/ul  | 98       |
| 68) Atrazine                   | 16.56 | 200  | 37250    | 1.863 | ng/ul  | 95       |
| 69) Pentachlorophenol          | 16.74 | 266  | 13899    | 1.206 | ng/ul  | 94       |
| 70) Phenanthrene               | 17.13 | 178  | 318637   | 2.994 | ng/ul  | 99       |
| 72) Anthracene                 | 17.22 | 178  | 325299   | 3.043 | ng/ul  | 99       |
| 73) 1,2,3,4-Tetrachlorobenzene | 13.13 | 216  | 89331    | 3.143 | ng/uL  | 97       |
| 74) Pentachlorobenzene         | 14.66 | 250  | 82355    | 2.848 | ng/uL  | 99       |
| 75) Carbazole                  | 17.49 | 167  | 231167   | 2.559 | ng/ul  | 99       |
| 76) Di-n-butylphthalate        | 18.07 | 149  | 171769   | 1.805 | ng/ul  | 99       |
| 77) Fluoranthene               | 19.10 | 202  | 329938   | 2.813 | ng/ul  | 98       |
| 80) Pyrene                     | 19.45 | 202  | 412759   | 3.031 | ng/ul  | 99       |
| 81) Butylbenzylphthalate       | 20.35 | 149  | 45003    | 1.114 | ng/ul  | 95       |
| 82) 3,3'-Dichlorobenzidine     | 21.10 | 252  | 42741    | 1.036 | ng/ul  | 100      |
| 83) Benzo(a)anthracene         | 21.16 | 228  | 371579   | 2.684 | ng/ul  | 98       |
| 84) Bis(2-ethylhexyl)phthalate | 21.12 | 149  | 86417    | 1.310 | ng/ul  | 99       |
| 85) Chrysene                   | 21.21 | 228  | 390264   | 2.917 | ng/ul  | 99       |
| 87) Di-n-octyl phthalate       | 21.99 | 149  | 131691   | 1.227 | ng/ul  | 100      |
| 88) Benzo(b)fluoranthene       | 22.74 | 252  | 339229   | 2.439 | ng/ul  | 99       |
| 89) Benzo(k)fluoranthene       | 22.79 | 252  | 396909   | 2.825 | ng/ul  | 100      |
| 91) Benzo(a)pyrene             | 23.32 | 252  | 350266   | 2.654 | ng/ul  | 100      |
| 92) Indeno(1,2,3-cd)pyrene     | 25.67 | 276  | 425442   | 2.461 | ng/ul  | 99       |
| 93) Dibenzo(a,h)anthracene     | 25.69 | 278  | 355903   | 2.468 | ng/ul  | 99       |
| 94) Benzo(g,h,i)perylene       | 26.36 | 276  | 360185   | 2.447 | ng/ul  | 96       |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP021420\  
Quantitation Report (QT Reviewed)

Data File : BP001752.D  
Acq On : 14 Feb 2020 18:54  
Operator : CG/JU  
Sample : K5695-12  
Misc : MDL-WATER-05  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
MDL-WATER-05

Manual Integrations  
APPROVED

mohammad  
2/17/2020 3:50:47 PM

Quant Time: Feb 15 05:38:11 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 15 04:45:21 2020  
Response via : Initial Calibration

| Internal Standards                                                         | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------------------------------------------------------|------|------|----------|------|-------|----------|
| -----                                                                      |      |      |          |      |       |          |
| (#) = qualifier out of range (m) = manual integration (+) = signals summed |      |      |          |      |       |          |

Data File : BP001752.D  
Acq On : 14 Feb 2020 18:54  
Operator : CG/JU  
Sample : K5695-12  
Misc : MDL-WATER-05  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
MDL-WATER-05

Manual Integrations  
APPROVED

mohammad  
2/17/2020 3:50:47 PM

Quant Time: Feb 15 05:38:11 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP021320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 15 04:45:21 2020  
Response via : Initial Calibration

