

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
 Data File : BP013859.D
 Acq On : 21 Feb 2023 10:03
 Operator : CG/JU
 Sample : PB150955BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK955

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.452	42	45	55	rVB	39910	56219	1.20%	0.132%
2	3.887	115	119	135	rBV	494224	772781	16.49%	1.815%
3	4.222	172	176	180	rVB	11807	17581	0.38%	0.041%
4	7.252	684	691	704	rBV	661277	1058497	22.59%	2.486%
5	7.422	714	720	732	rVB	530480	831181	17.74%	1.952%
6	7.628	748	755	770	rBV	667445	1108456	23.66%	2.603%
7	8.105	829	836	847	rBV	477715	765031	16.33%	1.797%
8	8.810	948	956	970	rBV	841496	1378018	29.41%	3.237%
9	9.275	1028	1035	1048	rBV	596033	1010422	21.56%	2.373%
10	10.005	1150	1159	1172	rBV	532189	896874	19.14%	2.107%
11	10.546	1243	1251	1267	rBV	796874	1378487	29.42%	3.238%
12	10.934	1309	1317	1325	rBV	613954	1039237	22.18%	2.441%
13	11.069	1330	1340	1357	rBV	760256	1371819	29.28%	3.222%
14	12.510	1580	1585	1591	rBV2	13099	24135	0.52%	0.057%
15	13.628	1770	1775	1781	rBV2	15664	22376	0.48%	0.053%
16	14.145	1853	1863	1874	rBV	1765826	2418522	51.62%	5.680%
17	14.440	1905	1913	1923	rBV	1764288	2638163	56.30%	6.196%
18	14.745	1957	1965	1973	rBV	1049003	1538481	32.83%	3.613%
19	14.804	1973	1975	1980	rVB6	3238	4733	0.10%	0.011%
20	14.928	1990	1996	2013	rBV	660963	1063083	22.69%	2.497%
21	15.140	2030	2032	2041	rVB9	4142	8084	0.17%	0.019%
22	15.734	2120	2133	2140	rBV	2268483	3398223	72.53%	7.981%
23	15.845	2146	2152	2167	rBV	760194	1125313	24.02%	2.643%
24	15.975	2170	2174	2181	rVB4	12654	22344	0.48%	0.052%
25	17.175	2374	2378	2381	rBV6	4725	7730	0.16%	0.018%
26	17.292	2394	2398	2405	rVB9	3866	7139	0.15%	0.017%
27	17.498	2426	2433	2441	rBV	1402010	1960012	41.83%	4.604%
28	17.598	2443	2450	2461	rVV2	2799492	3901036	83.26%	9.162%
29	18.369	2576	2581	2583	rBV6	9574	15620	0.33%	0.037%
30	19.392	2751	2755	2759	rBV2	38413	55642	1.19%	0.131%
31	19.463	2763	2767	2771	rBV	36515	53655	1.15%	0.126%
32	19.816	2821	2827	2843	rBV	3380068	4685540	100.00%	11.005%
33	21.574	3121	3126	3135	rBV	1613857	2083191	44.46%	4.893%
34	23.963	3525	3532	3542	rVB2	1955792	4007136	85.52%	9.412%
35	24.127	3554	3560	3569	rVB2	900399	1851703	39.52%	4.349%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013859.D
Acq On : 21 Feb 2023 10:03
Operator : CG/JU
Sample : PB150955BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK955

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42576464

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013859.D
Acq On : 21 Feb 2023 10:03
Operator : CG/JU
Sample : PB150955BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK955

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

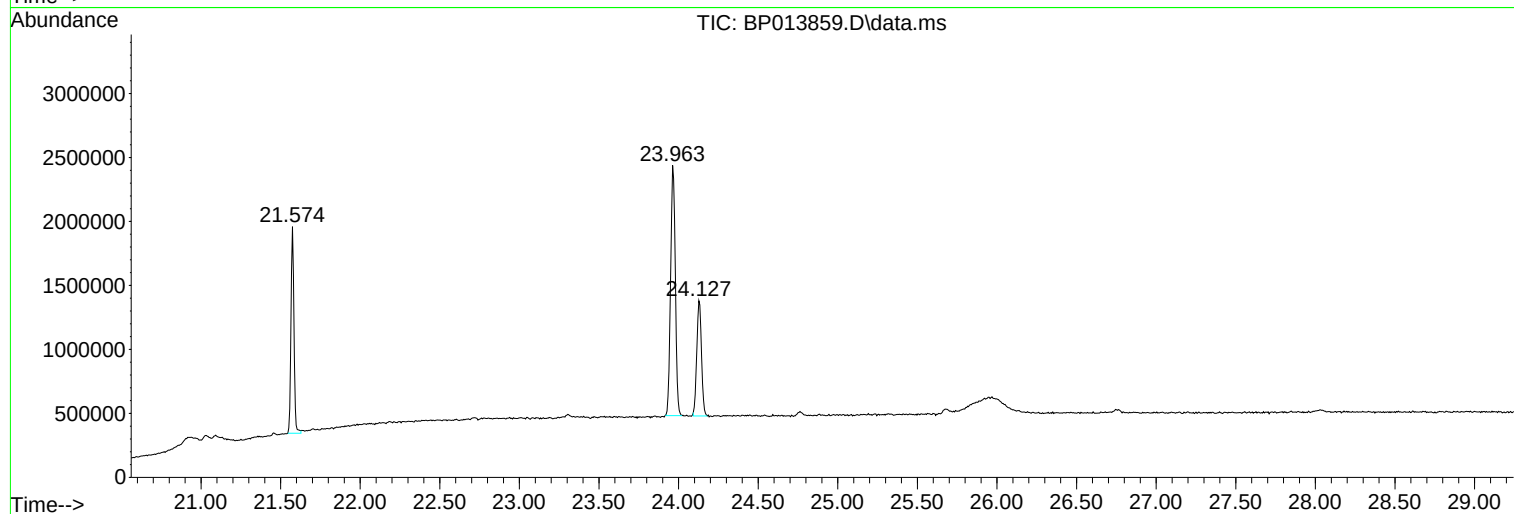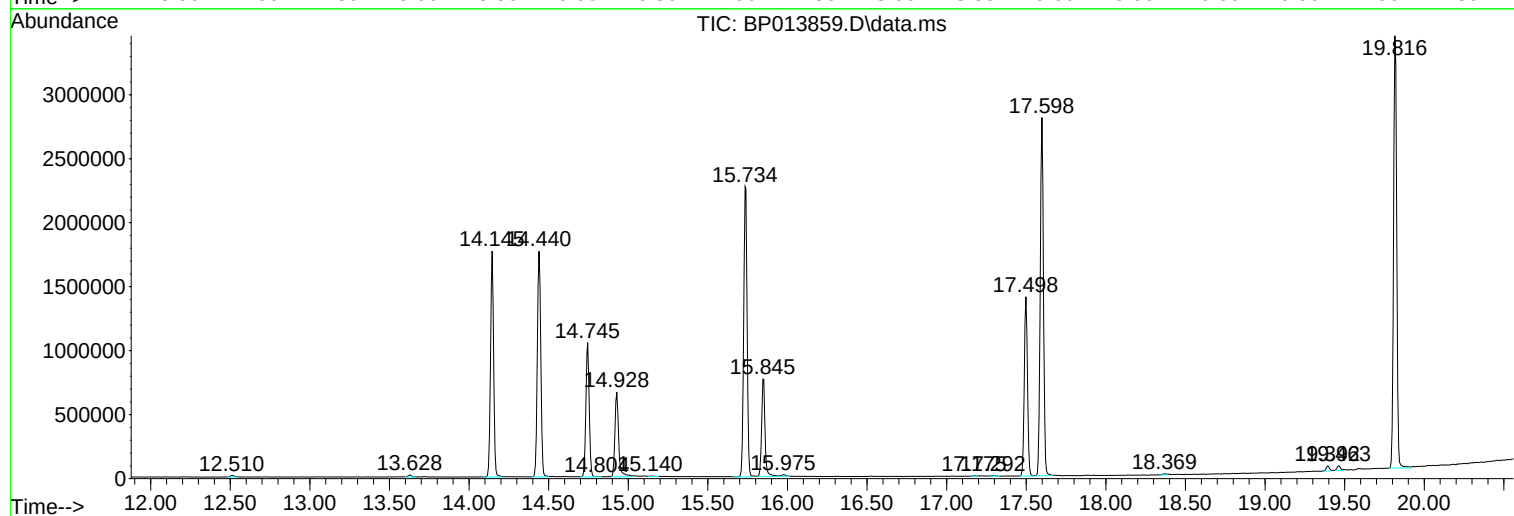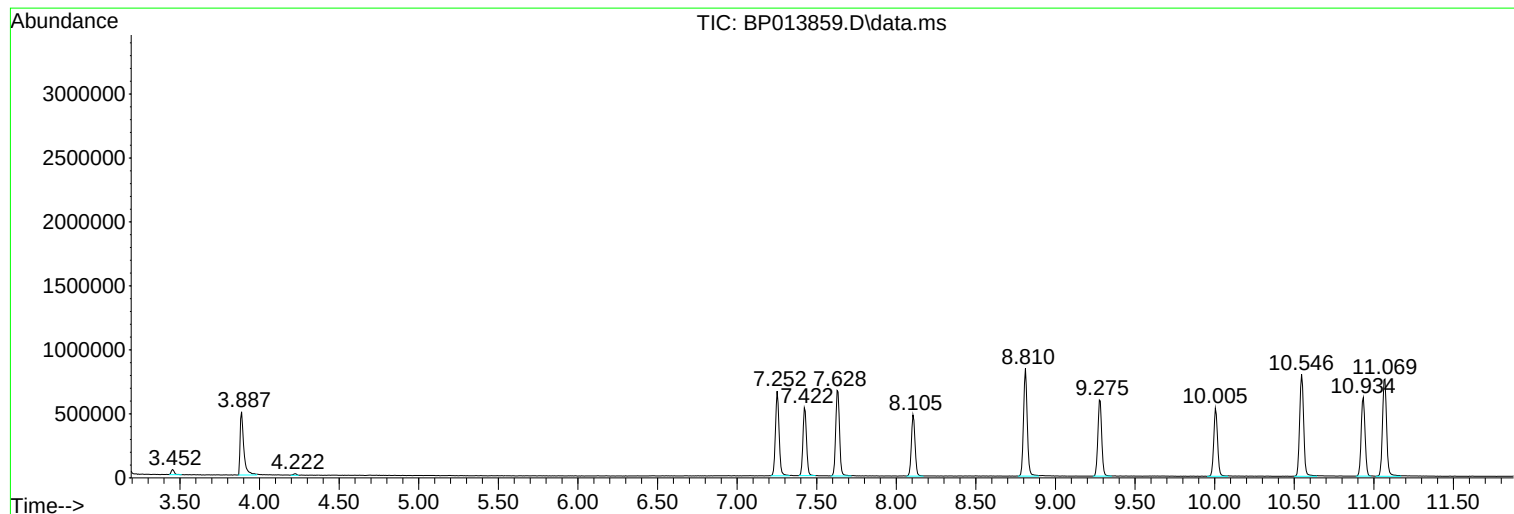

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013859.D
Acq On : 21 Feb 2023 10:03
Operator : CG/JU
Sample : PB150955BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK955

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013859.D
Acq On : 21 Feb 2023 10:03
Operator : CG/JU
Sample : PB150955BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK955

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc