

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
 Data File : BP013864.D
 Acq On : 21 Feb 2023 13:23
 Operator : CG/JU
 Sample : PB150959BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	41	46	56	rVB	33490	54626	1.19%	0.117%
2	3.887	116	119	138	rBV	399901	647815	14.05%	1.386%
3	4.228	172	177	183	rVB	11938	20294	0.44%	0.043%
4	7.257	684	692	705	rBV	595493	946640	20.54%	2.025%
5	7.428	715	721	733	rVB	460367	739445	16.04%	1.582%
6	7.634	749	756	774	rVB	602604	984356	21.35%	2.105%
7	8.110	829	837	851	rBV	649797	1030052	22.35%	2.203%
8	8.816	949	957	973	rBV	752144	1248652	27.09%	2.671%
9	9.281	1028	1036	1048	rBV	572005	969267	21.03%	2.073%
10	10.010	1152	1160	1171	rBV	526110	865246	18.77%	1.851%
11	10.551	1244	1252	1271	rBV	773410	1327085	28.79%	2.838%
12	10.940	1310	1318	1327	rBV	907355	1532342	33.24%	3.277%
13	11.069	1332	1340	1354	rBV	735459	1338505	29.04%	2.863%
14	12.516	1580	1586	1593	rBV2	13583	25821	0.56%	0.055%
15	13.634	1770	1776	1781	rVB5	11829	19186	0.42%	0.041%
16	14.151	1855	1864	1877	rBV	1629096	2285052	49.57%	4.887%
17	14.445	1905	1914	1932	rBV	1730648	2518096	54.63%	5.386%
18	14.751	1958	1966	1976	rBV	1550873	2324044	50.42%	4.971%
19	14.934	1990	1997	2010	rBV	661371	1042459	22.62%	2.230%
20	15.157	2031	2035	2040	rVB8	3752	7072	0.15%	0.015%
21	15.739	2127	2134	2142	rBV	2359738	3278085	71.12%	7.011%
22	15.851	2147	2153	2167	rBV	752535	1090736	23.66%	2.333%
23	15.981	2172	2175	2184	rVB3	12400	19432	0.42%	0.042%
24	17.180	2374	2379	2383	rBV8	4839	8533	0.19%	0.018%
25	17.292	2395	2398	2402	rVB4	3661	5221	0.11%	0.011%
26	17.504	2427	2434	2444	rBV	2058814	2960290	64.22%	6.332%
27	17.604	2444	2451	2462	rVV	2620910	3759724	81.56%	8.041%
28	18.363	2576	2580	2586	rBV8	13278	25423	0.55%	0.054%
29	19.398	2752	2756	2762	rBV	40820	60215	1.31%	0.129%
30	19.469	2764	2768	2773	rVV	36371	50958	1.11%	0.109%
31	19.822	2822	2828	2839	rBV	3440246	4609518	100.00%	9.859%
32	21.580	3122	3127	3137	rBV	2417753	3254053	70.59%	6.960%
33	23.974	3526	3534	3547	rVB2	2148242	4471230	97.00%	9.563%
34	24.139	3555	3562	3572	rVB2	1554755	3235097	70.18%	6.919%

Sum of corrected areas: 46754570

Instrument :

BNA_P

ClientSampleId :




SBLK959

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013864.D
Acq On : 21 Feb 2023 13:23
Operator : CG/JU
Sample : PB150959BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

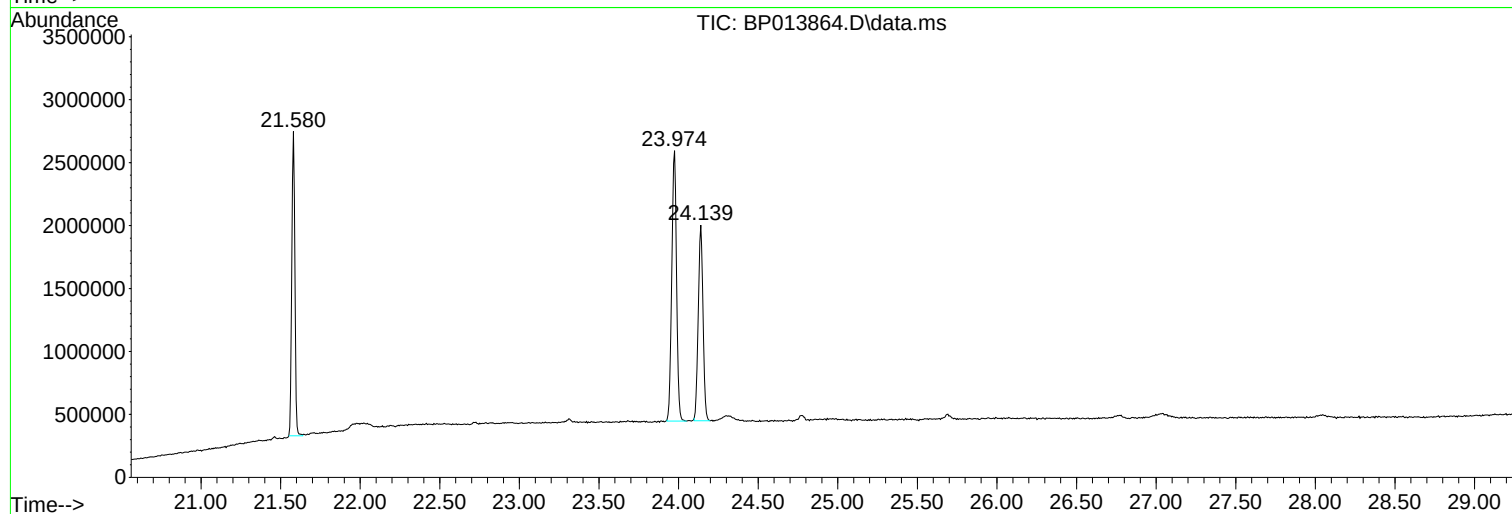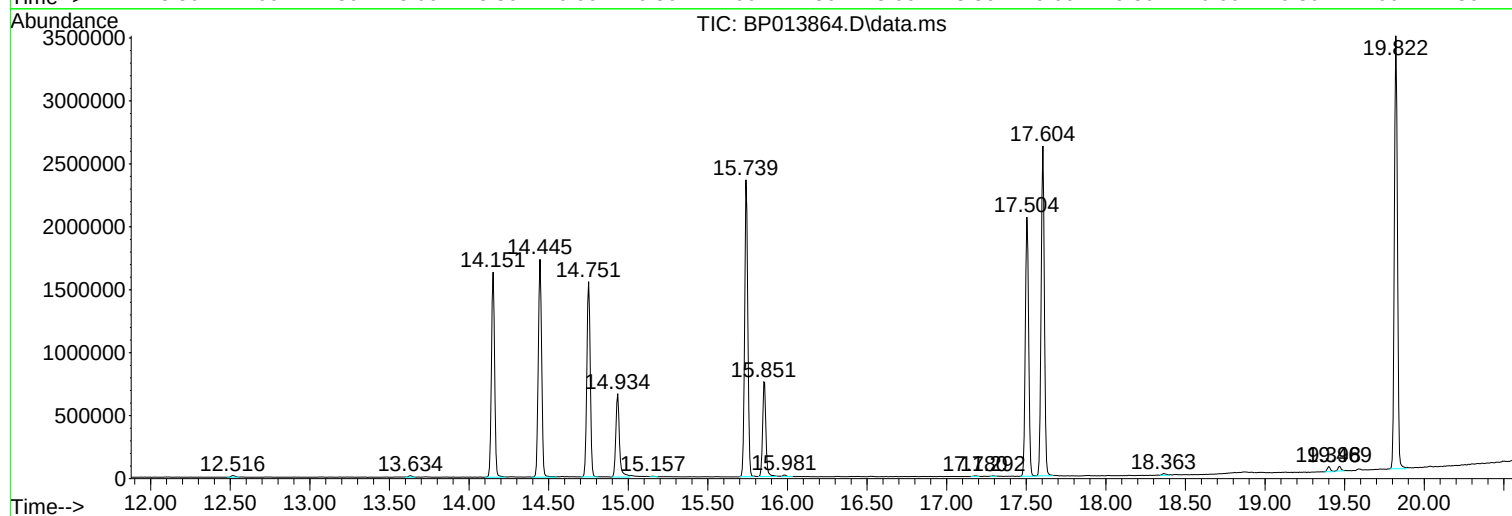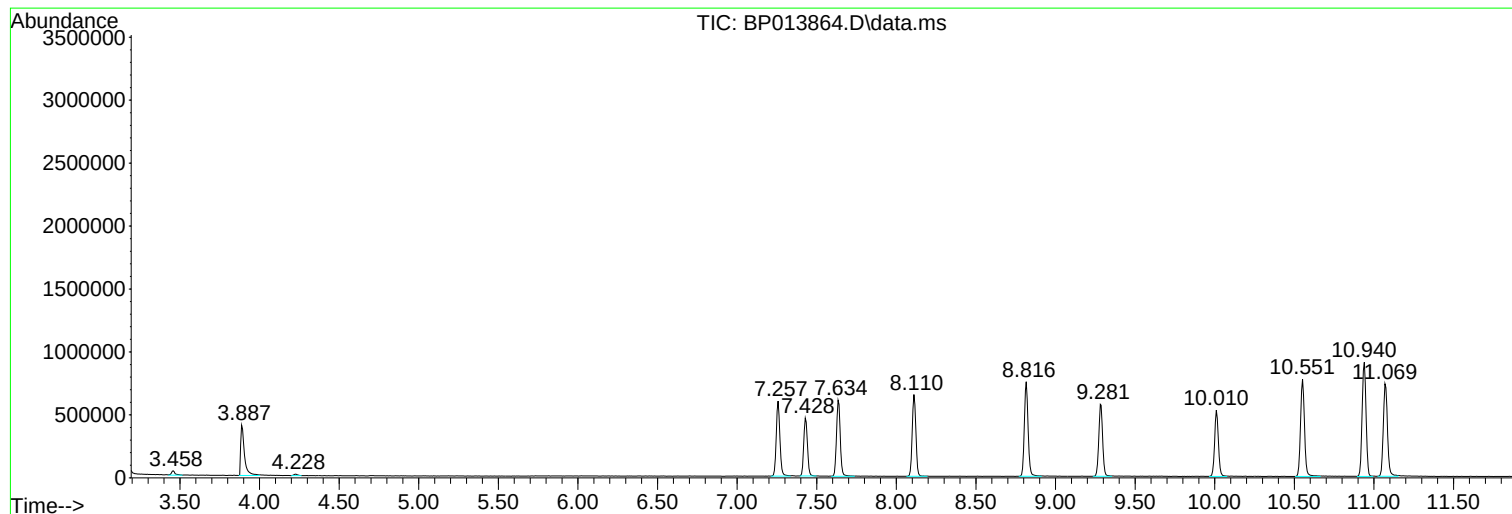

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013864.D
Acq On : 21 Feb 2023 13:23
Operator : CG/JU
Sample : PB150959BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013864.D
Acq On : 21 Feb 2023 13:23
Operator : CG/JU
Sample : PB150959BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc