

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
 Data File : BP013865.D
 Acq On : 21 Feb 2023 13:57
 Operator : CG/JU
 Sample : PB150960BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK960

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.452	41	45	51	rBV	40792	52810	1.18%	0.123%
2	3.887	115	119	137	rBV	486193	762014	17.00%	1.776%
3	4.222	172	176	180	rBV	11042	15112	0.34%	0.035%
4	4.693	252	256	259	rBV6	4010	7409	0.17%	0.017%
5	7.252	679	691	705	rBV	571924	952979	21.26%	2.221%
6	7.422	713	720	734	rVB	469830	735374	16.41%	1.714%
7	7.628	748	755	769	rBV	653621	1033755	23.07%	2.410%
8	8.105	827	836	848	rBV	518439	845755	18.87%	1.971%
9	8.805	948	955	974	rBV	713406	1243725	27.75%	2.899%
10	9.275	1027	1035	1048	rVV	619503	1042463	23.26%	2.430%
11	10.004	1151	1159	1171	rBV	553230	941887	21.02%	2.195%
12	10.540	1242	1250	1267	rBV	806453	1431119	31.93%	3.336%
13	10.928	1306	1316	1325	rBV	783031	1321335	29.48%	3.080%
14	11.063	1331	1339	1357	rBV	800550	1413397	31.54%	3.295%
15	12.510	1579	1585	1593	rBV	14343	25979	0.58%	0.061%
16	13.628	1767	1775	1781	rBV9	7197	16504	0.37%	0.038%
17	14.145	1854	1863	1875	rBV	1647769	2369112	52.86%	5.522%
18	14.257	1878	1882	1887	rVB8	3261	6903	0.15%	0.016%
19	14.440	1906	1913	1926	rVB	1776338	2612880	58.30%	6.090%
20	14.739	1957	1964	1973	rBV	1284795	1991366	44.43%	4.642%
21	14.922	1989	1995	2015	rBV	642278	1075522	24.00%	2.507%
22	15.145	2030	2033	2037	rVB6	3793	4908	0.11%	0.011%
23	15.734	2126	2133	2140	rBV	2465680	3434375	76.63%	8.005%
24	15.845	2145	2152	2166	rVV	795991	1085815	24.23%	2.531%
25	15.975	2170	2174	2181	rVB5	13207	20792	0.46%	0.048%
26	16.510	2263	2265	2272	rVB8	3761	6672	0.15%	0.016%
27	17.169	2373	2377	2381	rBV7	5066	8673	0.19%	0.020%
28	17.286	2393	2397	2399	rBV5	4103	5801	0.13%	0.014%
29	17.498	2425	2433	2442	rBV	1607921	2376313	53.02%	5.539%
30	17.598	2443	2450	2461	rVV	2751362	3799044	84.77%	8.855%
31	19.392	2751	2755	2761	rVB2	41592	55272	1.23%	0.129%
32	19.463	2763	2767	2771	rVV	32272	44654	1.00%	0.104%
33	19.816	2821	2827	2839	rBV	3368609	4481653	100.00%	10.446%
34	21.574	3121	3126	3133	rBV	1684800	2234648	49.86%	5.209%
35	23.963	3525	3532	3543	rVB2	1629420	3440020	76.76%	8.018%
36	24.127	3554	3560	3570	rVB2	957335	2005424	44.75%	4.674%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013865.D
Acq On : 21 Feb 2023 13:57
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK960

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42901464

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013865.D
Acq On : 21 Feb 2023 13:57
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK960

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

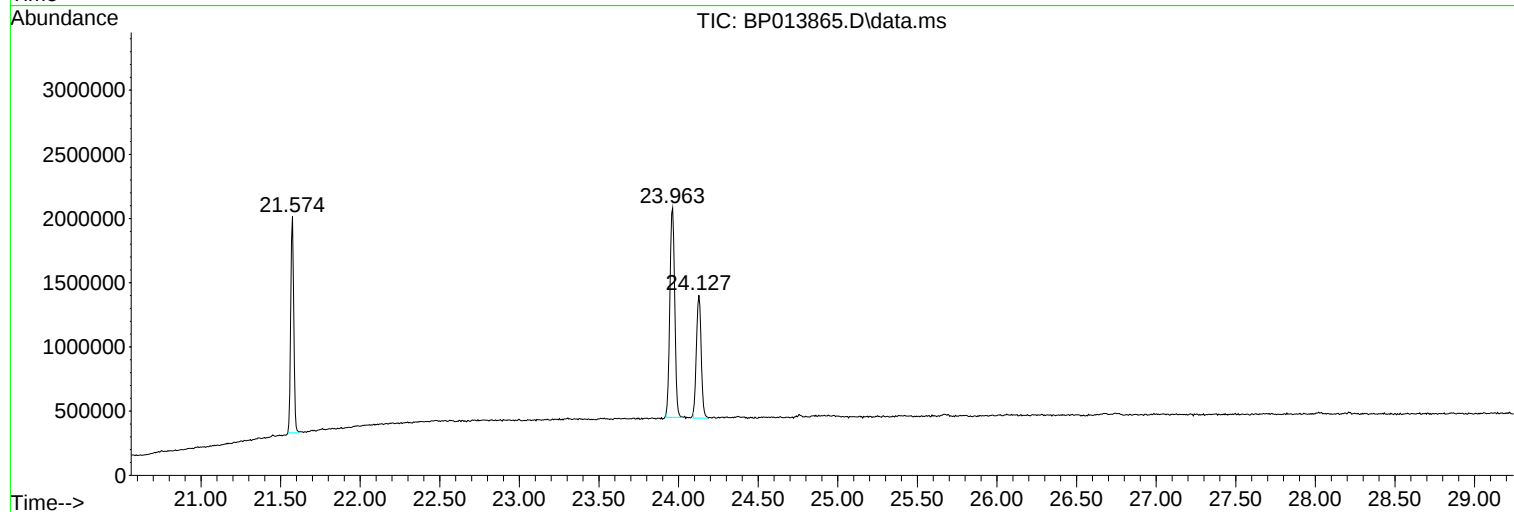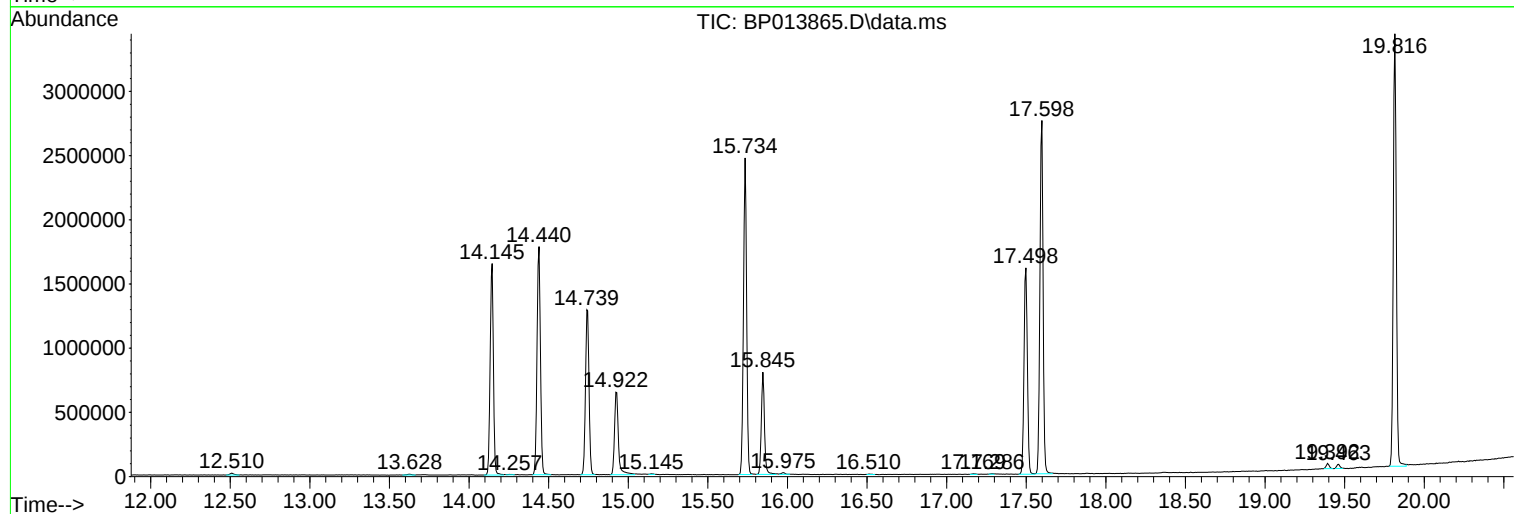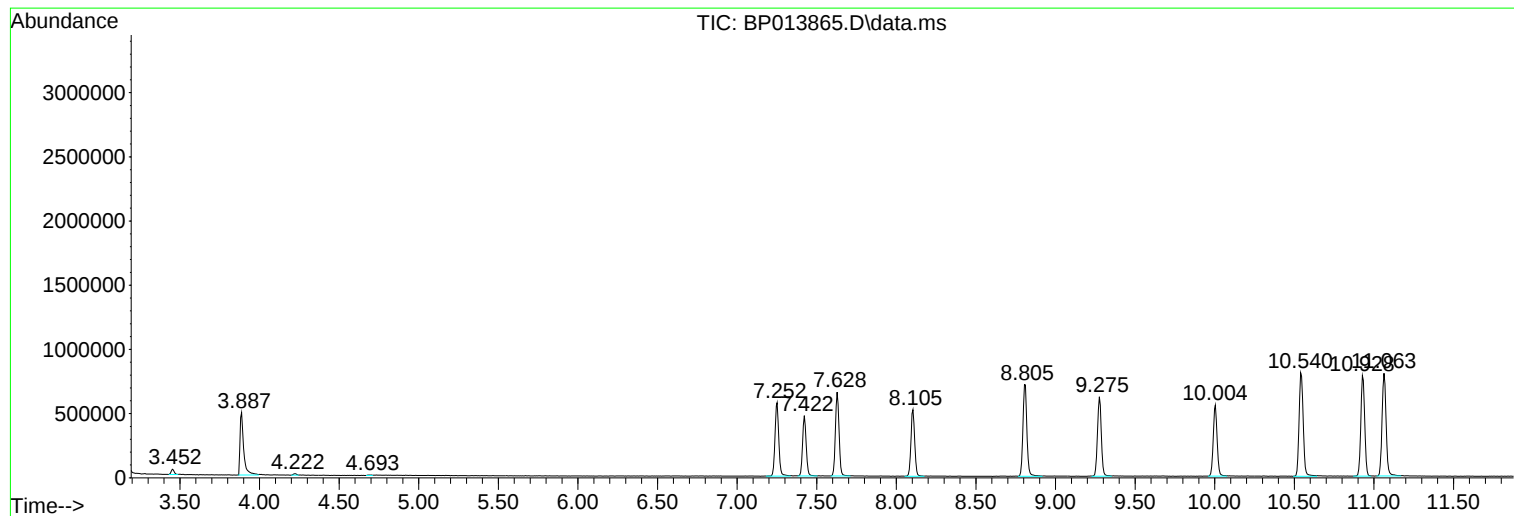

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013865.D
Acq On : 21 Feb 2023 13:57
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK960

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022123\
Data File : BP013865.D
Acq On : 21 Feb 2023 13:57
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK960

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc