
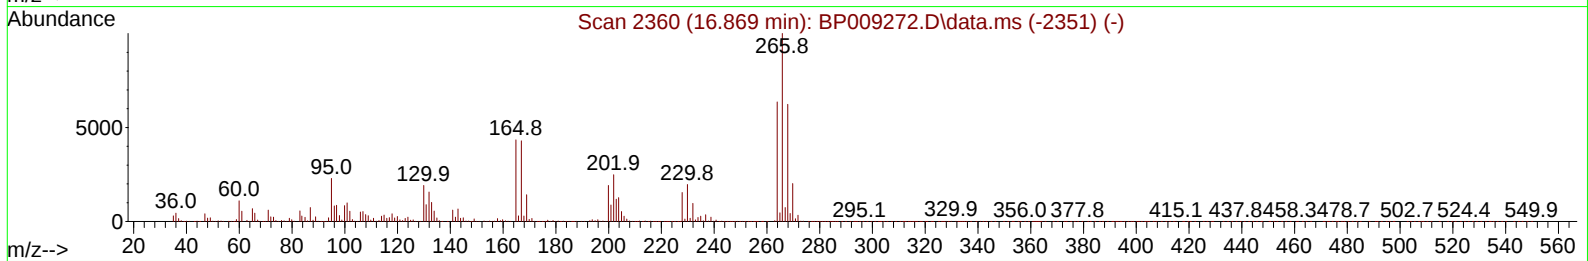
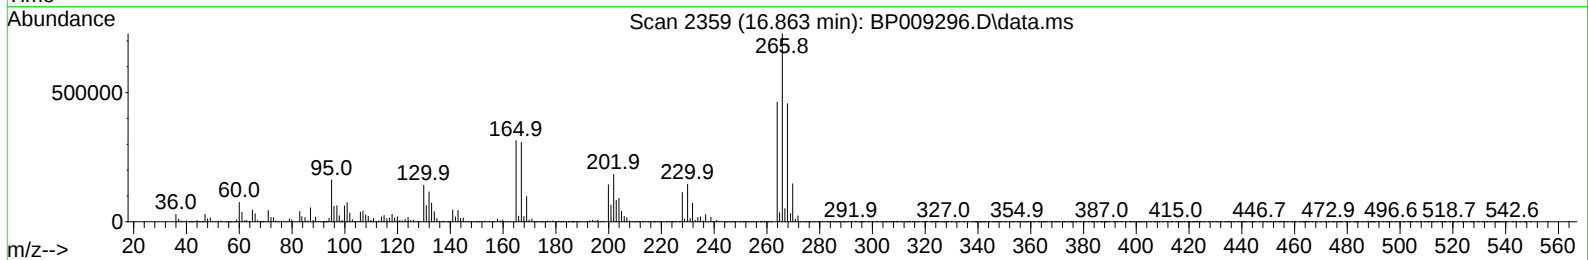


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
 Data File : BP009296.D
 Acq On : 08 Mar 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 04:10:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

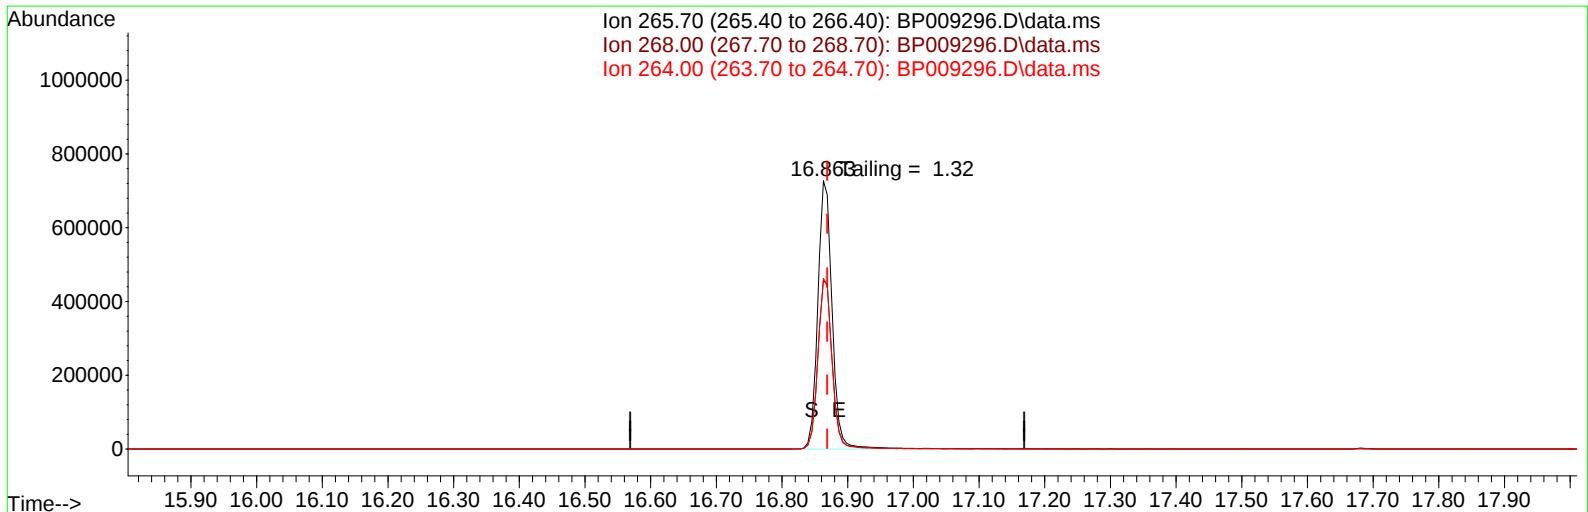

TIC: BP009296.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.006) 306543.95 ng

response 1097342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.85
264.00	63.60	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009296.D
Acq On : 08 Mar 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 04:10:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

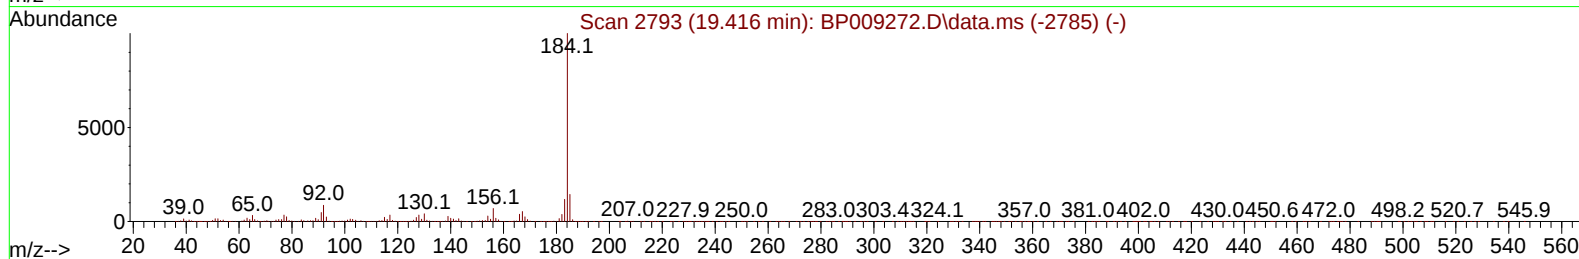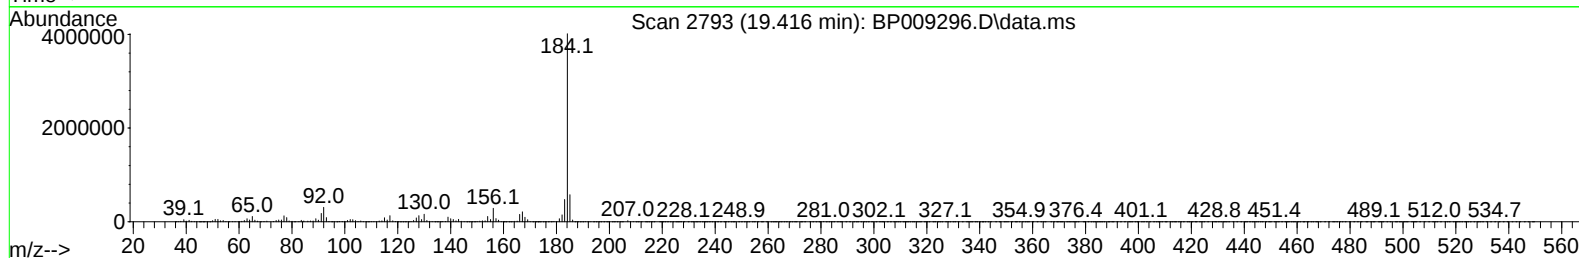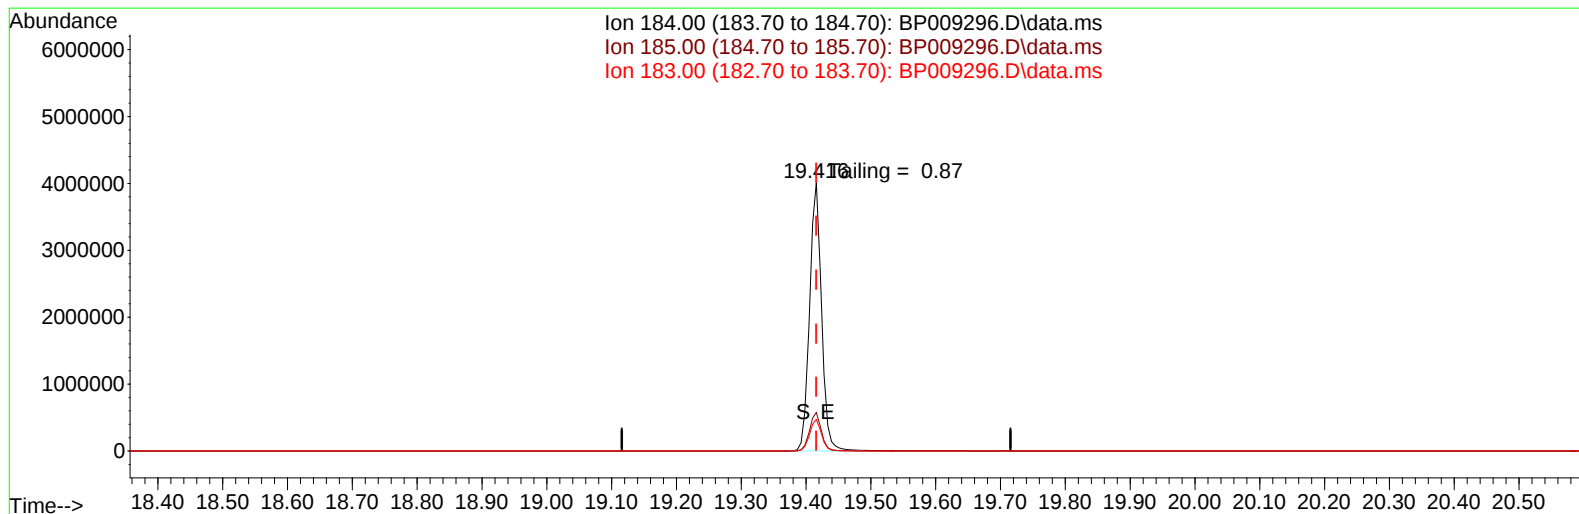

TIC: BP009296.D\data.ms

(77) Benzidine**19.416min (+ 0.000) 184155.41 ng****response 5174330**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.70	11.81
0.00	0.00	0.00