

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009298.D
Acq On : 08 Mar 2022 11:19
Operator : CG/JU
Sample : PB143133BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143133BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009298.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.417	405	413	428	rBV	8558594	13761917	56.47%	11.204%
2	6.993	672	681	693	rBV	8074182	13832973	56.76%	11.262%
3	7.816	814	821	832	rBV	1628609	2824073	11.59%	2.299%
4	8.969	1008	1017	1027	rBV	5021298	8880723	36.44%	7.230%
5	10.610	1288	1296	1308	rBV	2176115	3854045	15.81%	3.138%
6	13.081	1707	1716	1728	rBV	13104274	20674150	84.83%	16.831%
7	14.457	1942	1950	1959	rBV	3130925	4936217	20.25%	4.019%
8	15.951	2196	2204	2227	rBV	9380168	14235398	58.41%	11.589%
9	17.216	2412	2419	2432	rBV	3611172	5361839	22.00%	4.365%
10	19.792	2851	2857	2865	rBV	18359390	24371342	100.00%	19.841%
11	21.322	3112	3117	3125	rBV	3822065	5002001	20.52%	4.072%
12	23.727	3519	3526	3536	rVB2	2338681	5095514	20.91%	4.148%




Sum of corrected areas: 122830192

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009298.D
Acq On : 08 Mar 2022 11:19
Operator : CG/JU
Sample : PB143133BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143133BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

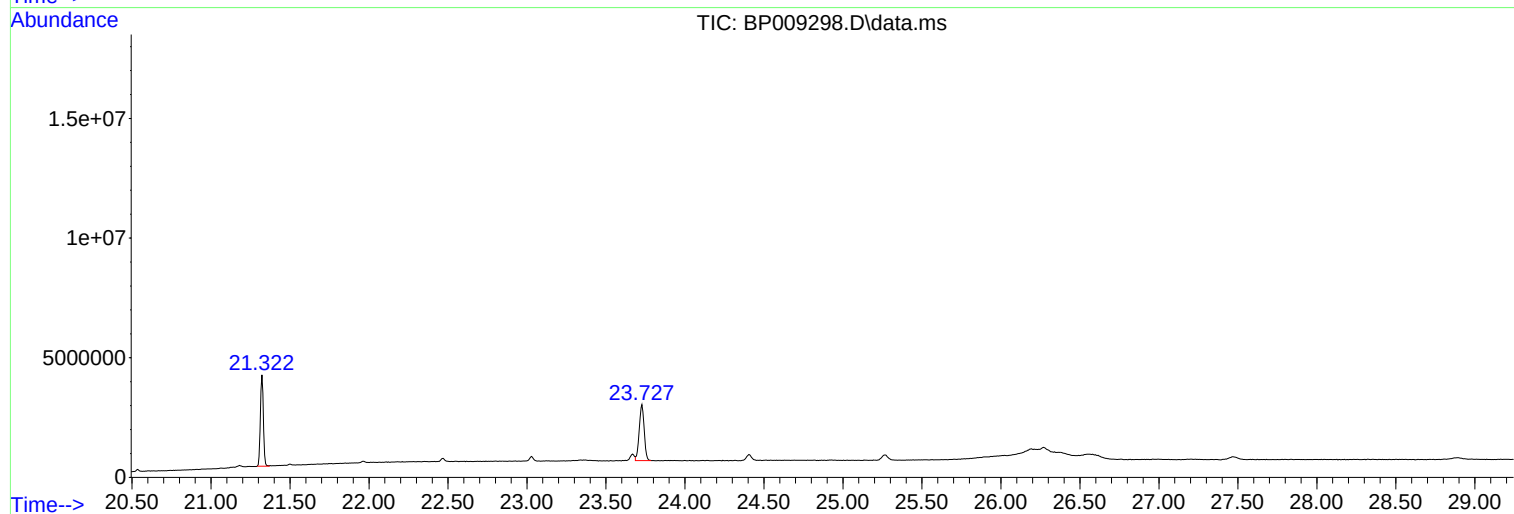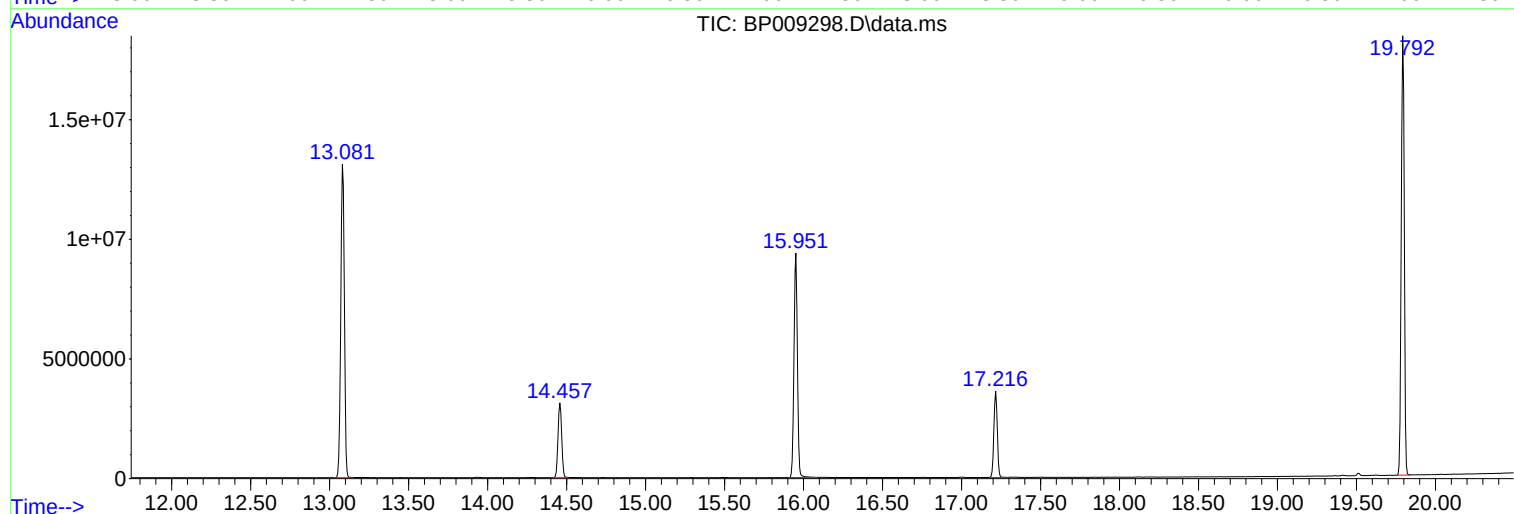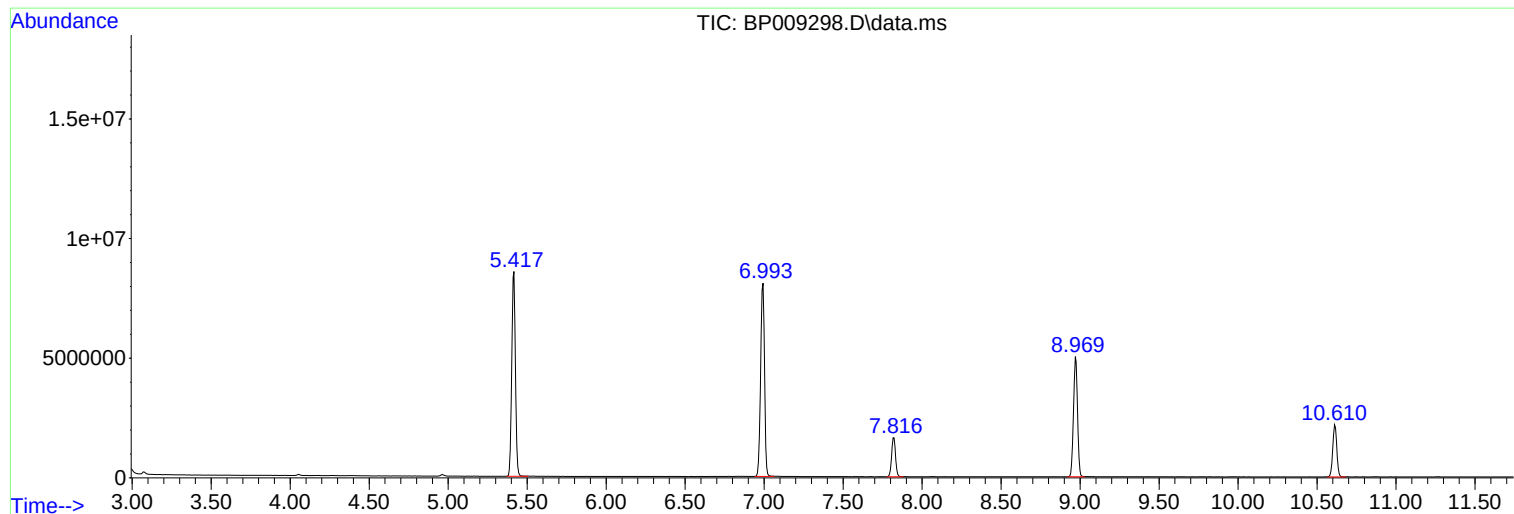

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009298.D
Acq On : 08 Mar 2022 11:19
Operator : CG/JU
Sample : PB143133BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143133BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009298.D
Acq On : 08 Mar 2022 11:19
Operator : CG/JU
Sample : PB143133BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143133BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------