

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
 Data File : BP009301.D
 Acq On : 08 Mar 2022 13:03
 Operator : CG/JU
 Sample : PB143112BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143112BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.411	405	412	424	rBV	8786818	14319620	61.55%	11.605%
2	6.993	672	681	690	rBV	8432119	14445031	62.09%	11.707%
3	7.816	813	821	832	rBV	1722487	2929149	12.59%	2.374%
4	8.969	1008	1017	1027	rBV	5191045	9192899	39.52%	7.450%
5	10.610	1287	1296	1307	rBV	2257845	4022342	17.29%	3.260%
6	13.081	1708	1716	1730	rBV	13466938	21206129	91.16%	17.186%
7	14.457	1942	1950	1967	rBV	3269939	5061785	21.76%	4.102%
8	15.951	2195	2204	2222	rBV	9099647	13984852	60.12%	11.334%
9	17.216	2412	2419	2428	rBV	3476767	5297652	22.77%	4.293%
10	19.792	2851	2857	2866	rBV	18357999	23263156	100.00%	18.854%
11	21.321	3112	3117	3124	rBV	3714178	4755288	20.44%	3.854%
12	23.727	3519	3526	3534	rVB2	2282377	4910511	21.11%	3.980%




Sum of corrected areas: 123388414

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009301.D
Acq On : 08 Mar 2022 13:03
Operator : CG/JU
Sample : PB143112BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143112BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

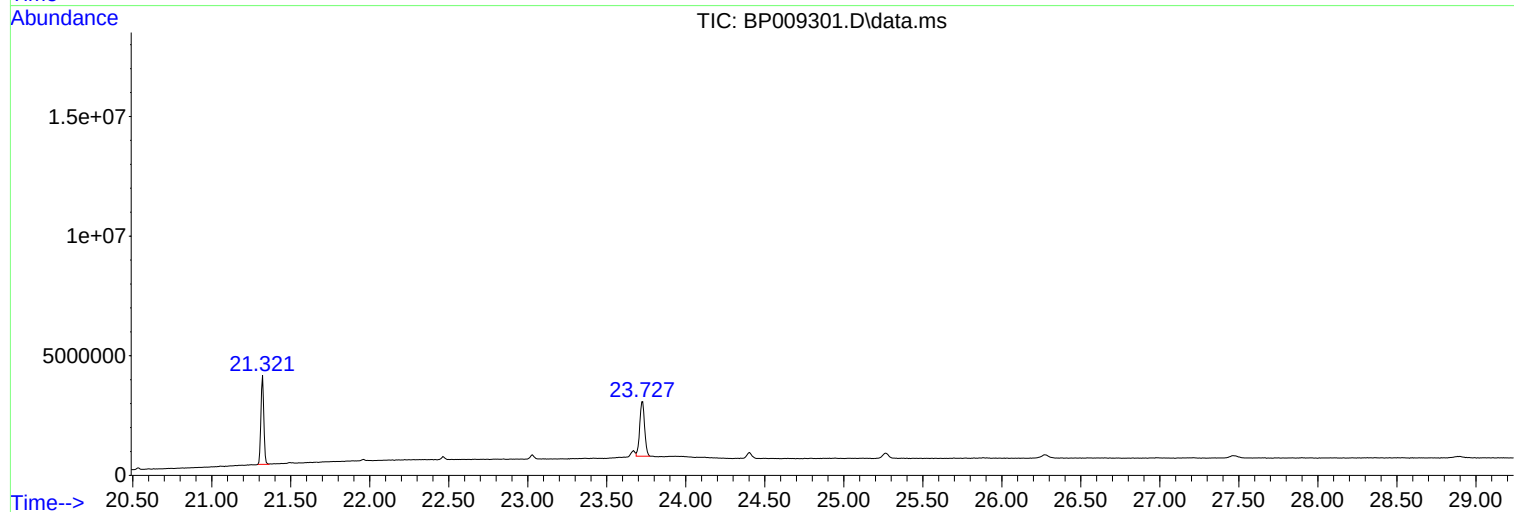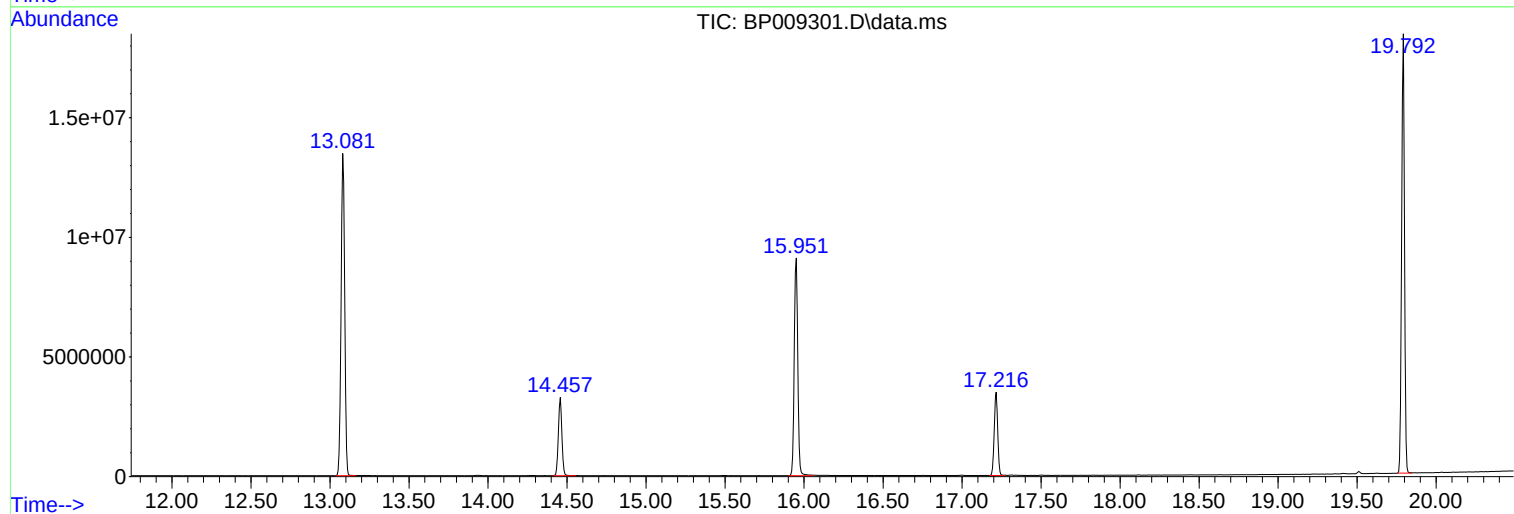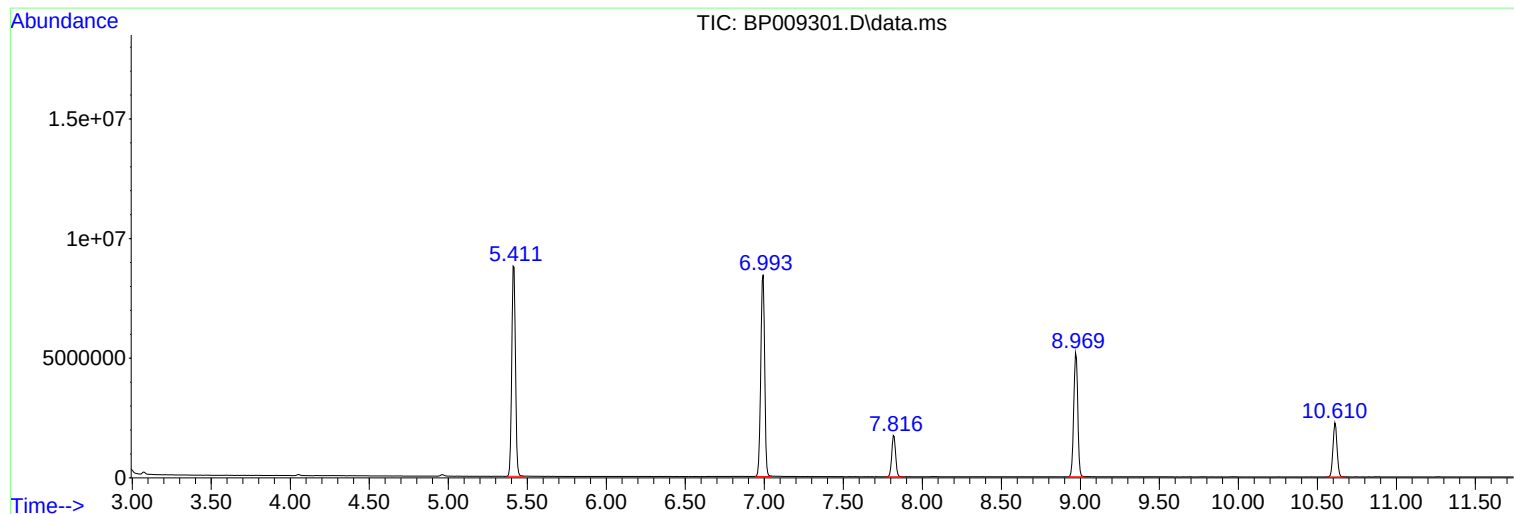

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009301.D
Acq On : 08 Mar 2022 13:03
Operator : CG/JU
Sample : PB143112BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143112BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009301.D
Acq On : 08 Mar 2022 13:03
Operator : CG/JU
Sample : PB143112BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143112BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------