

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
 Data File : BP009302.D
 Acq On : 08 Mar 2022 13:40
 Operator : CG/JU
 Sample : PB143161BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143161BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.417	405	413	430	rBV	9693699	15138192	64.06%	11.825%
2	6.993	672	681	695	rBV	8996337	15313244	64.80%	11.962%
3	7.822	814	822	831	rBV	1836593	3081446	13.04%	2.407%
4	8.975	1008	1018	1037	rBV	5638696	9734493	41.19%	7.604%
5	10.616	1288	1297	1306	rBV	2292063	4188106	17.72%	3.272%
6	13.087	1708	1717	1733	rBV	13698711	22154974	93.75%	17.306%
7	14.457	1943	1950	1969	rBV	3383713	5250597	22.22%	4.101%
8	15.951	2196	2204	2224	rBV	9958572	14353660	60.74%	11.212%
9	17.216	2412	2419	2431	rBV	3505966	5421386	22.94%	4.235%
10	19.792	2851	2857	2865	rBV	18397663	23631958	100.00%	18.460%
11	21.322	3112	3117	3123	rBV	3720852	4821704	20.40%	3.766%
12	23.727	3520	3526	3535	rVB2	2361588	4927502	20.85%	3.849%


Sum of corrected areas: 128017262

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009302.D
Acq On : 08 Mar 2022 13:40
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

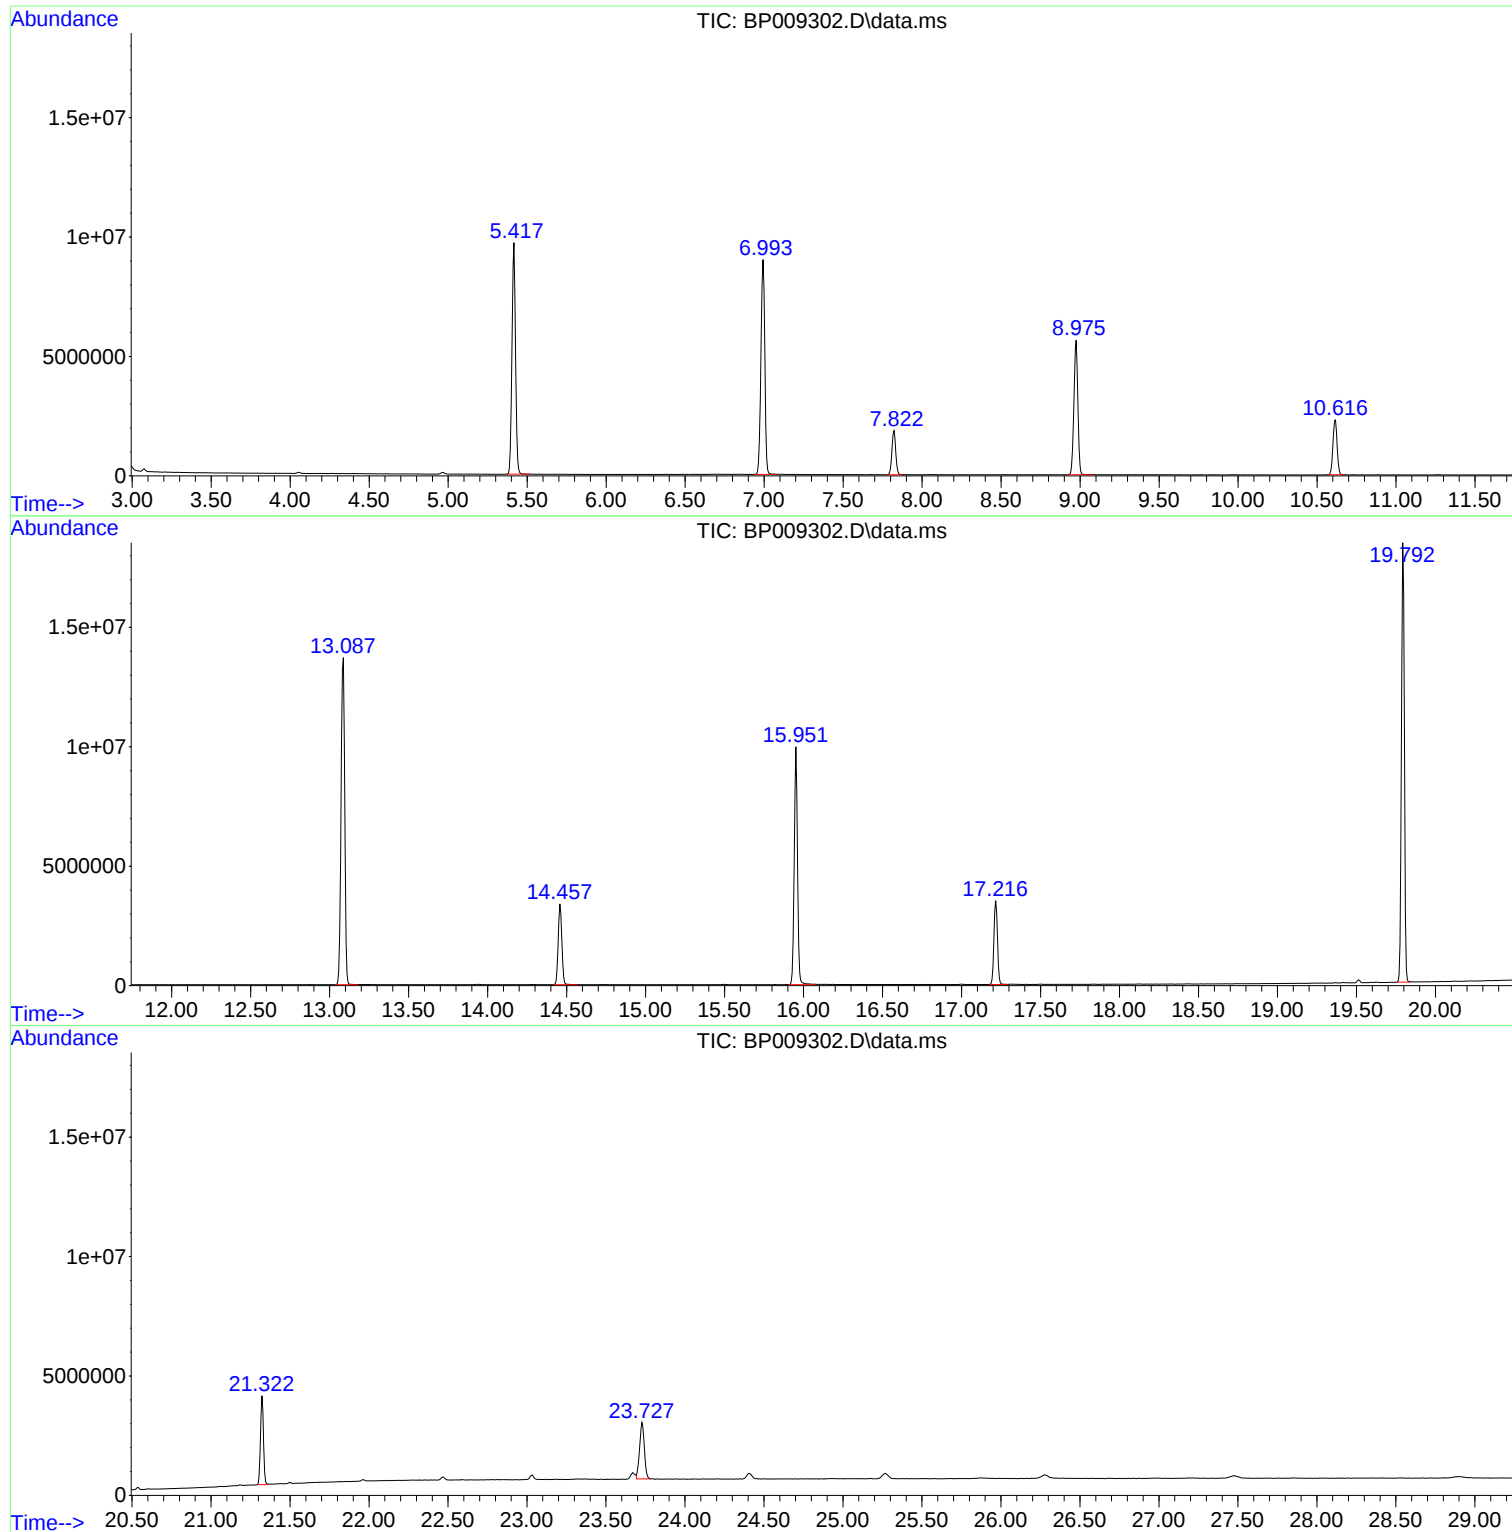

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009302.D
Acq On : 08 Mar 2022 13:40
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
Data File : BP009302.D
Acq On : 08 Mar 2022 13:40
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------