


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
 Data File : BP009296.D
 Acq On : 08 Mar 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

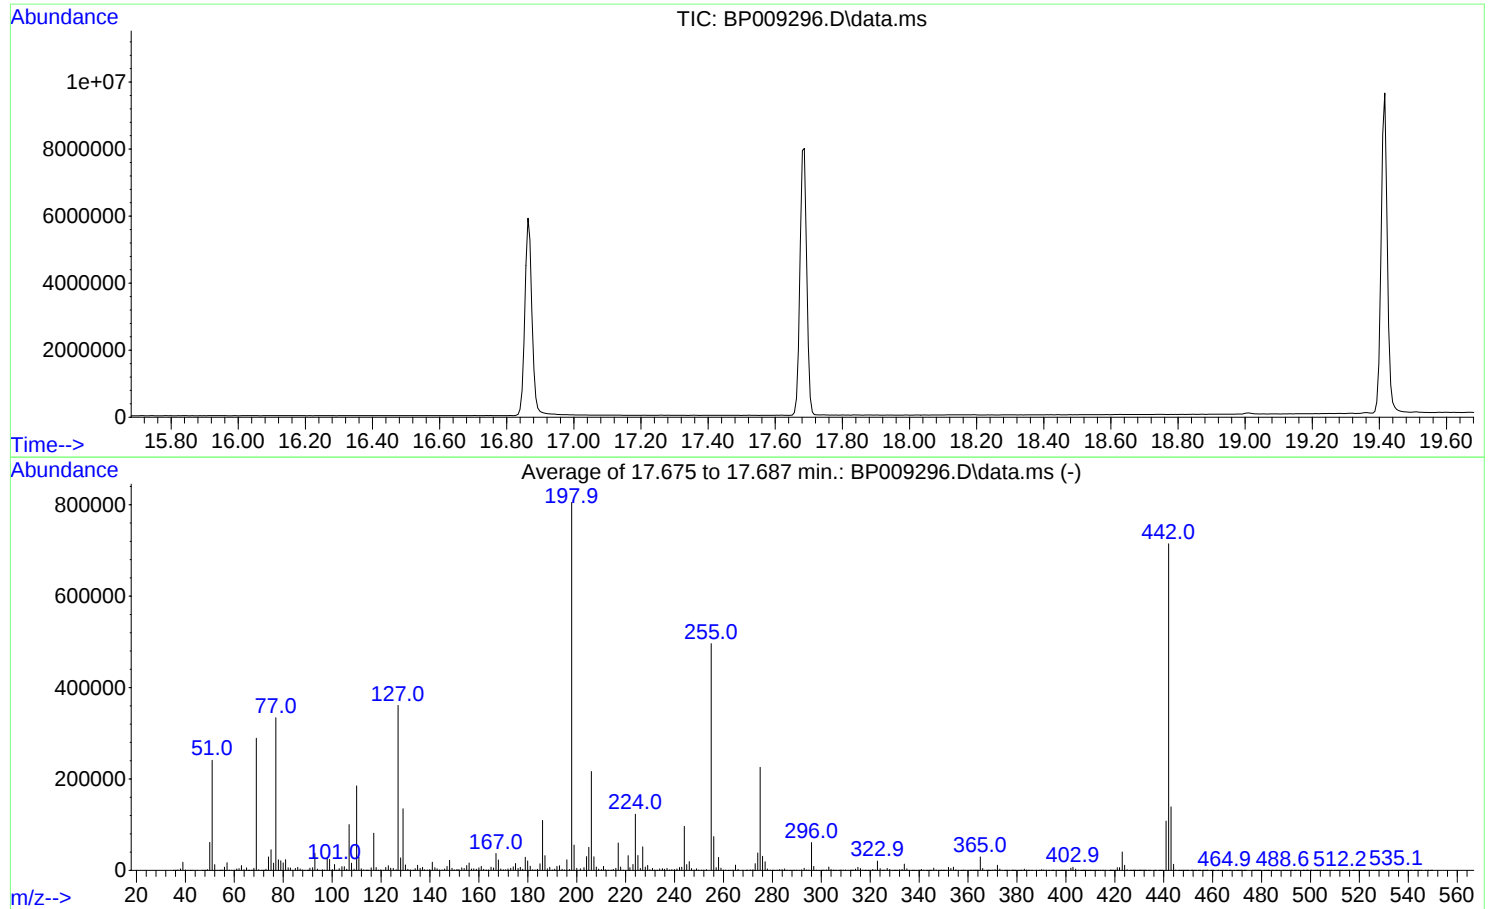




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	240862	PASS
68	69	0.00	2	1.6	4609	PASS
69	198	0.00	100	35.9	289164	PASS
70	69	0.00	2	0.4	1272	PASS
127	198	10	80	44.8	360837	PASS
197	198	0.00	2	0.3	2262	PASS
198	198	100	100	100.0	804960	PASS
199	198	5	9	6.9	55453	PASS
275	198	10	60	28.0	225621	PASS
365	198	1	100	3.7	29536	PASS
441	198	0.01	100	13.4	107930	PASS
442	442	100	100	100.0	714560	PASS
443	442	15	24	19.5	139115	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
 Data File : BP009296.D
 Acq On : 08 Mar 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 09 04:10:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

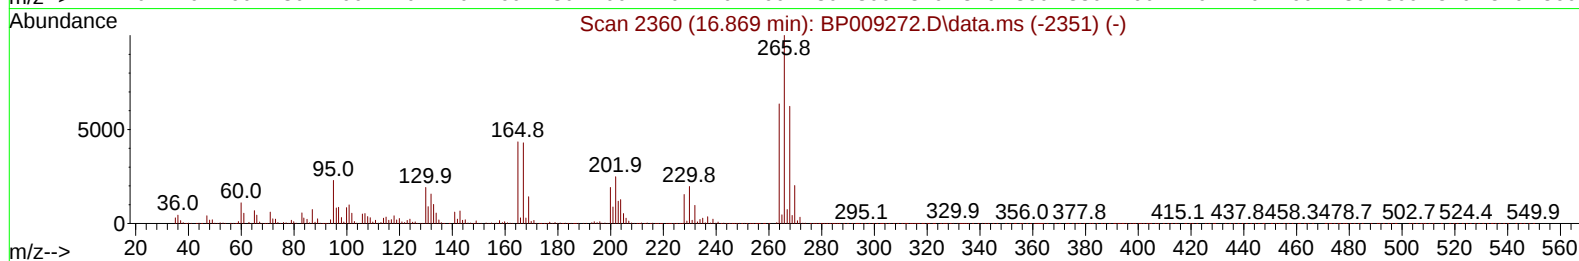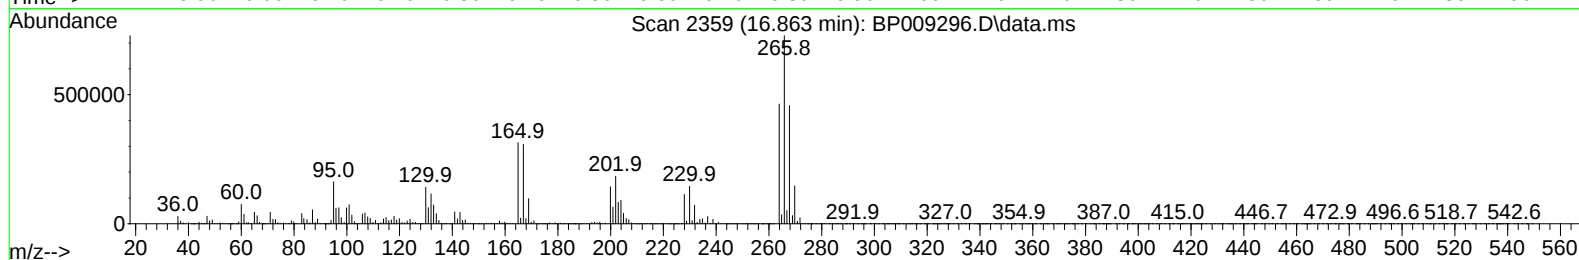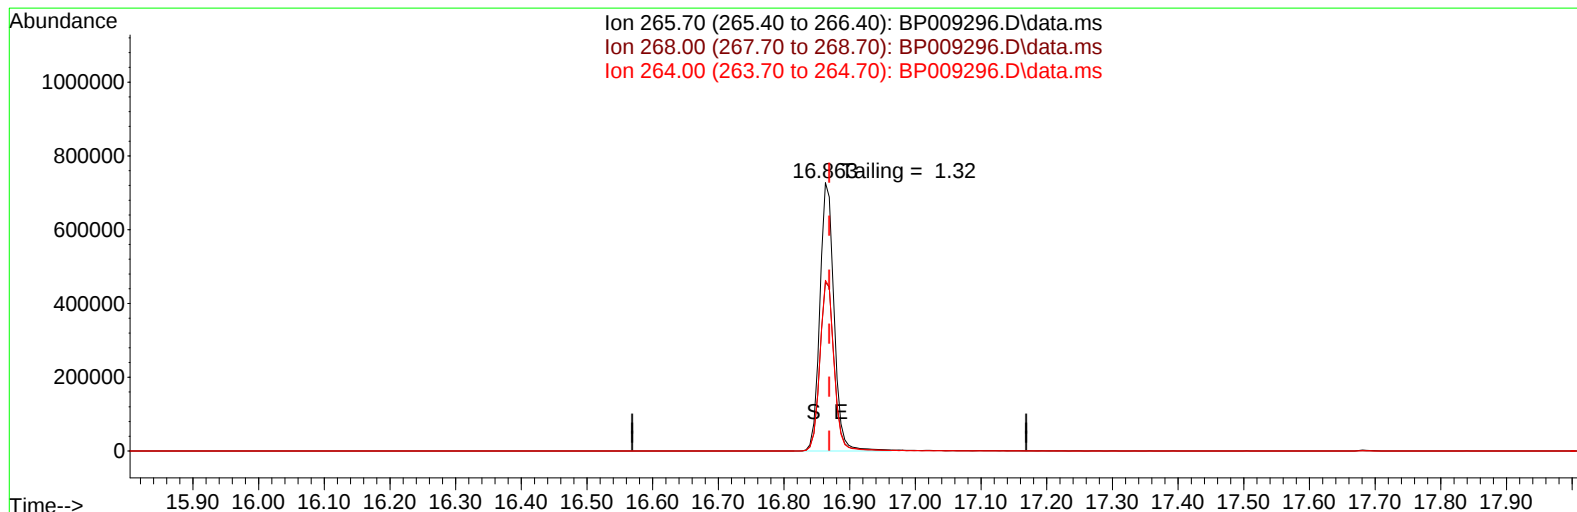

TIC: BP009296.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.006) 306543.95 ng




response 1097342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.85
264.00	63.60	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030822\
 Data File : BP009296.D
 Acq On : 08 Mar 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 09 04:10:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

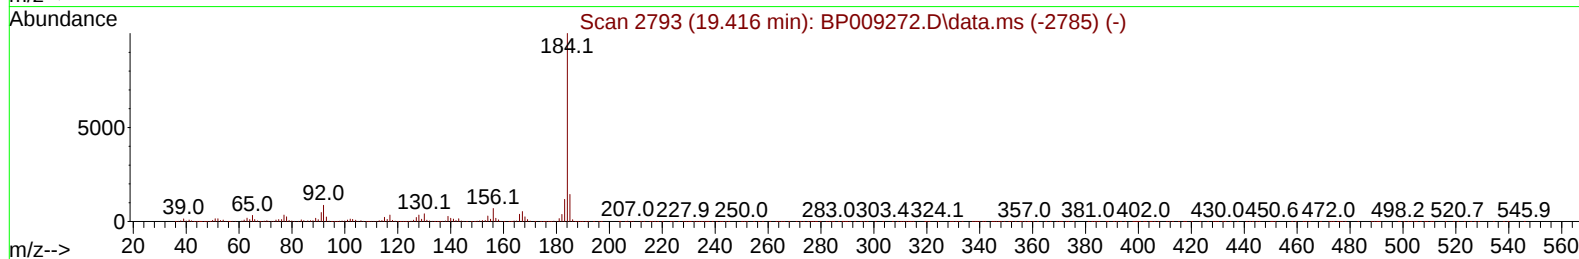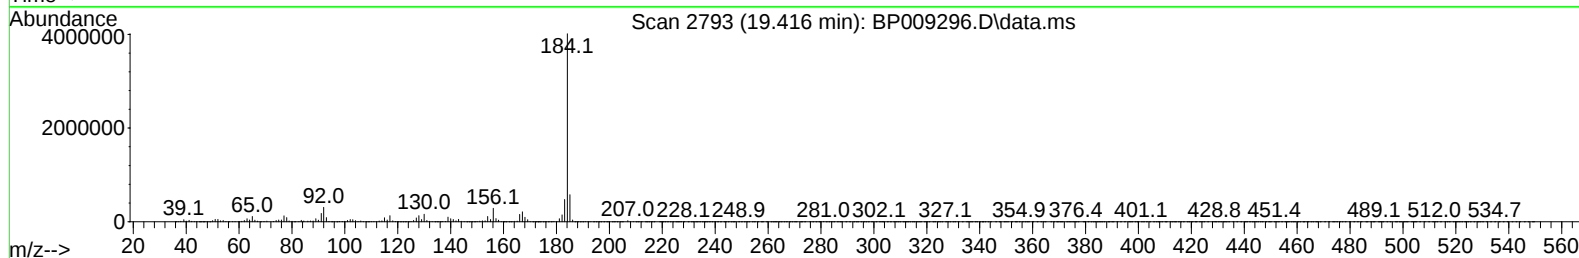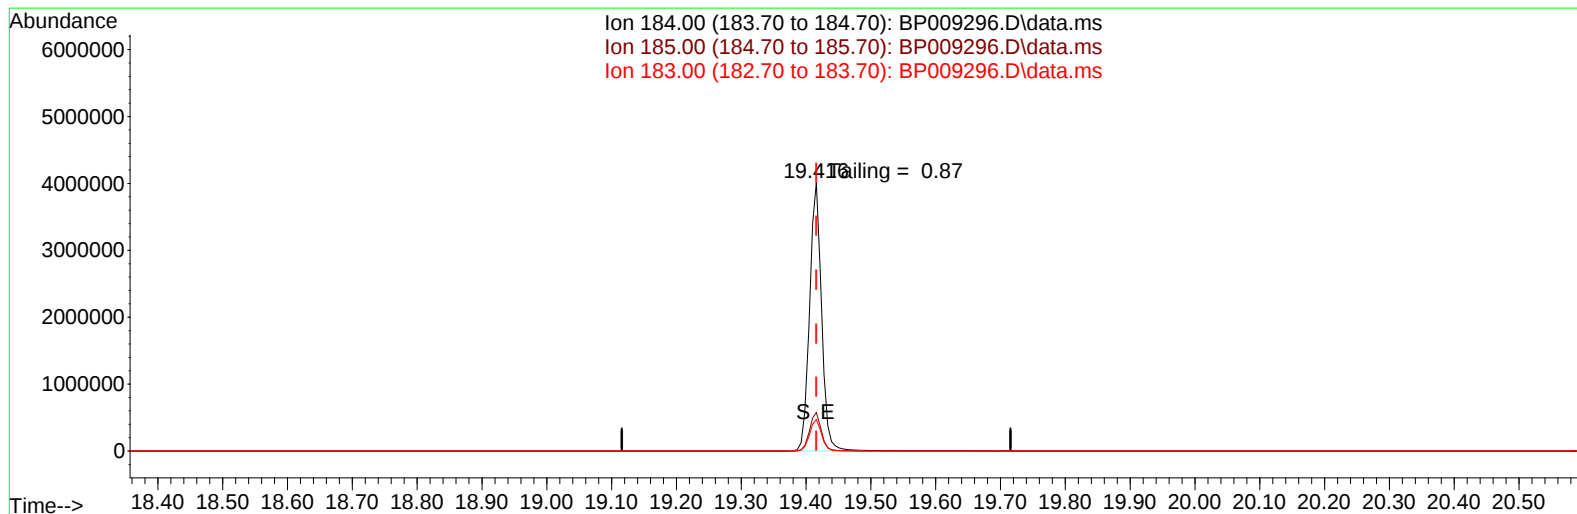

TIC: BP009296.D\data.ms

(77) Benzidine

19.416min (+ 0.000) 184155.41 ng

response 5174330

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.70	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/8/2022	BNA_P	<u>BP009296.D</u>
Compound Name	Response	Retention Time
DDT	2848681	20.633
DDD	39638	20.198
DDE	3005	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42643	2891324	1.47

Instrument :
BNA_P
ClientSampleId :
DFTPP