

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014005.D
 Acq On : 09 Mar 2023 12:05
 Operator : CG/JU
 Sample : 01713-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBZZ8

Quant Time: Mar 10 00:17:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	127517	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	528707	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	383711	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	935578	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1043633	20.000	ng/ul	0.00
88) Perylene-d12	24.086	264	1034764	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.440	96	9215	2.730	ng/uL	0.00
4) Pyridine-d5	3.858	84	153	0.016	ng/ul	-0.01
7) Phenol-d5	7.234	99	165190	14.680	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	97910	14.919	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	125502	14.638	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	117724	12.807	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	63291	15.003	ng/ul	0.00
24) 2-Nitrophenol-d4	9.981	143	73862	14.627	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	134769	14.184	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	130315	10.364	ng/ul	0.00
46) Dimethylphthalate-d6	14.122	166	511030	15.693	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	534217	15.486	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	72800	12.686	ng/ul	0.00
60) Fluorene-d10	15.710	176	444506	16.106	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.828	200	86724	12.264	ng/ul	0.00
73) Anthracene-d10	17.569	188	721240	15.880	ng/ul	0.00
81) Pyrene-d10	19.792	212	1055049	18.330	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	977129	17.753	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.910	105	25602	1.724	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014005.D
Acq On : 09 Mar 2023 12:05
Operator : CG/JU
Sample : 01713-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBZZ8

Quant Time: Mar 10 00:17:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

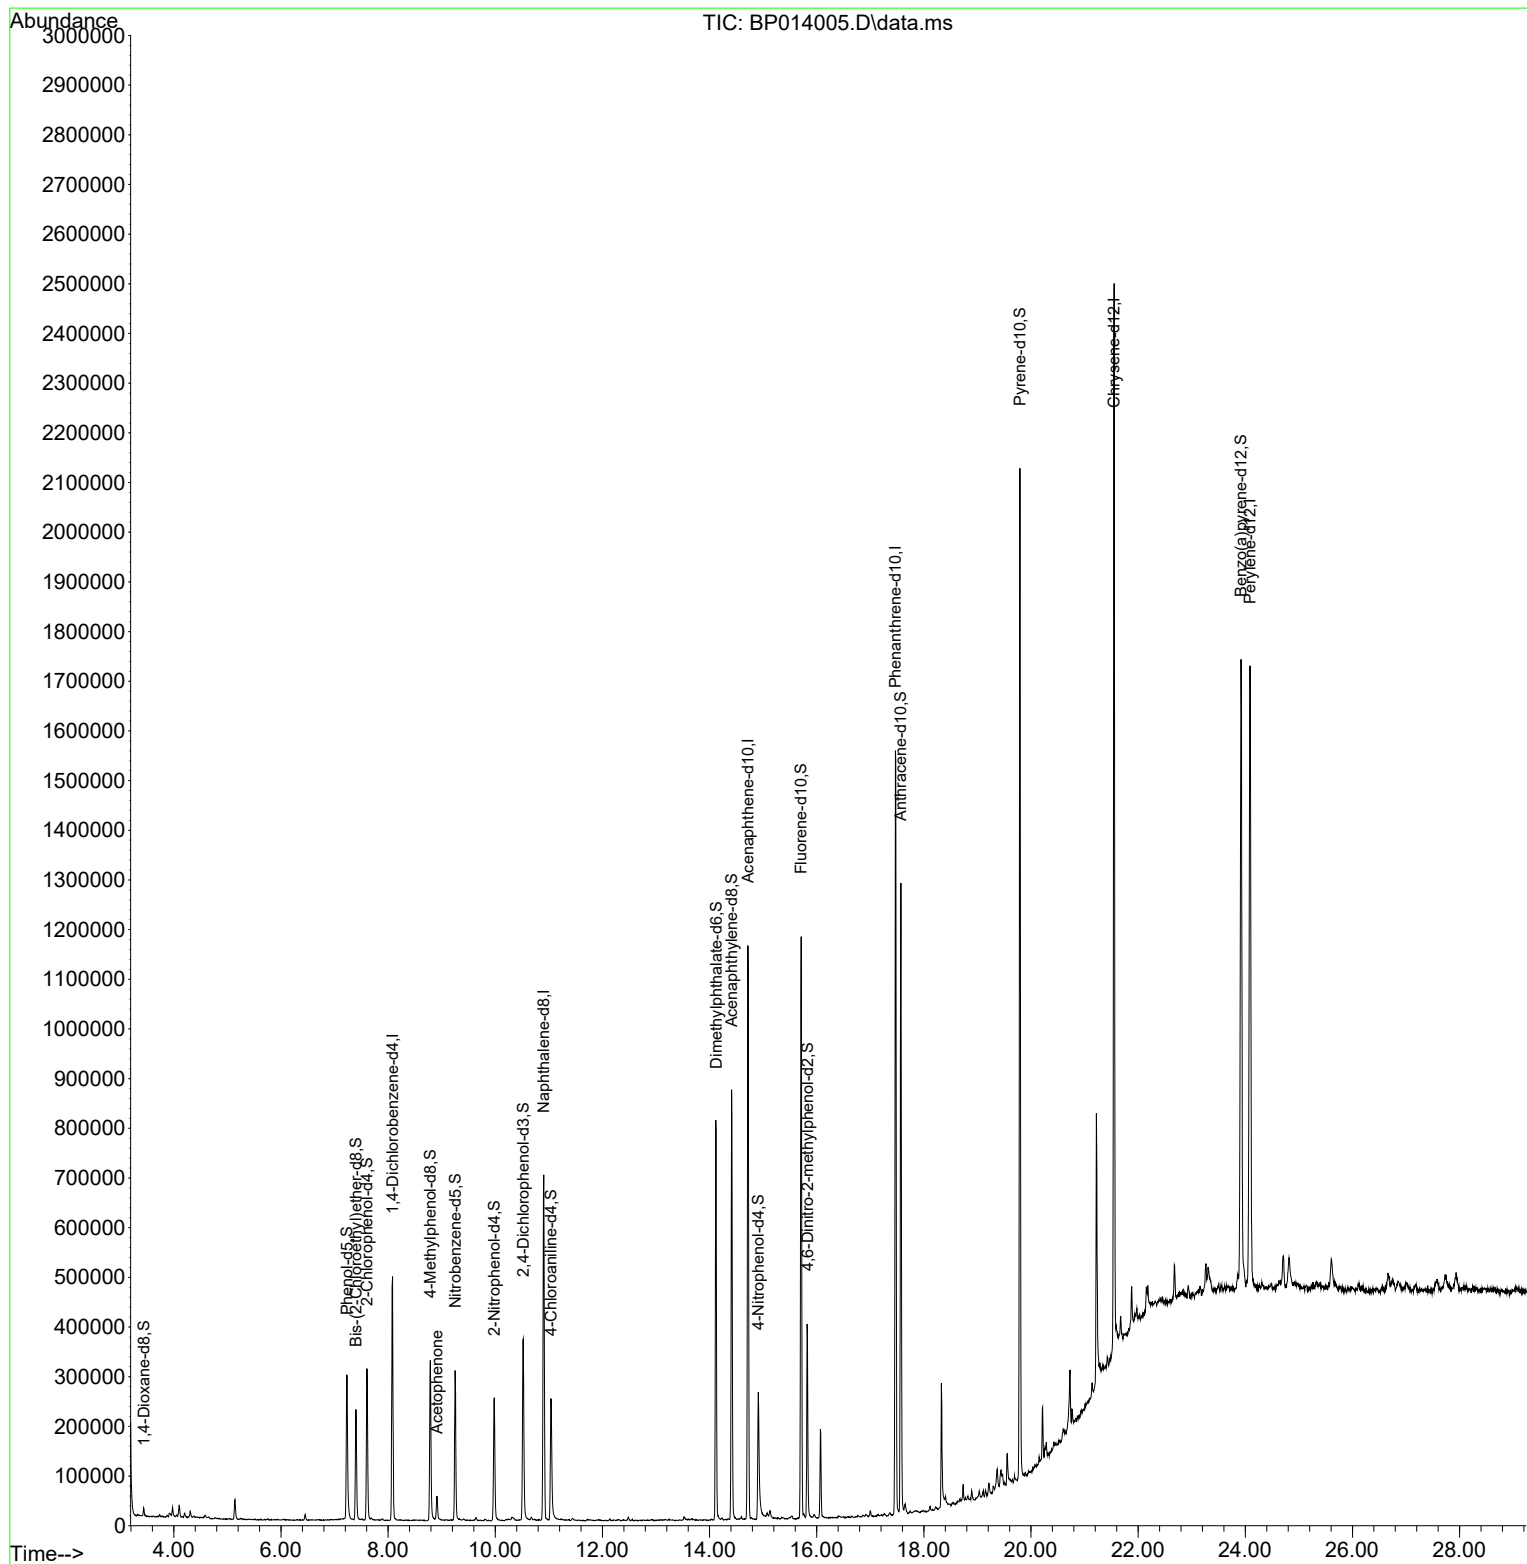

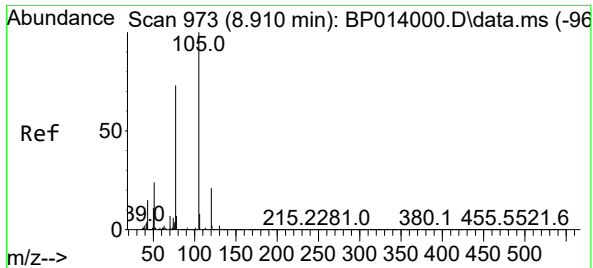

#16
Acetophenone
Concen: 1.724 ng/ul
RT: 8.910 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP014005.D
Acq: 09 Mar 2023 12:05

Instrument :
BNA_P
ClientSampleId :
DBZZ8

Tgt Ion:	105	Resp:	25602
Ion Ratio	Lower	Upper	
105	100		
77	83.5	65.4	98.2
51	27.0	21.8	32.8

