




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013992.D
Acq On : 08 Mar 2023 23:27
Operator : CG/JU
Sample : 01729-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY1

Manual IntegrationsAPPROVED

Quant Time: Mar 09 01:18:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

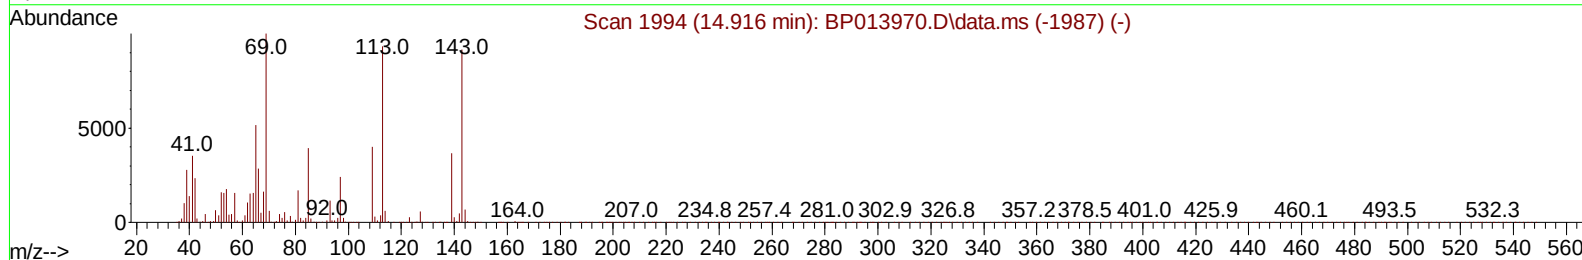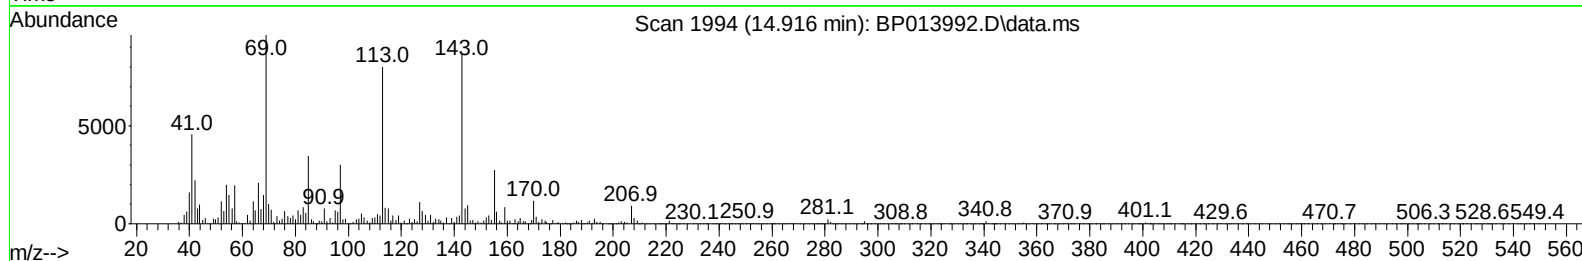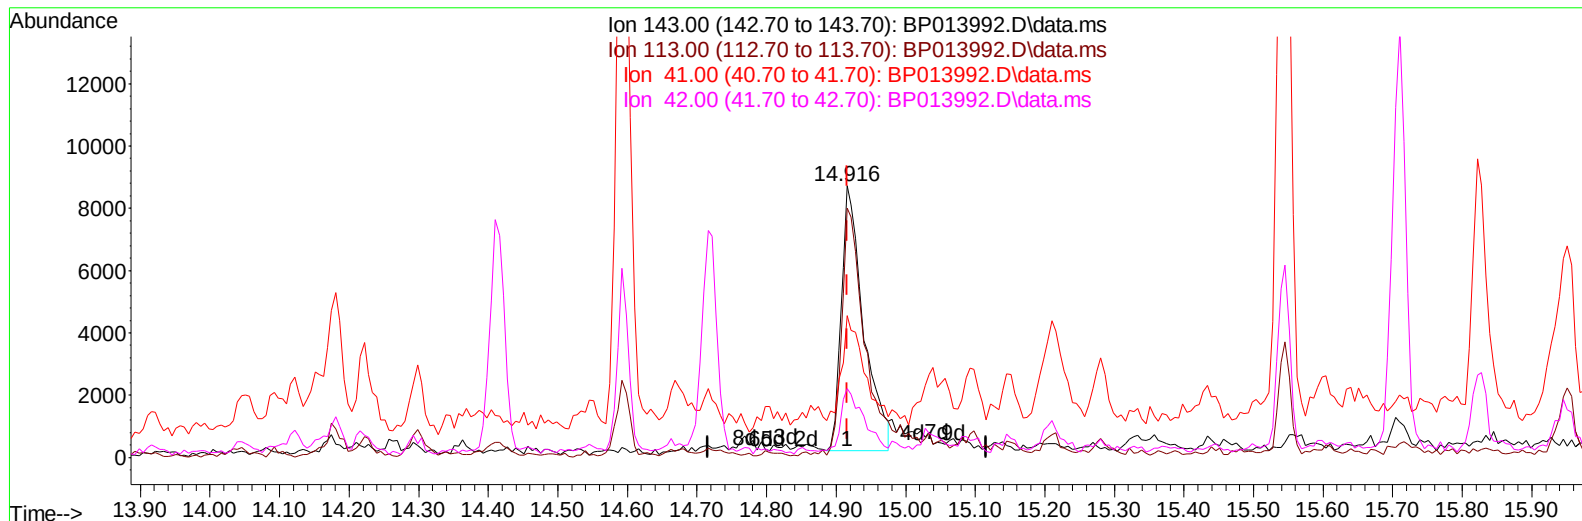

TIC: BP013992.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (-0.000) 3.87 ng/u1

response 18860

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	91.83
41.00	40.20	52.24#
42.00	28.50	25.46




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013992.D
Acq On : 08 Mar 2023 23:27
Operator : CG/JU
Sample : 01729-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY1

Manual IntegrationsAPPROVED

Quant Time: Mar 09 01:18:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

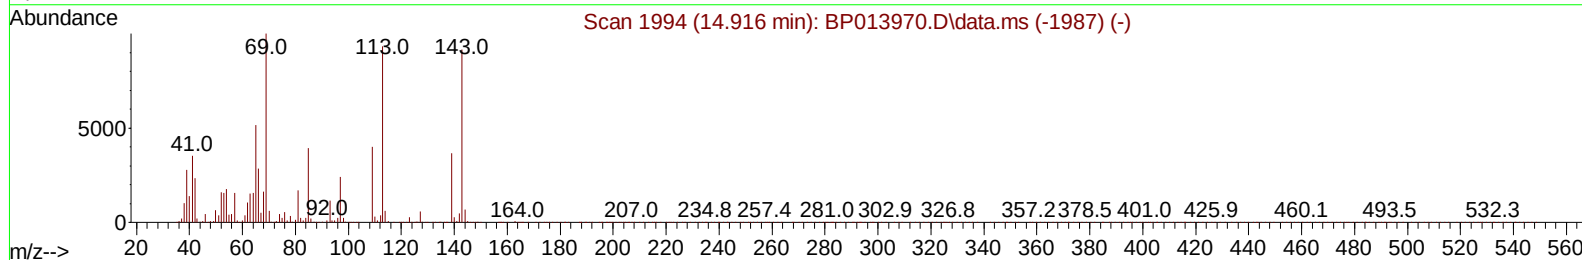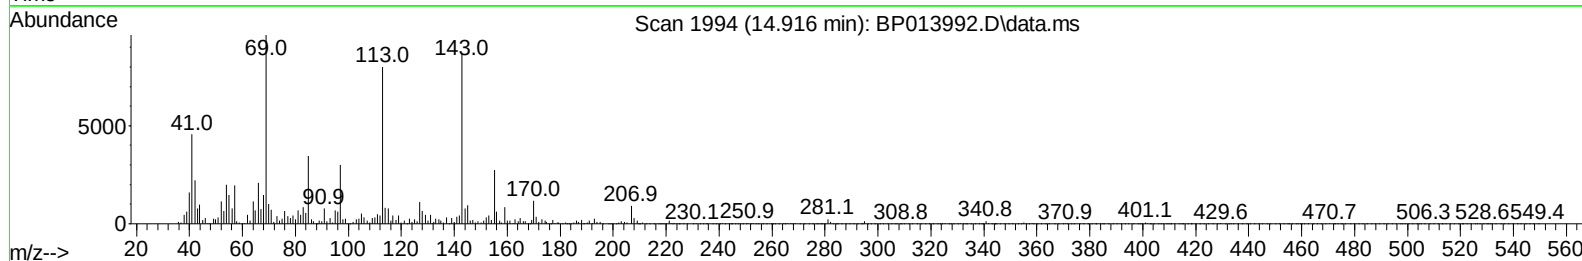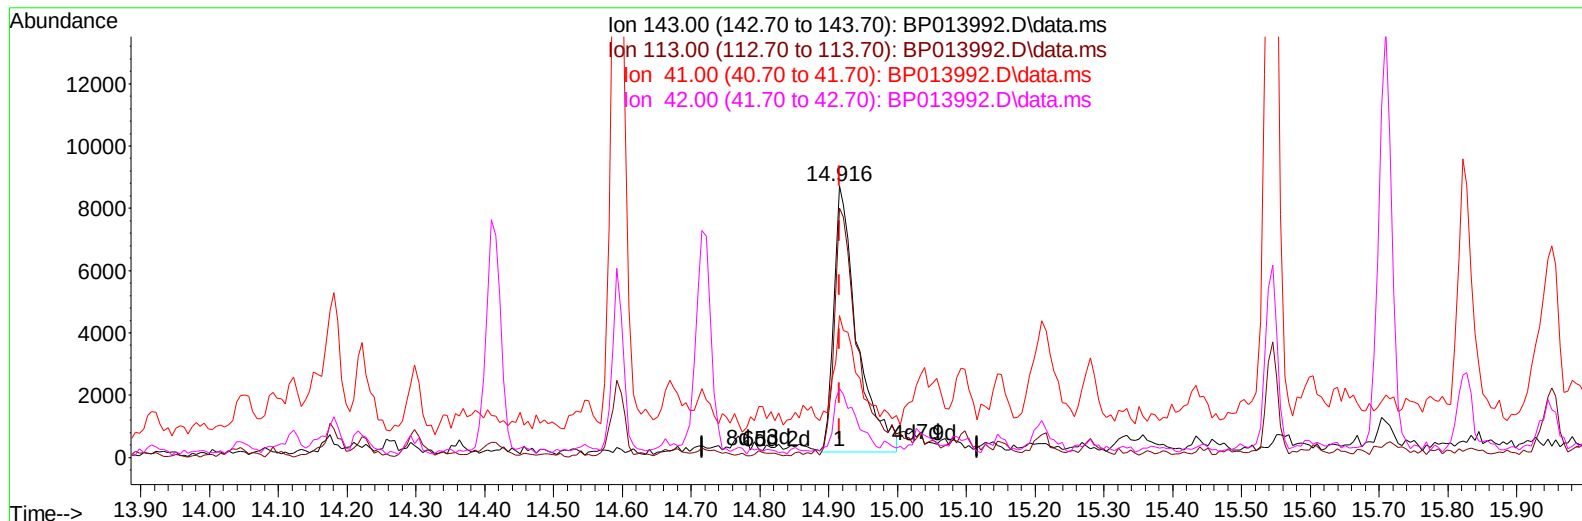

TIC: BP013992.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (-0.000) 4.14 ng/ul m

response 20168

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	91.83
41.00	40.20	52.24#
42.00	28.50	25.46

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013992.D
 Acq On : 08 Mar 2023 23:27
 Operator : CG/JU
 Sample : 01729-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BY1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 01:18:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	111272	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	454519	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.722	164	325781	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.475	188	846496	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1002370	20.000	ng/ul	0.00
88) Perylene-d12	24.086	264	1156748	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	12686	4.308	ng/uL	0.00
4) Pyridine-d5	3.875	84	47017	5.766	ng/ul	0.00
7) Phenol-d5	7.234	99	49163	5.007	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	162969	28.458	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	157102	20.999	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	92861	11.577	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	104793	28.896	ng/ul	0.00
24) 2-Nitrophenol-d4	9.981	143	117974	27.175	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	197525	24.182	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	225968	20.904	ng/ul	0.00
46) Dimethylphthalate-d6	14.122	166	827547	29.931	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	854227	29.166	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	20168m	4.139	ng/ul	0.00
60) Fluorene-d10	15.710	176	725663	30.969	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.828	200	156262	24.424	ng/ul	0.00
73) Anthracene-d10	17.575	188	1255827	30.560	ng/ul	0.00
81) Pyrene-d10	19.792	212	1642059	29.702	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	1923762	31.265	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013992.D
Acq On : 08 Mar 2023 23:27
Operator : CG/JU
Sample : 01729-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 01:18:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

