




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013993.D
Acq On : 09 Mar 2023 00:01
Operator : CG/JU
Sample : 01729-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY2

Manual IntegrationsAPPROVED

Quant Time: Mar 09 02:26:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

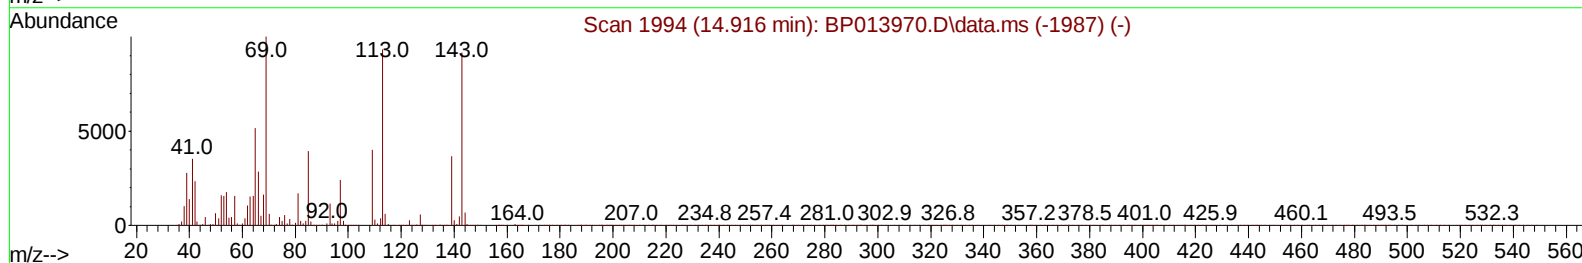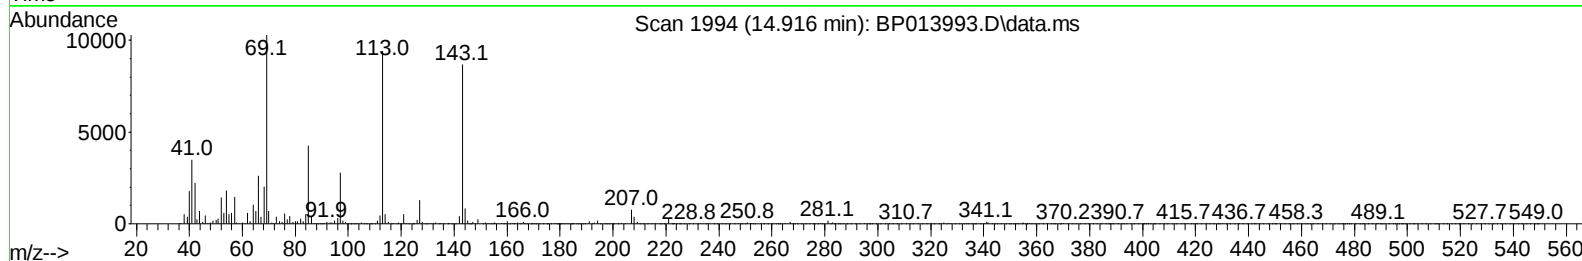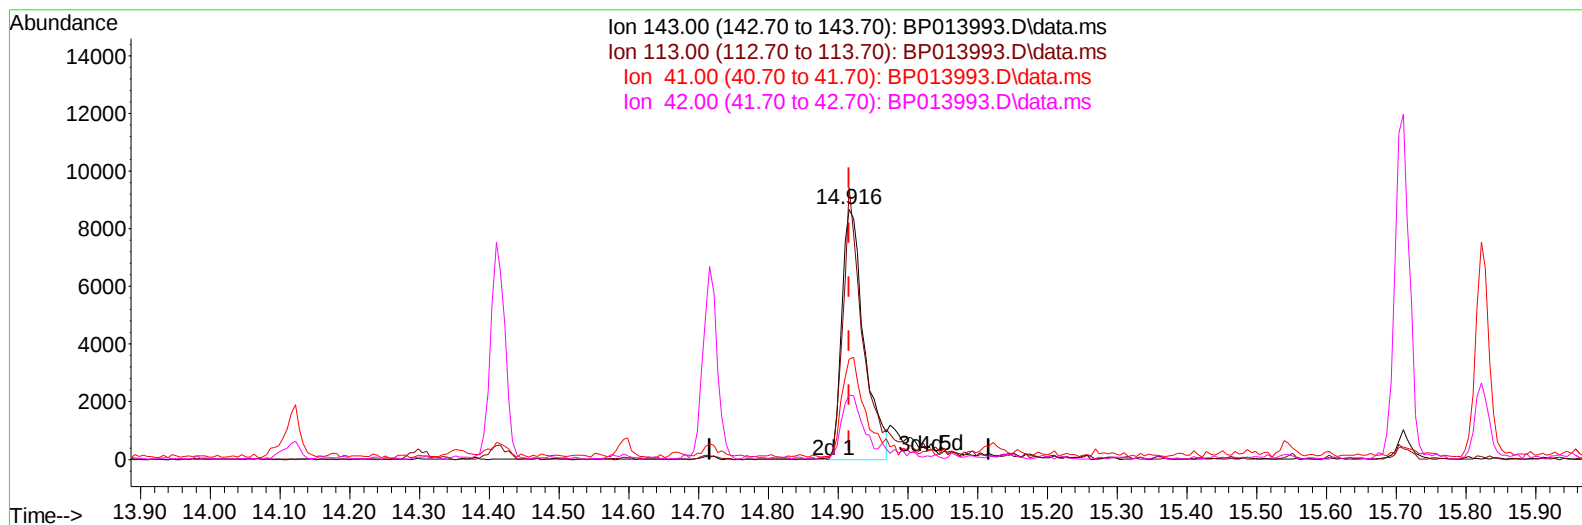

TIC: BP013993.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (-0.000) 4.48 ng/u1

response 19226

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	108.61
41.00	40.20	40.08
42.00	28.50	25.64




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013993.D
Acq On : 09 Mar 2023 00:01
Operator : CG/JU
Sample : 01729-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY2

Manual IntegrationsAPPROVED

Quant Time: Mar 09 02:26:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

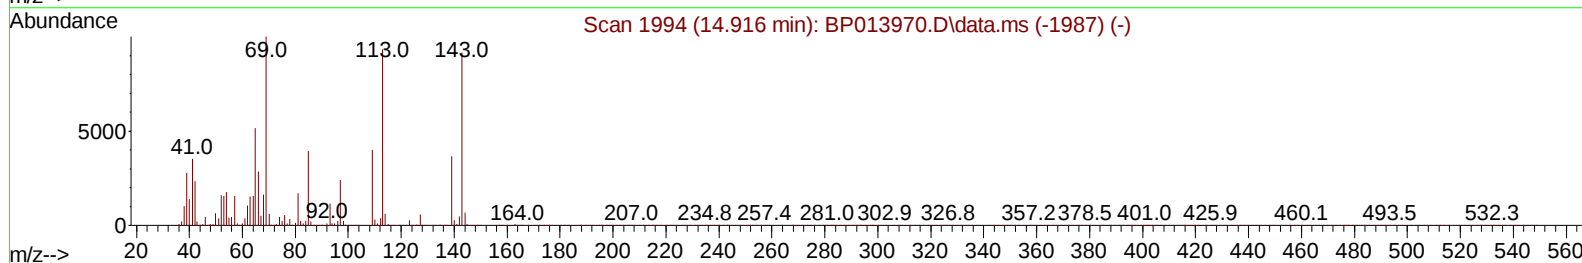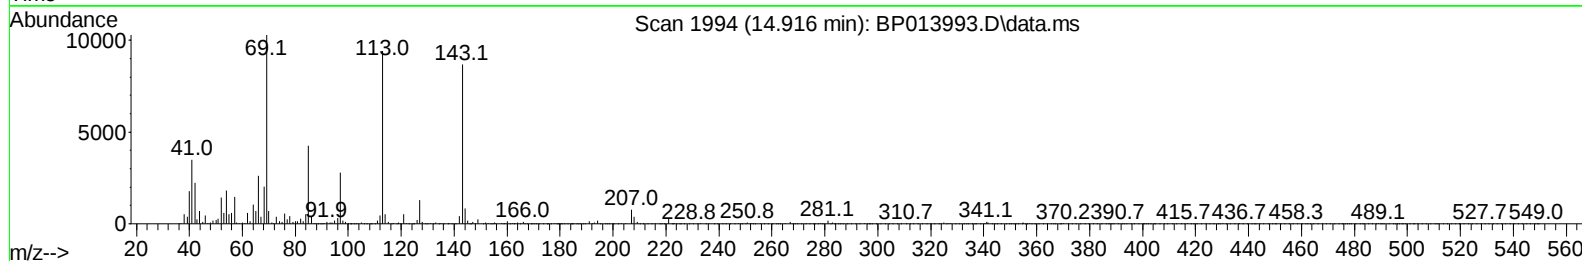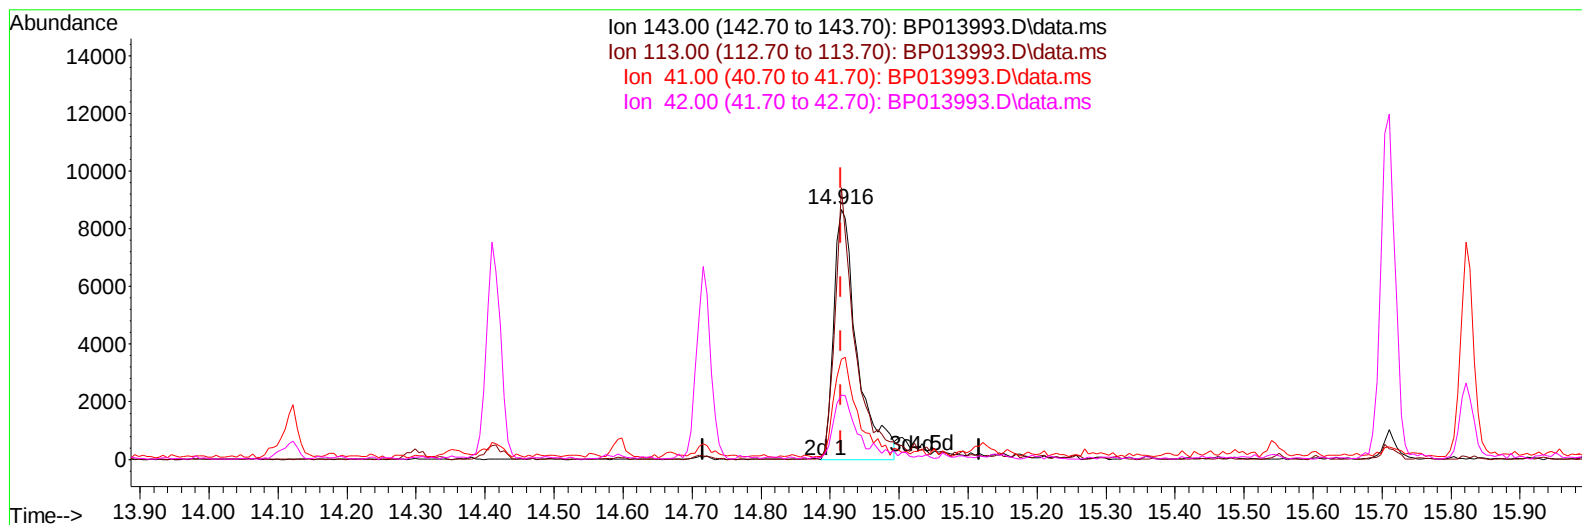

TIC: BP013993.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (-0.000) 4.79 ng/ul m

response 20542

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	108.61
41.00	40.20	40.08
42.00	28.50	25.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013993.D
 Acq On : 09 Mar 2023 00:01
 Operator : CG/JU
 Sample : 01729-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BY2

Manual IntegrationsAPPROVED

Quant Time: Mar 09 02:26:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	107296	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	430294	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	287017	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.475	188	774585	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	952999	20.000	ng/ul	-0.01
88) Perylene-d12	24.086	264	1078583	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	12877	4.534	ng/uL	0.00
4) Pyridine-d5	3.881	84	44536	5.664	ng/ul	0.01
7) Phenol-d5	7.234	99	52482	5.543	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	158055	28.622	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	155866	21.606	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	100296	12.968	ng/ul	0.00
21) Nitrobenzene-d5	9.252	128	102141	29.750	ng/ul	0.00
24) 2-Nitrophenol-d4	9.981	143	118071	28.729	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	198245	25.636	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	210992	20.617	ng/ul	0.00
46) Dimethylphthalate-d6	14.122	166	769112	31.575	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	795508	30.829	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	20542m	4.786	ng/ul	0.00
60) Fluorene-d10	15.710	176	677152	32.802	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.828	200	148527	25.370	ng/ul	0.00
73) Anthracene-d10	17.569	188	1216524	32.352	ng/ul	0.00
81) Pyrene-d10	19.792	212	1663973	31.658	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	1919753	33.461	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013993.D
Acq On : 09 Mar 2023 00:01
Operator : CG/JU
Sample : 01729-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 02:26:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

