




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014002.D
Acq On : 09 Mar 2023 10:22
Operator : CG/JU
Sample : 01713-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBZZ0

Manual IntegrationsAPPROVED

Quant Time: Mar 10 00:16:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

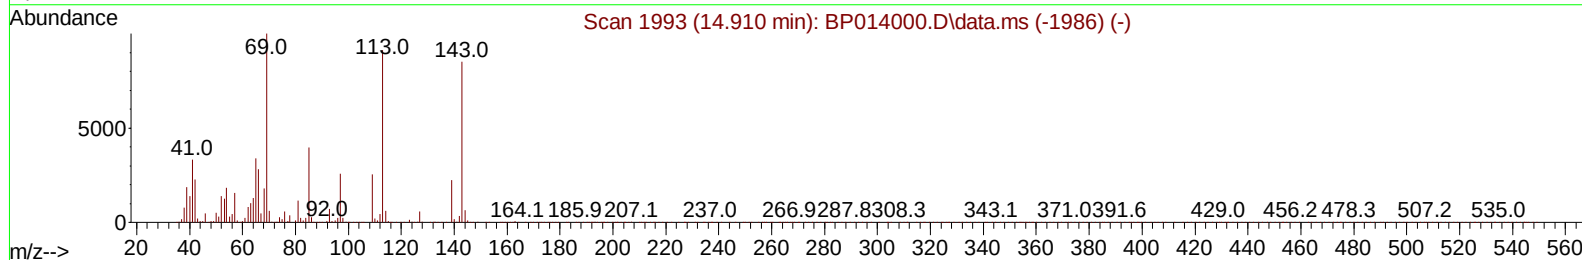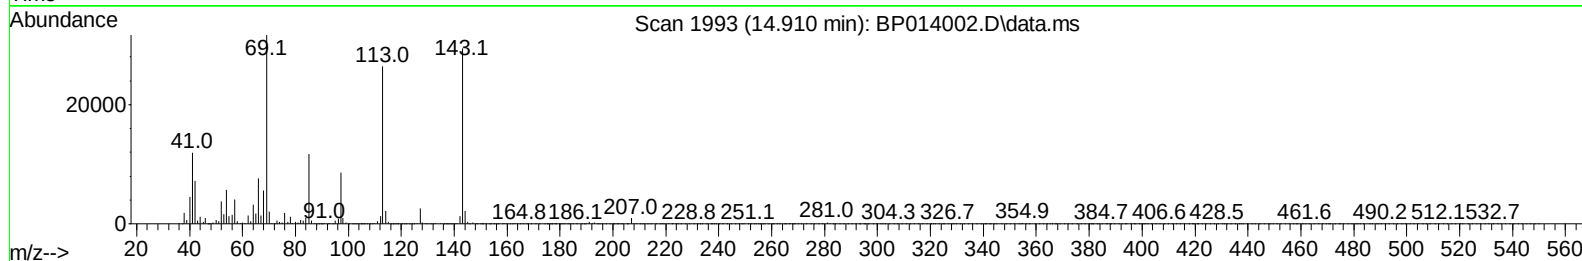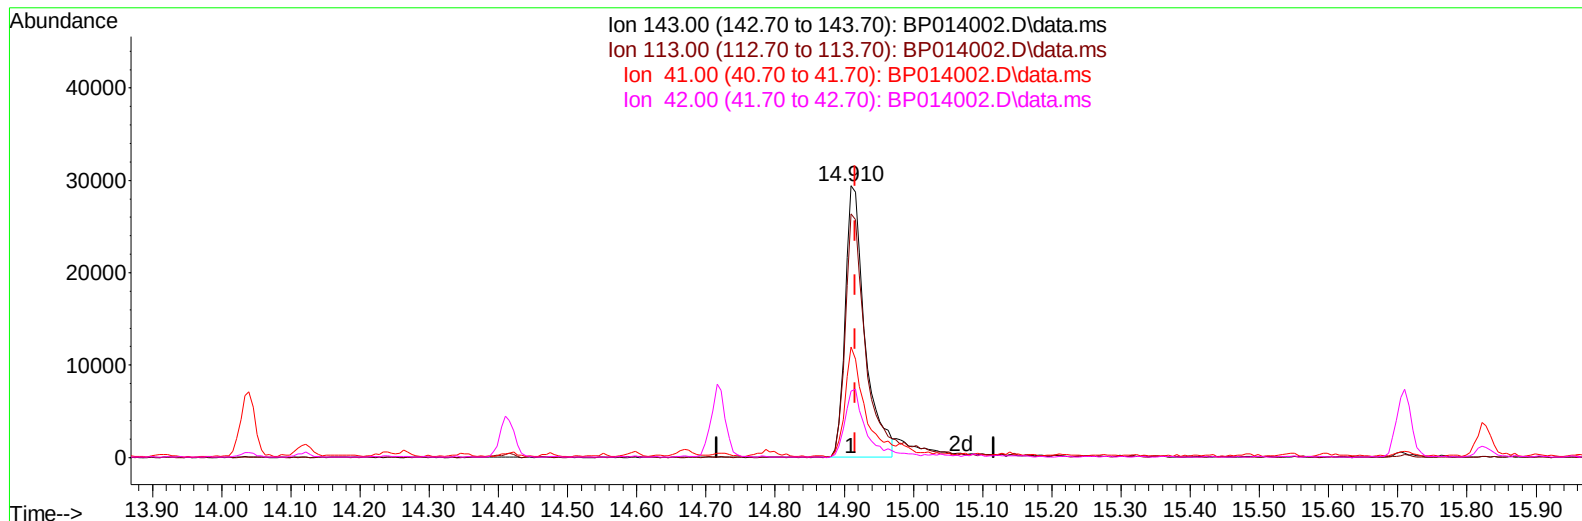

TIC: BP014002.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (-0.006) 10.86 ng/ul

response 58109

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	89.74
41.00	40.20	40.69
42.00	28.50	24.36




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014002.D
Acq On : 09 Mar 2023 10:22
Operator : CG/JU
Sample : 01713-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBZZ0

Manual IntegrationsAPPROVED

Quant Time: Mar 10 00:16:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

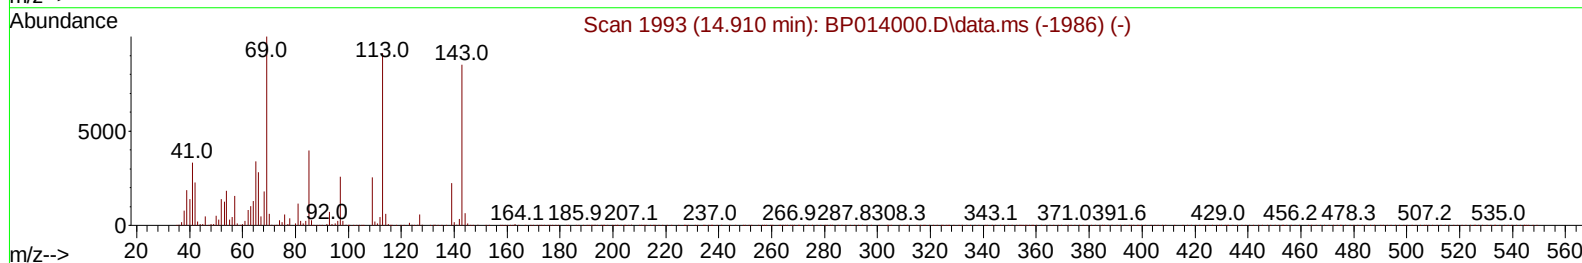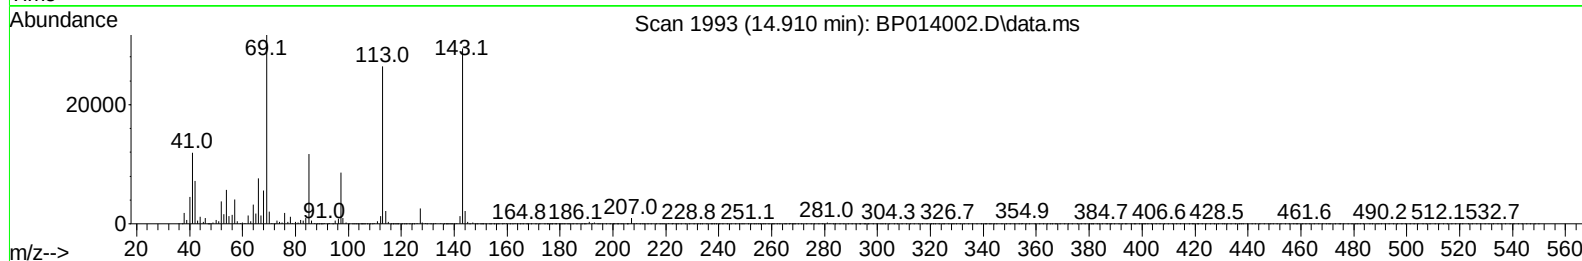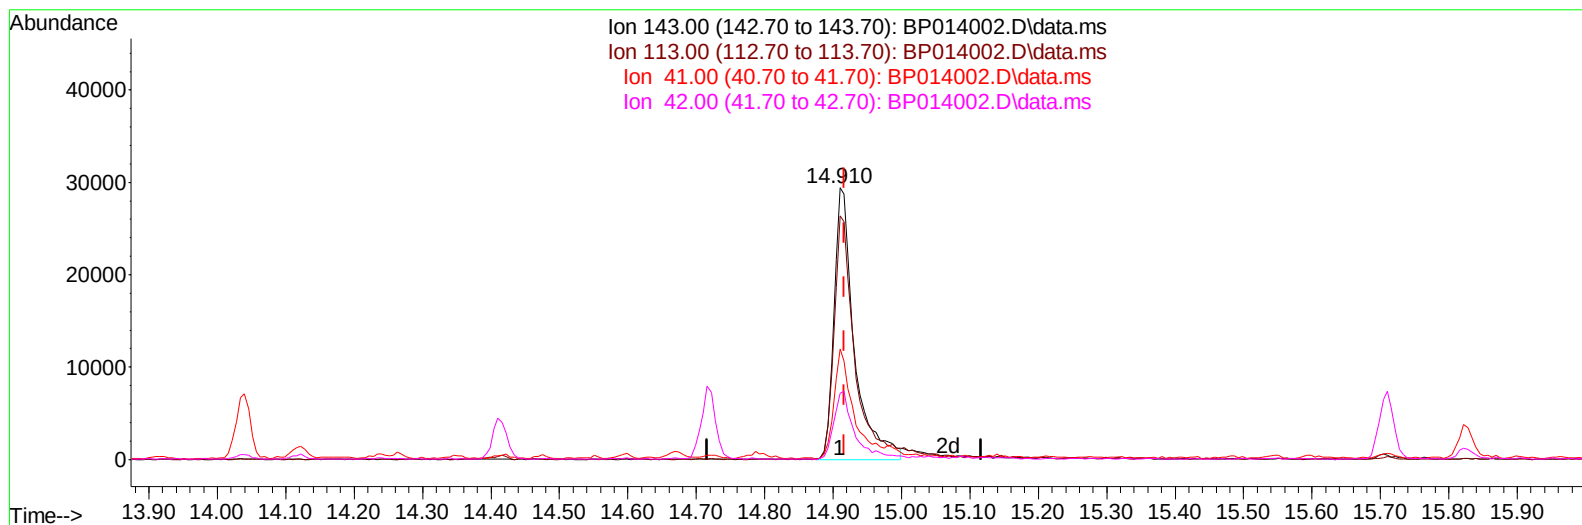

TIC: BP014002.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (-0.006) 11.41 ng/ul m

response 61025

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	89.74
41.00	40.20	40.69
42.00	28.50	24.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014002.D
 Acq On : 09 Mar 2023 10:22
 Operator : CG/JU
 Sample : 01713-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBZZ0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 00:16:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	121412	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	486033	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	357702	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.475	188	880186	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1034715	20.000	ng/ul	0.00
88) Perylene-d12	24.092	264	1081632	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.440	96	9700	3.019	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.228	99	154602	14.430	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	97030	15.528	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	121488	14.883	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	100475	11.480	ng/ul	0.00
21) Nitrobenzene-d5	9.252	128	60872	15.697	ng/ul	0.00
24) 2-Nitrophenol-d4	9.981	143	70665	15.222	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	125405	14.357	ng/ul	0.00
31) 4-Chloroaniline-d4	11.046	131	124382	10.760	ng/ul	0.00
46) Dimethylphthalate-d6	14.122	166	478874	15.775	ng/ul	0.00
49) Acenaphthylene-d8	14.416	160	497201	15.461	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	61025m	11.407	ng/ul	0.00
60) Fluorene-d10	15.710	176	418506	16.267	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.828	200	75781	11.391	ng/ul	0.00
73) Anthracene-d10	17.575	188	650372	15.221	ng/ul	0.00
81) Pyrene-d10	19.792	212	973805	17.064	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	964736	16.768	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014002.D
Acq On : 09 Mar 2023 10:22
Operator : CG/JU
Sample : 01713-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBZZ0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 00:16:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

