

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013971.D
 Acq On : 08 Mar 2023 09:58
 Operator : CG/JU
 Sample : PB151237BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	39	43	53	rVB	26358	40185	1.08%	0.117%
2	3.869	113	116	140	rBV	303468	526151	14.17%	1.533%
3	4.205	169	173	180	rVB	7839	11990	0.32%	0.035%
4	7.234	679	688	702	rBV	382967	648235	17.46%	1.889%
5	7.404	710	717	728	rBV	310531	485138	13.07%	1.414%
6	7.610	744	752	766	rBV	388273	641757	17.29%	1.870%
7	8.081	824	832	844	rBV	469504	763202	20.56%	2.224%
8	8.787	943	952	969	rBV	459889	800504	21.56%	2.333%
9	9.257	1024	1032	1047	rBV	380534	642819	17.32%	1.873%
10	9.981	1147	1155	1171	rBV	336907	572861	15.43%	1.669%
11	10.522	1239	1247	1265	rBV	464027	830978	22.38%	2.422%
12	10.904	1305	1312	1323	rBV	632644	1082142	29.15%	3.153%
13	11.045	1328	1336	1354	rBV	456326	839989	22.63%	2.448%
14	12.498	1577	1583	1588	rBV4	6545	13814	0.37%	0.040%
15	13.604	1767	1771	1778	rVB9	3620	6293	0.17%	0.018%
16	14.122	1853	1859	1873	rBV	1118171	1550988	41.78%	4.520%
17	14.416	1902	1909	1921	rBV	1105123	1612968	43.45%	4.700%
18	14.722	1954	1961	1970	rBV	1092491	1649241	44.43%	4.806%
19	14.910	1987	1993	2014	rBV	370673	709854	19.12%	2.069%
20	15.128	2027	2030	2036	rVB7	3739	6075	0.16%	0.018%
21	15.710	2121	2129	2143	rBV	1506447	2190359	59.00%	6.383%
22	15.828	2143	2149	2166	rVV	553791	808716	21.79%	2.357%
23	15.951	2167	2170	2178	rVB5	8466	15839	0.43%	0.046%
24	17.263	2390	2393	2399	rVB3	3540	5223	0.14%	0.015%
25	17.474	2422	2429	2439	rBV	1600552	2257298	60.81%	6.578%
26	17.574	2439	2446	2459	rVV	1785956	2536540	68.33%	7.392%
27	19.374	2748	2752	2758	rBV4	25115	33445	0.90%	0.097%
28	19.439	2760	2763	2767	rBV	20136	28240	0.76%	0.082%
29	19.798	2818	2824	2836	rBV	2493191	3239293	87.26%	9.439%
30	21.551	3117	3122	3132	rBV	2058534	2939699	79.19%	8.566%
31	23.927	3519	3526	3540	rVB2	1825419	3712210	100.00%	10.818%
32	24.092	3547	3554	3566	rVB2	1426408	3114398	83.90%	9.076%




Sum of corrected areas: 34316444

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013971.D
Acq On : 08 Mar 2023 09:58
Operator : CG/JU
Sample : PB151237BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK237

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

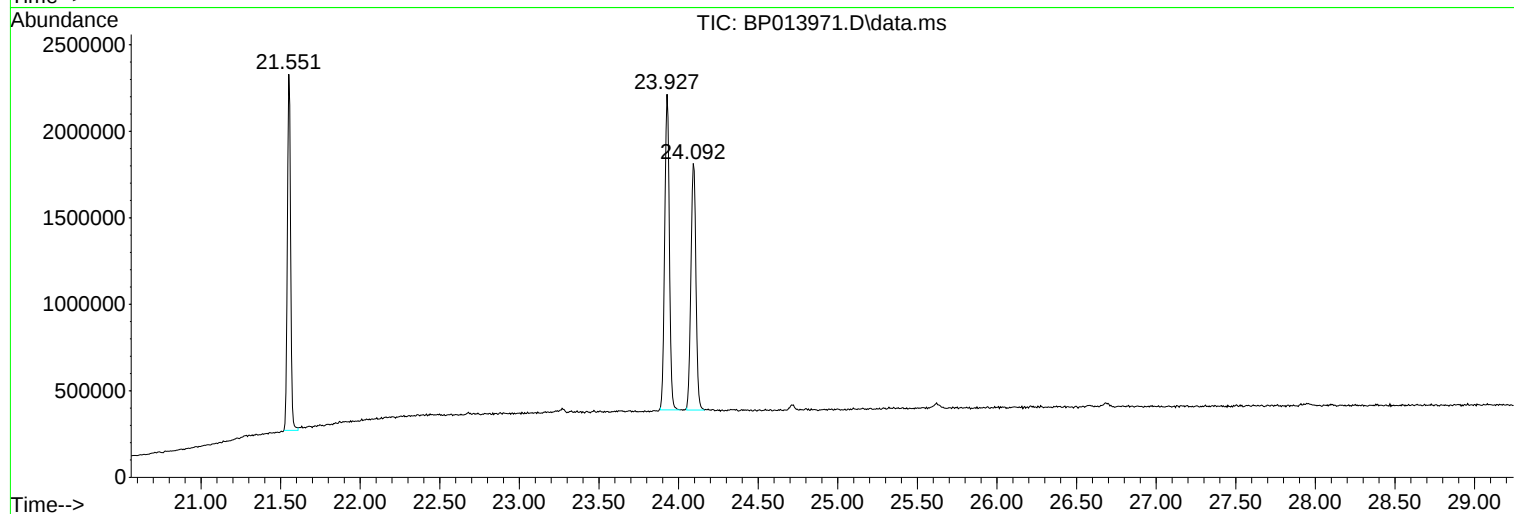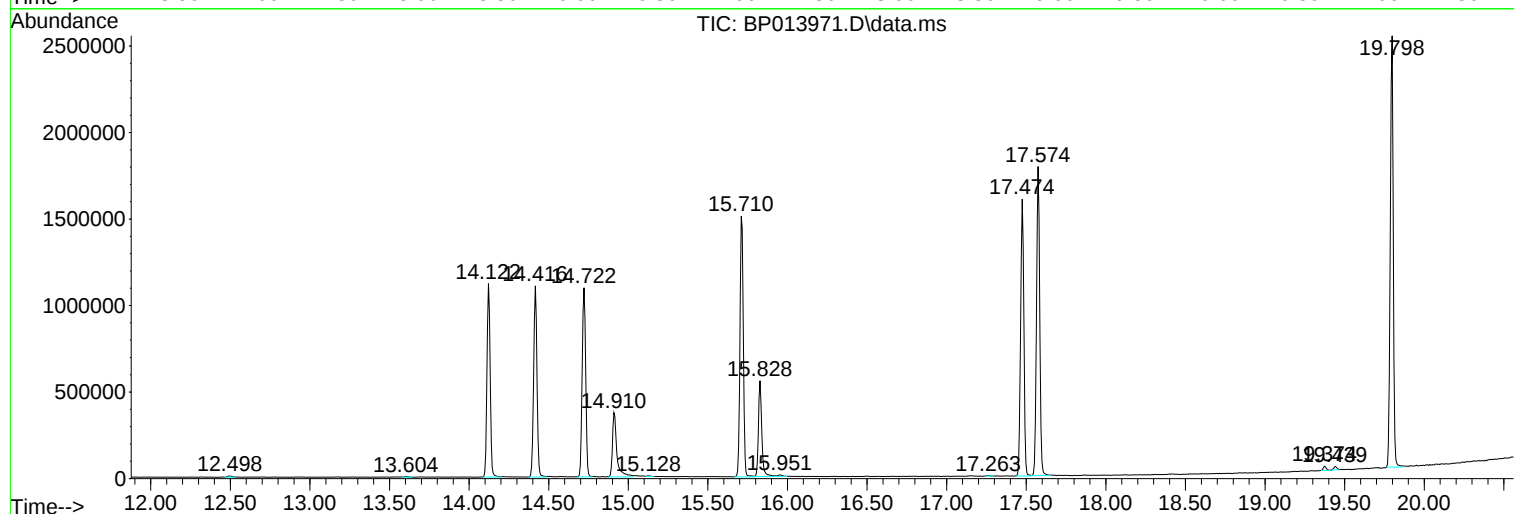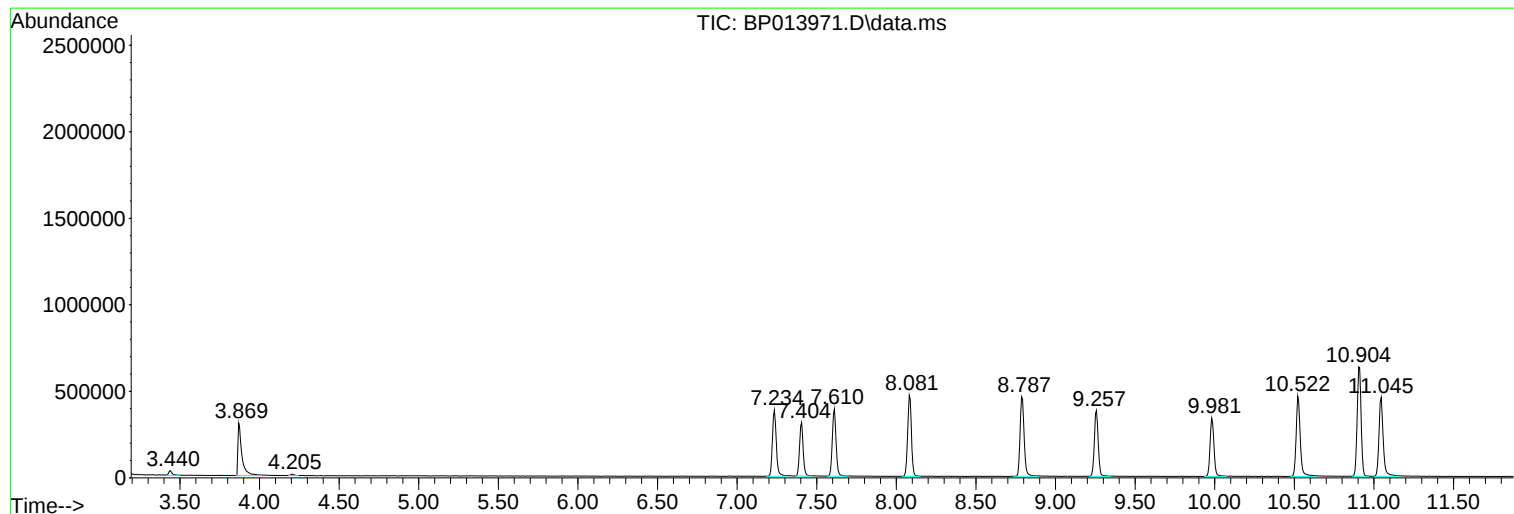

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013971.D
Acq On : 08 Mar 2023 09:58
Operator : CG/JU
Sample : PB151237BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK237

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013971.D
Acq On : 08 Mar 2023 09:58
Operator : CG/JU
Sample : PB151237BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK237

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc