

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013983.D
 Acq On : 08 Mar 2023 18:19
 Operator : CG/JU
 Sample : PB151191BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	39	42	49	rBV	29019	40802	0.98%	0.113%
2	3.869	114	116	134	rBV	362858	590965	14.22%	1.630%
3	4.205	169	173	180	rVB2	7491	11842	0.29%	0.033%
4	7.234	681	688	701	rBV	437764	730237	17.58%	2.015%
5	7.404	710	717	729	rVB	347520	548122	13.19%	1.512%
6	7.610	745	752	767	rBV	484763	771371	18.57%	2.128%
7	8.081	823	832	847	rVB	423448	684726	16.48%	1.889%
8	8.793	944	953	967	rBV	548768	941666	22.66%	2.598%
9	9.257	1024	1032	1043	rBV	445874	745800	17.95%	2.058%
10	9.981	1148	1155	1164	rBV	392407	666246	16.04%	1.838%
11	10.522	1239	1247	1265	rBV	560564	977328	23.52%	2.696%
12	10.904	1304	1312	1323	rBV	570590	971376	23.38%	2.680%
13	11.045	1328	1336	1354	rBV	540993	987889	23.78%	2.725%
14	12.492	1575	1582	1588	rBV4	8378	18281	0.44%	0.050%
15	14.122	1851	1859	1871	rBV	1347086	1796215	43.23%	4.955%
16	14.416	1901	1909	1923	rBV	1294804	1897653	45.67%	5.235%
17	14.722	1954	1961	1974	rVB	1038975	1544830	37.18%	4.262%
18	14.910	1986	1993	2011	rBV	490632	895375	21.55%	2.470%
19	15.128	2028	2030	2035	rVB5	4695	5256	0.13%	0.015%
20	15.710	2121	2129	2139	rBV	1819474	2569505	61.84%	7.089%
21	15.827	2143	2149	2164	rVV	635337	928196	22.34%	2.561%
22	15.951	2167	2170	2178	rVB4	10216	18063	0.43%	0.050%
23	17.474	2422	2429	2439	rBV	1450938	2032847	48.93%	5.608%
24	17.574	2439	2446	2458	rBV	1979601	2827429	68.05%	7.800%
25	19.374	2748	2752	2758	rBV2	28168	39472	0.95%	0.109%
26	19.439	2760	2763	2767	rVB	21337	29722	0.72%	0.082%
27	19.798	2817	2824	2837	rBV	2583878	3554871	85.56%	9.807%
28	21.551	3117	3122	3131	rBV	1890034	2540597	61.15%	7.009%
29	23.927	3518	3526	3538	rBV	2012696	4154786	100.00%	11.462%
30	24.092	3547	3554	3565	rVB	1295116	2725949	65.61%	7.520%




Sum of corrected areas: 36247417

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013983.D
Acq On : 08 Mar 2023 18:19
Operator : CG/JU
Sample : PB151191BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

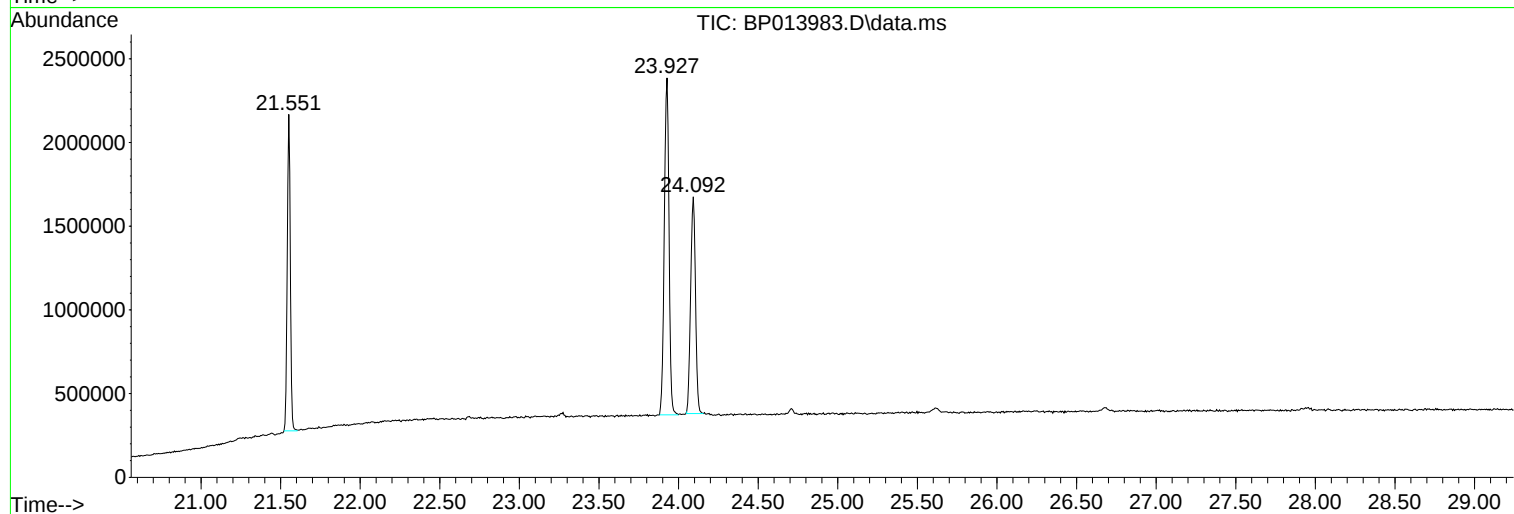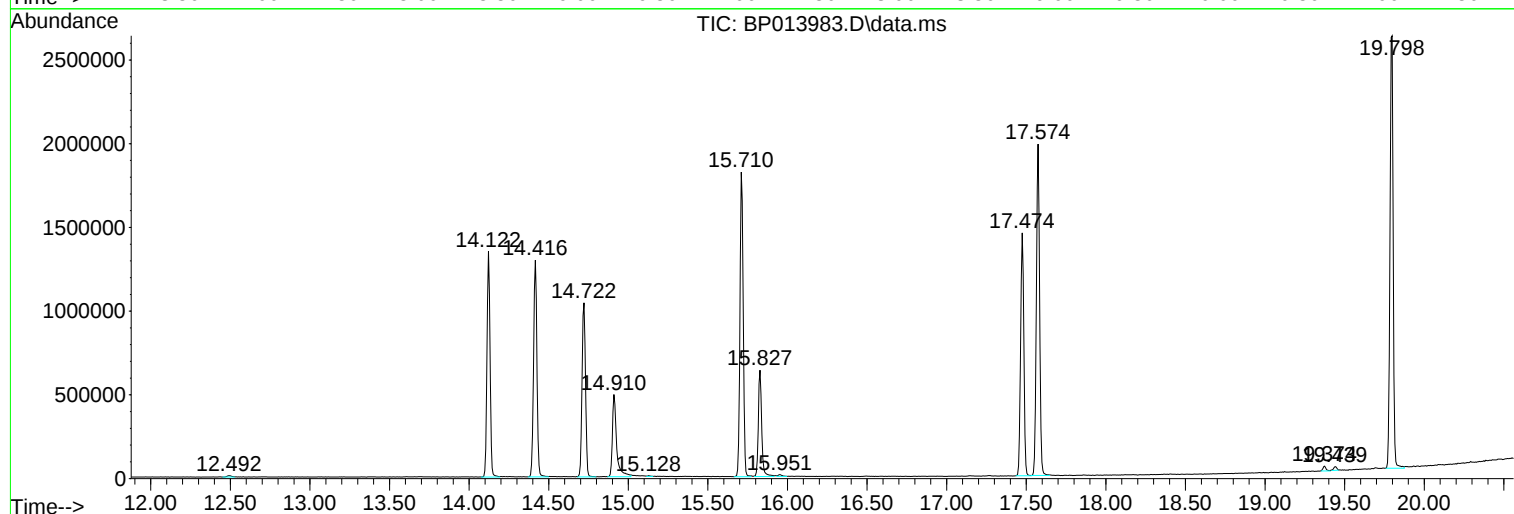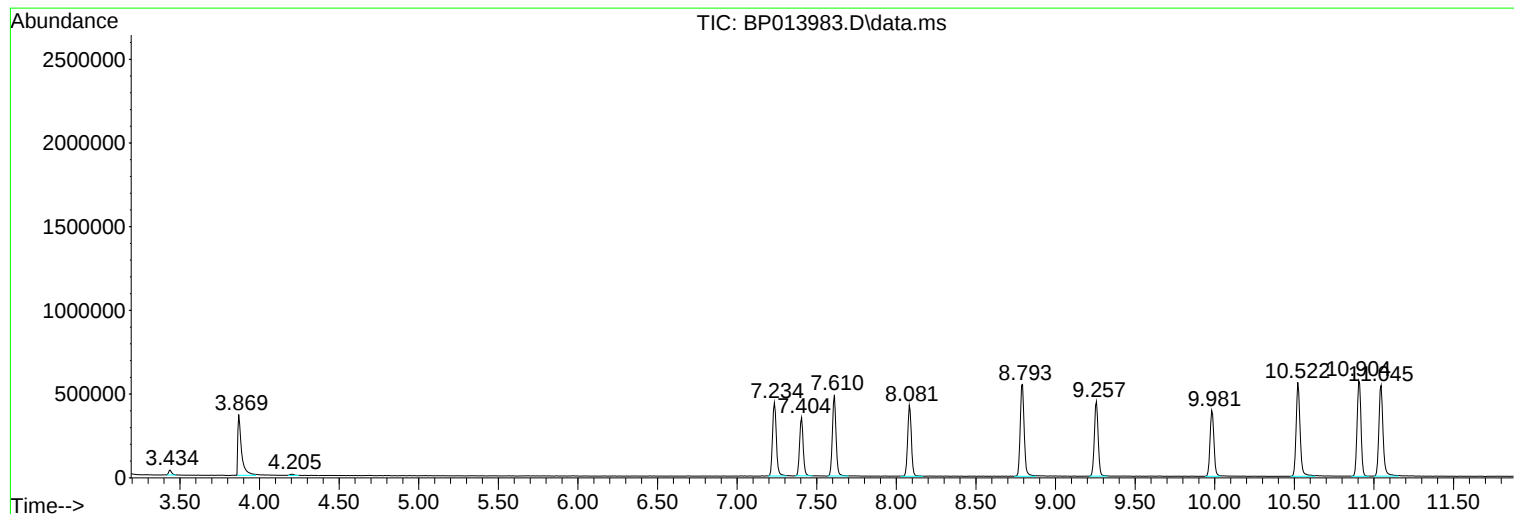

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013983.D
Acq On : 08 Mar 2023 18:19
Operator : CG/JU
Sample : PB151191BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013983.D
Acq On : 08 Mar 2023 18:19
Operator : CG/JU
Sample : PB151191BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc