

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013984.D
 Acq On : 08 Mar 2023 18:53
 Operator : CG/JU
 Sample : PB151193BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	38	43	50	rVB	30891	45686	0.99%	0.120%
2	3.869	114	116	132	rBV	396516	629440	13.58%	1.656%
3	4.205	170	173	178	rVB2	7074	10192	0.22%	0.027%
4	7.234	680	688	701	rBV	509313	833369	17.98%	2.193%
5	7.405	710	717	726	rBV	405174	627655	13.54%	1.651%
6	7.610	745	752	762	rBV	513122	828084	17.86%	2.179%
7	8.081	823	832	840	rBV	383038	628884	13.57%	1.655%
8	8.787	945	952	969	rBV	642039	1084627	23.40%	2.854%
9	9.257	1023	1032	1047	rBV	505205	855038	18.44%	2.250%
10	9.981	1146	1155	1169	rBV	448463	748006	16.14%	1.968%
11	10.522	1239	1247	1269	rBV	627445	1096450	23.65%	2.885%
12	10.904	1300	1312	1322	rBV	511243	873731	18.85%	2.299%
13	11.040	1328	1335	1351	rBV	593373	1105161	23.84%	2.908%
14	12.498	1575	1583	1587	rBV2	9237	18207	0.39%	0.048%
15	13.604	1764	1771	1777	rBV10	2565	5575	0.12%	0.015%
16	14.122	1851	1859	1873	rBV	1448807	2006076	43.27%	5.278%
17	14.416	1900	1909	1924	rBV	1470627	2109654	45.51%	5.551%
18	14.722	1953	1961	1970	rBV	888537	1320417	28.48%	3.474%
19	14.910	1987	1993	2016	rBV	586355	1013421	21.86%	2.666%
20	15.710	2122	2129	2142	rBV	1912355	2705898	58.37%	7.120%
21	15.828	2142	2149	2165	rVV	759388	1070490	23.09%	2.817%
22	15.951	2167	2170	2176	rVB5	9832	15815	0.34%	0.042%
23	17.475	2422	2429	2439	rBV	1279390	1807195	38.98%	4.755%
24	17.575	2439	2446	2463	rVV	2271907	3207949	69.20%	8.441%
25	19.374	2748	2752	2757	rBV3	32164	42216	0.91%	0.111%
26	19.439	2760	2763	2768	rVB	26501	37012	0.80%	0.097%
27	19.798	2818	2824	2831	rBV	2976499	3972922	85.70%	10.453%
28	21.551	3117	3122	3130	rBV	1719333	2243802	48.40%	5.904%
29	23.927	3518	3526	3535	rBV2	2281779	4635794	100.00%	12.197%
30	24.092	3547	3554	3567	rVB2	1161591	2427508	52.36%	6.387%




Sum of corrected areas: 38006274

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013984.D
Acq On : 08 Mar 2023 18:53
Operator : CG/JU
Sample : PB151193BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

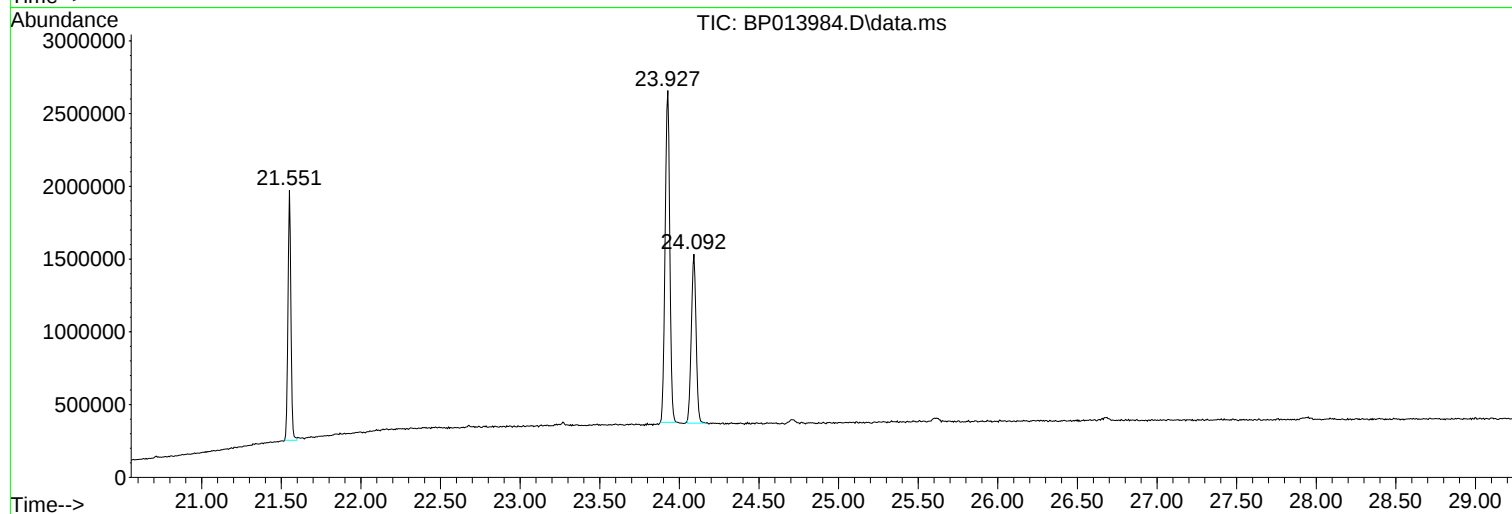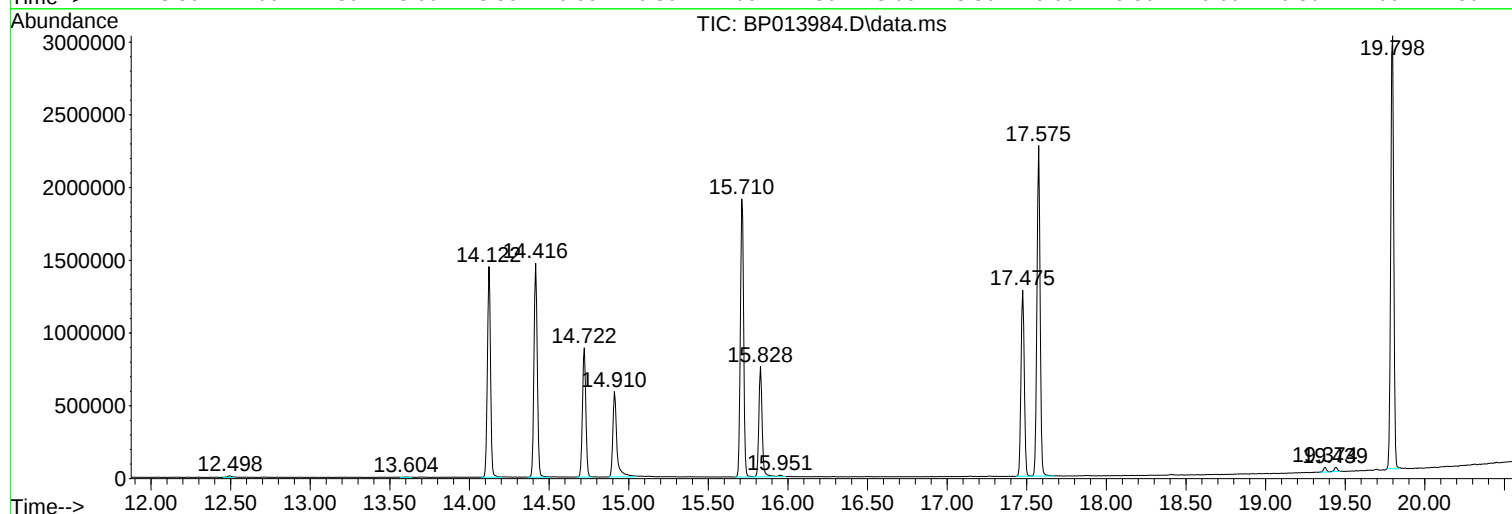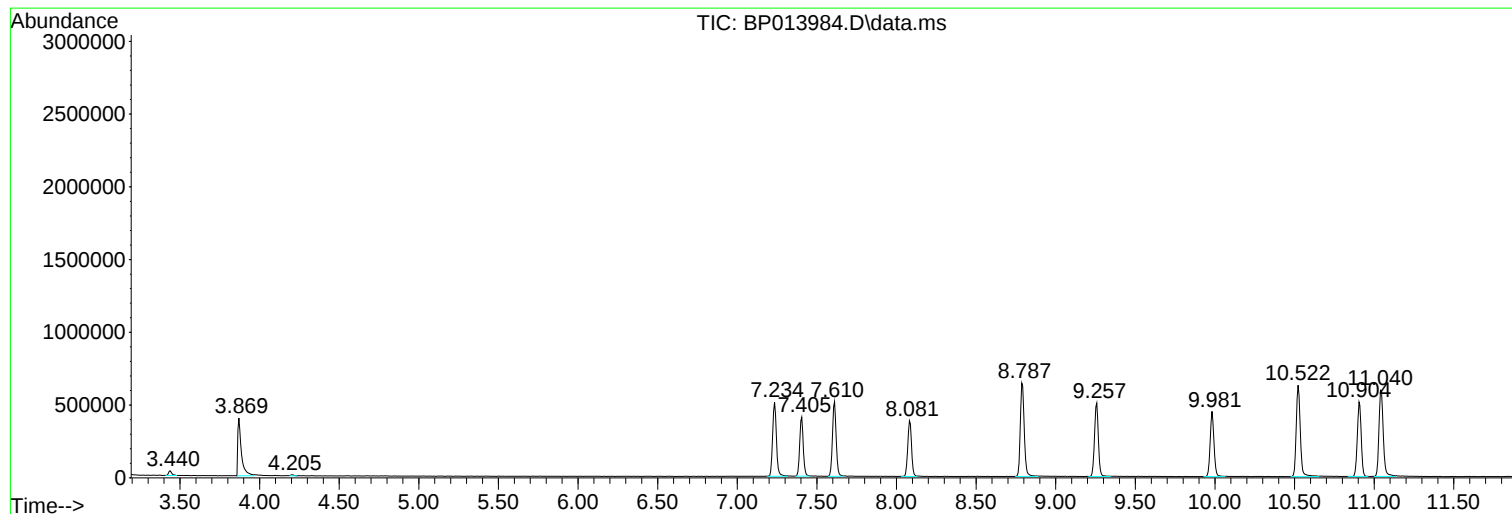

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013984.D
Acq On : 08 Mar 2023 18:53
Operator : CG/JU
Sample : PB151193BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013984.D
Acq On : 08 Mar 2023 18:53
Operator : CG/JU
Sample : PB151193BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc