

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013985.D
 Acq On : 08 Mar 2023 19:28
 Operator : CG/JU
 Sample : PB151254BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	50	rVB	29578	40470	0.99%	0.121%
2	3.869	113	116	135	rBV	355158	577883	14.13%	1.731%
3	4.199	168	172	178	rVB	7341	11887	0.29%	0.036%
4	7.234	681	688	698	rBV	428671	699721	17.11%	2.097%
5	7.405	710	717	728	rBV	316206	516328	12.63%	1.547%
6	7.610	745	752	763	rBV	435801	709158	17.34%	2.125%
7	8.081	825	832	843	rBV	357142	572517	14.00%	1.715%
8	8.793	945	953	966	rBV	516537	892223	21.82%	2.673%
9	9.257	1024	1032	1047	rBV	421913	714681	17.48%	2.141%
10	9.981	1148	1155	1165	rBV	383320	637114	15.58%	1.909%
11	10.522	1238	1247	1269	rBV	531584	941023	23.01%	2.820%
12	10.904	1304	1312	1321	rBV	477021	818998	20.03%	2.454%
13	11.040	1328	1335	1352	rBV	509324	938604	22.95%	2.812%
14	12.493	1576	1582	1594	rVB2	8066	16592	0.41%	0.050%
15	14.122	1852	1859	1871	rBV	1235028	1680696	41.10%	5.036%
16	14.416	1901	1909	1922	rBV	1208401	1755185	42.92%	5.259%
17	14.722	1953	1961	1971	rBV	840439	1242487	30.38%	3.723%
18	14.910	1987	1993	2018	rBV	444709	829514	20.28%	2.485%
19	15.710	2122	2129	2142	rBV	1590711	2294527	56.11%	6.875%
20	15.828	2142	2149	2165	rVV	595672	853033	20.86%	2.556%
21	15.951	2166	2170	2179	rVB4	10404	17586	0.43%	0.053%
22	17.151	2369	2374	2379	rBV7	3791	6560	0.16%	0.020%
23	17.263	2390	2393	2399	rBV7	2832	4591	0.11%	0.014%
24	17.475	2422	2429	2438	rBV	1188472	1698447	41.53%	5.089%
25	17.575	2439	2446	2458	rVV	1864291	2696293	65.93%	8.079%
26	18.122	2535	2539	2542	rBV6	3181	5306	0.13%	0.016%
27	19.369	2748	2751	2756	rBV3	24819	32557	0.80%	0.098%
28	19.439	2760	2763	2768	rVB2	23527	31523	0.77%	0.094%
29	19.792	2817	2823	2831	rBV	2674818	3455933	84.51%	10.355%
30	21.551	3117	3122	3130	rBV	1614896	2188376	53.51%	6.557%
31	23.927	3518	3526	3537	rVB2	1960884	4089581	100.00%	12.253%
32	24.092	3547	3554	3564	rVB2	1134819	2405742	58.83%	7.208%




Sum of corrected areas: 33375136

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013985.D
Acq On : 08 Mar 2023 19:28
Operator : CG/JU
Sample : PB151254BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

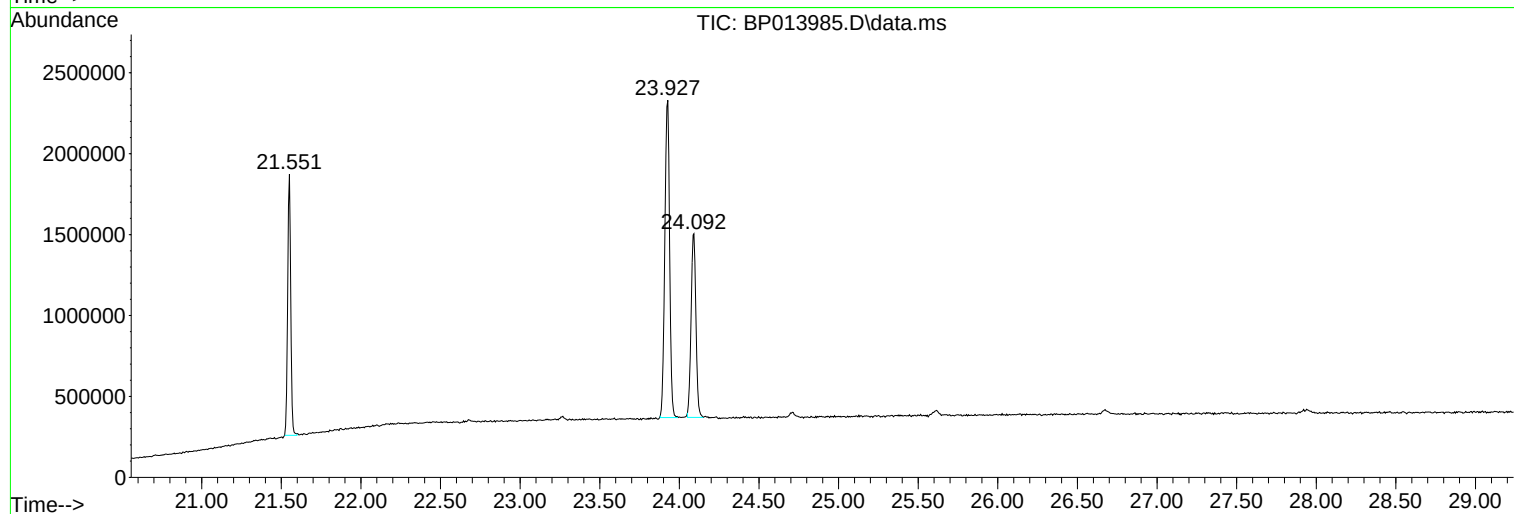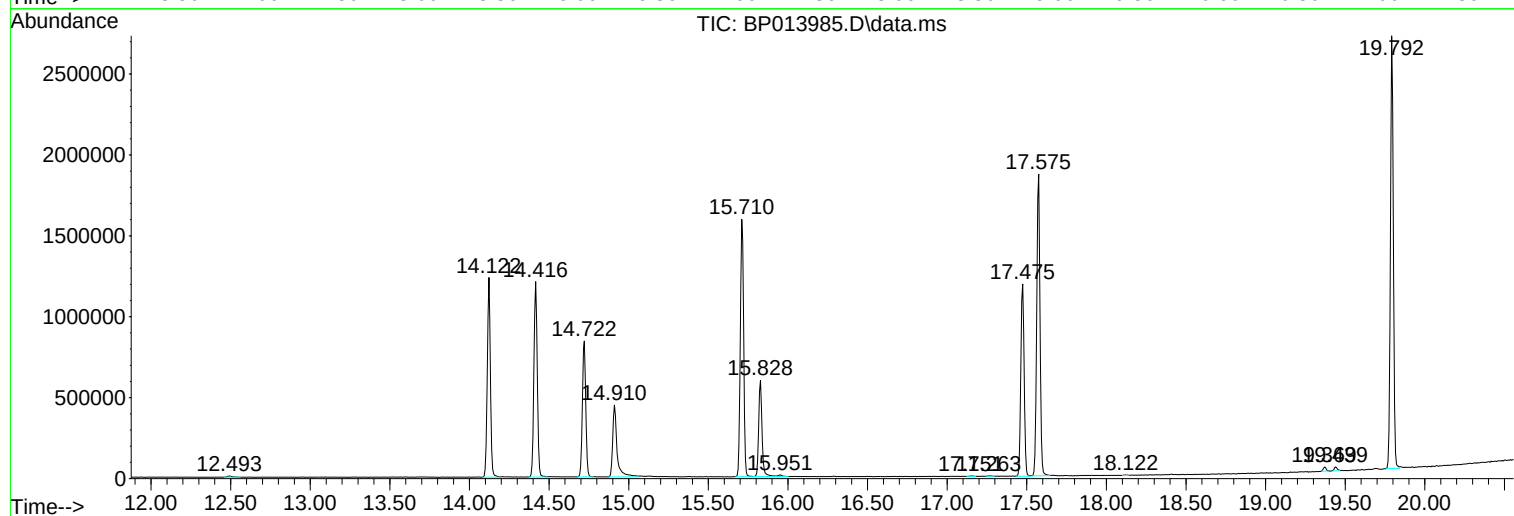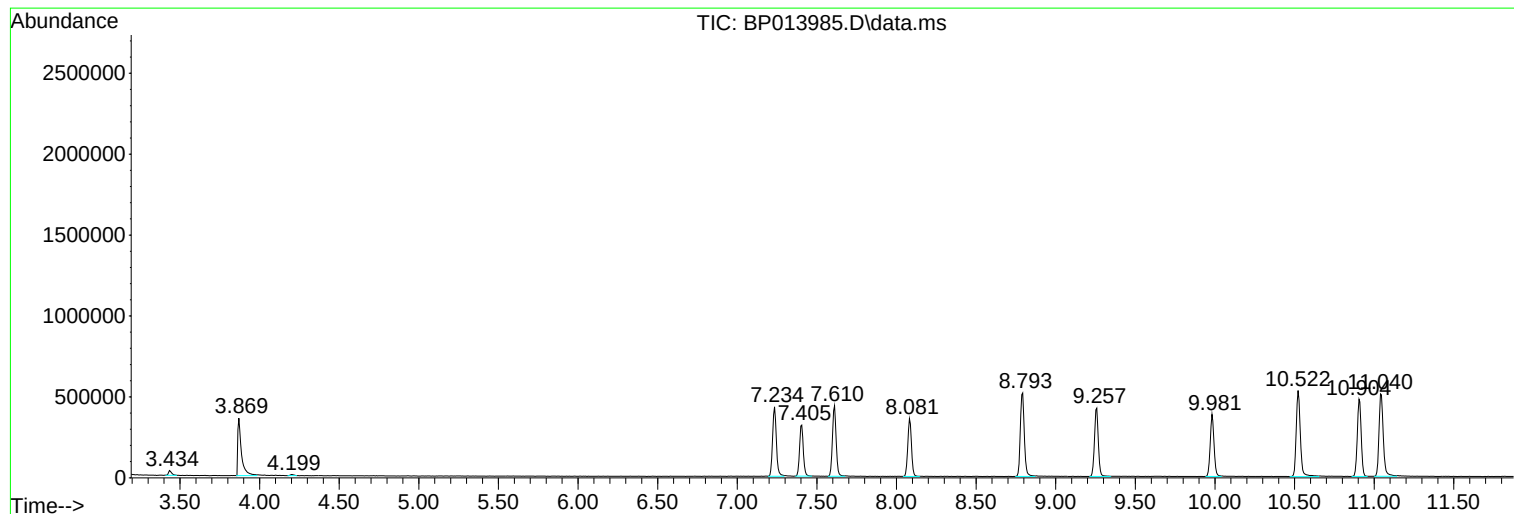

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013985.D
Acq On : 08 Mar 2023 19:28
Operator : CG/JU
Sample : PB151254BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013985.D
Acq On : 08 Mar 2023 19:28
Operator : CG/JU
Sample : PB151254BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc