

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013995.D
 Acq On : 09 Mar 2023 01:09
 Operator : CG/JU
 Sample : 01729-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	52	rVB	27609	42633	0.74%	0.107%
2	3.875	115	117	130	rBV	136469	238121	4.14%	0.597%
3	4.099	150	155	160	rBV	15141	22539	0.39%	0.057%
4	4.205	168	173	177	rBV2	8438	12524	0.22%	0.031%
5	4.305	187	190	196	rVB6	8405	12099	0.21%	0.030%
6	4.658	245	250	252	rBV2	3526	6178	0.11%	0.015%
7	5.140	328	332	337	rBV	8998	14835	0.26%	0.037%
8	5.752	431	436	440	rVB8	3456	6531	0.11%	0.016%
9	6.452	549	555	561	rBV5	7760	13302	0.23%	0.033%
10	7.181	675	679	681	rBV5	4038	5839	0.10%	0.015%
11	7.234	682	688	697	rVV	99034	176737	3.07%	0.443%
12	7.399	709	716	725	rBV	397510	633014	10.99%	1.587%
13	7.605	745	751	762	rBV	395781	658151	11.43%	1.650%
14	7.681	762	764	770	rVB7	3782	5988	0.10%	0.015%
15	8.081	824	832	845	rBV	457438	733548	12.74%	1.840%
16	8.787	945	952	964	rBV	308223	530292	9.21%	1.330%
17	9.252	1024	1031	1043	rBV	520095	874685	15.19%	2.193%
18	9.640	1094	1097	1102	rBV6	3753	6180	0.11%	0.015%
19	9.981	1147	1155	1166	rBV	383980	650989	11.30%	1.632%
20	10.522	1239	1247	1264	rBV	584460	1041267	18.08%	2.611%
21	10.904	1304	1312	1323	rVB	631725	1035989	17.99%	2.598%
22	11.040	1327	1335	1353	rBV	559636	1031692	17.92%	2.587%
23	12.140	1515	1522	1527	rVB5	6614	10674	0.19%	0.027%
24	12.487	1573	1581	1587	rBV3	10245	19087	0.33%	0.048%
25	13.693	1778	1786	1790	rBV10	3753	7685	0.13%	0.019%
26	14.122	1852	1859	1872	rBV	1513979	2053848	35.67%	5.150%
27	14.416	1901	1909	1920	rBV	1421453	2116031	36.75%	5.306%
28	14.716	1952	1960	1969	rBV	1000627	1484147	25.77%	3.722%
29	14.916	1989	1994	2009	rBV2	64176	163508	2.84%	0.410%
30	15.134	2026	2031	2039	rVB2	5589	11657	0.20%	0.029%
31	15.710	2122	2129	2140	rVV	2109546	2942871	51.11%	7.380%
32	15.822	2142	2148	2164	rVV	606602	901389	15.65%	2.260%
33	15.951	2166	2170	2175	rVB5	11377	17917	0.31%	0.045%
34	16.204	2209	2213	2220	rBV4	14420	22911	0.40%	0.057%
35	16.410	2242	2248	2250	rBV7	5798	9031	0.16%	0.023%
36	17.139	2369	2372	2376	rVB6	3913	6218	0.11%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013995.D
 Acq On : 09 Mar 2023 01:09
 Operator : CG/JU
 Sample : 01729-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	17.210	2380	2384	2387	rVV5	5007	6479	0.11%	0.016%
38	17.257	2389	2392	2399	rVV7	4361	9357	0.16%	0.023%
39	17.475	2422	2429	2437	rBV	1402861	2060007	35.77%	5.166%
40	17.569	2439	2445	2455	rVV	2498814	3621516	62.89%	9.082%
41	17.657	2457	2460	2467	rVB8	16463	25595	0.44%	0.064%
42	17.939	2505	2508	2513	rBV7	4560	6586	0.11%	0.017%
43	18.116	2535	2538	2542	rVB6	9643	12661	0.22%	0.032%
44	18.328	2571	2574	2584	rBV7	30624	54279	0.94%	0.136%
45	18.398	2584	2586	2591	rVB3	4481	5802	0.10%	0.015%
46	18.604	2619	2621	2625	rVB5	6435	7661	0.13%	0.019%
47	19.210	2721	2724	2726	rBV4	9750	11677	0.20%	0.029%
48	19.369	2747	2751	2756	rBV4	40002	56569	0.98%	0.142%
49	19.439	2758	2763	2769	rBV	39355	68450	1.19%	0.172%
50	19.557	2780	2783	2793	rBV10	21708	41795	0.73%	0.105%
51	19.692	2803	2806	2810	rBV5	15970	19140	0.33%	0.048%
52	19.792	2817	2823	2834	rBV	3598470	4745173	82.40%	11.899%
53	20.727	2979	2982	2986	rVB	54575	54925	0.95%	0.138%
54	21.545	3116	3121	3129	rBV	2062862	2813694	48.86%	7.056%
55	23.921	3517	3525	3538	rVB2	2819071	5758475	100.00%	14.440%
56	24.086	3546	3553	3563	rVB2	1425301	2977344	51.70%	7.466%




Sum of corrected areas: 39877292

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013995.D
Acq On : 09 Mar 2023 01:09
Operator : CG/JU
Sample : 01729-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

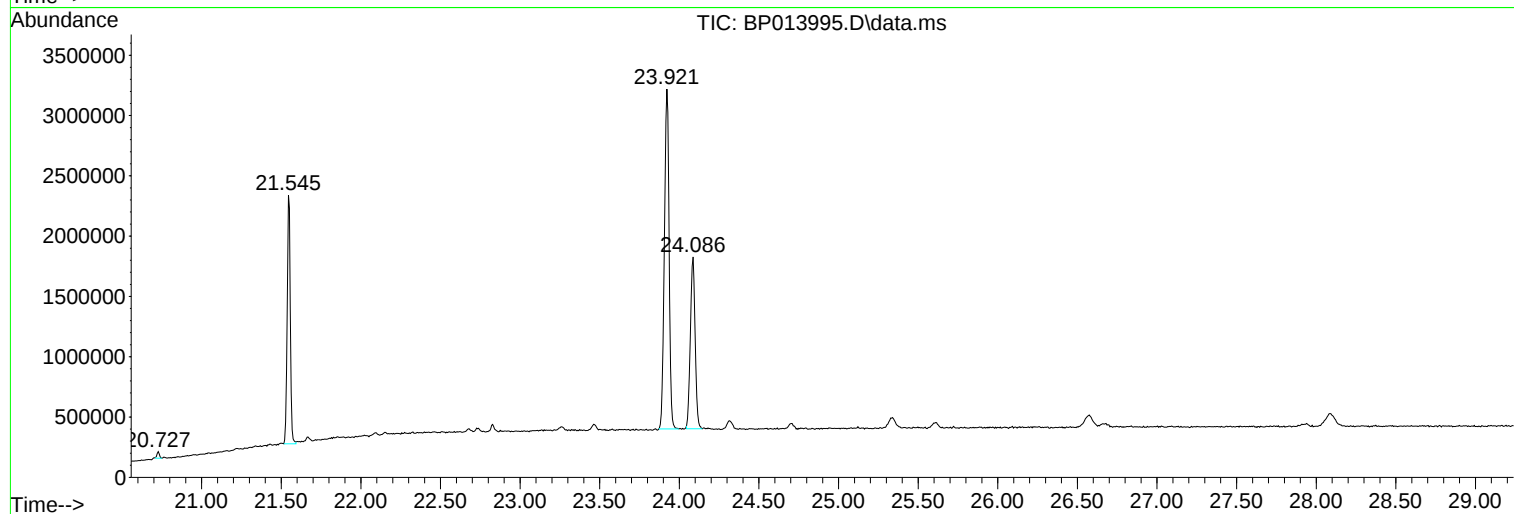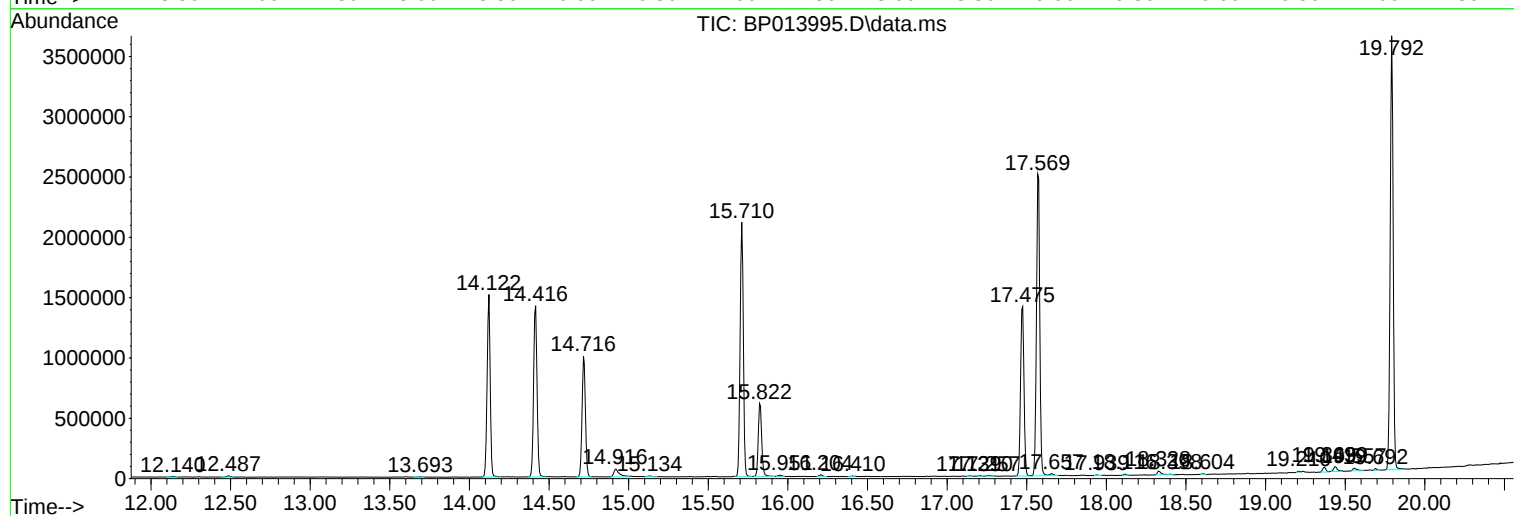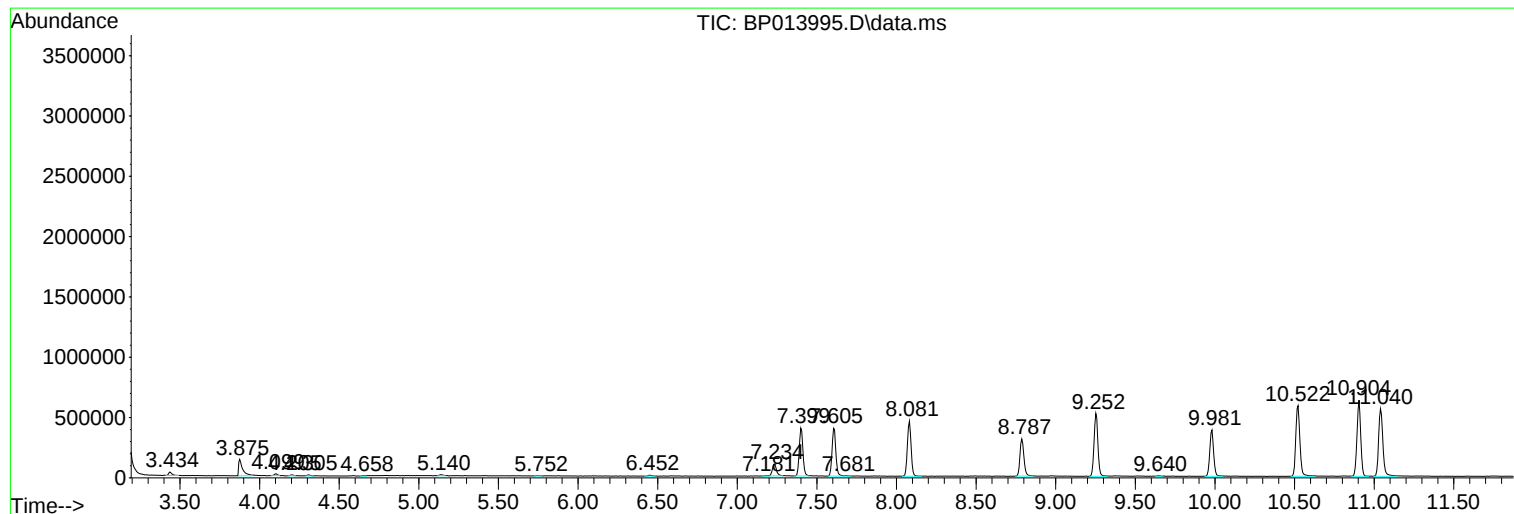

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013995.D
Acq On : 09 Mar 2023 01:09
Operator : CG/JU
Sample : 01729-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013995.D
Acq On : 09 Mar 2023 01:09
Operator : CG/JU
Sample : 01729-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc