

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013996.D
 Acq On : 09 Mar 2023 01:44
 Operator : CG/JU
 Sample : 01746-01DL2 50X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAC1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.205	166	173	178	rBV3	6637	10728	0.41%	0.099%
2	4.781	266	271	273	rVB6	2173	3468	0.13%	0.032%
3	4.805	273	275	278	rBV3	2479	3132	0.12%	0.029%
4	5.969	469	473	478	rVB6	1639	3398	0.13%	0.031%
5	6.063	487	489	493	rVB4	2246	2693	0.10%	0.025%
6	7.405	711	717	723	rBV3	6033	13491	0.52%	0.125%
7	7.616	749	753	758	rBV6	4472	7710	0.30%	0.071%
8	7.804	781	785	794	rVB7	4356	8316	0.32%	0.077%
9	8.081	825	832	850	rBV	386691	644564	24.68%	5.955%
10	8.628	920	925	928	rBV5	2017	3102	0.12%	0.029%
11	8.810	952	956	960	rBV7	2643	4447	0.17%	0.041%
12	8.951	975	980	986	rBV9	4667	9255	0.35%	0.085%
13	9.269	1026	1034	1040	rBV5	5917	13392	0.51%	0.124%
14	9.528	1071	1078	1079	rBV6	2369	3633	0.14%	0.034%
15	9.987	1152	1156	1166	rVB10	4744	10872	0.42%	0.100%
16	10.304	1207	1210	1216	rVB8	1578	3427	0.13%	0.032%
17	10.546	1244	1251	1252	rBV6	4113	5325	0.20%	0.049%
18	10.904	1305	1312	1317	rBV	509566	885071	33.89%	8.176%
19	10.951	1317	1320	1328	rVB	149201	247497	9.48%	2.286%
20	11.075	1334	1341	1352	rVB	21891	45302	1.73%	0.419%
21	12.445	1571	1574	1578	rBV5	1528	2613	0.10%	0.024%
22	12.557	1587	1593	1602	rBV2	12431	23539	0.90%	0.217%
23	12.775	1625	1630	1638	rVB3	12753	23852	0.91%	0.220%
24	13.045	1671	1676	1678	rBV6	2430	2980	0.11%	0.028%
25	13.557	1756	1763	1772	rBV2	9219	16752	0.64%	0.155%
26	13.904	1821	1822	1828	rVB6	2405	3054	0.12%	0.028%
27	14.034	1839	1844	1850	rBV9	1845	3315	0.13%	0.031%
28	14.122	1850	1859	1864	rBV	23923	40114	1.54%	0.371%
29	14.416	1903	1909	1919	rBV2	21320	38329	1.47%	0.354%
30	14.716	1951	1960	1967	rBV	821157	1255310	48.06%	11.597%
31	14.781	1967	1971	1979	rVV2	33578	54916	2.10%	0.507%
32	14.857	1979	1984	1991	rVB	10769	21067	0.81%	0.195%
33	15.116	2023	2028	2036	rBV	25227	43442	1.66%	0.401%
34	15.281	2052	2056	2062	rBV9	5502	10623	0.41%	0.098%
35	15.569	2101	2105	2107	rBV5	1838	2749	0.11%	0.025%
36	15.710	2123	2129	2135	rBV2	36772	56445	2.16%	0.521%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013996.D
 Acq On : 09 Mar 2023 01:44
 Operator : CG/JU
 Sample : 01746-01DL2 50X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAC1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	15.769	2135	2139	2145	rVB3	10941	15755	0.60%	0.146%
38	15.857	2148	2154	2160	rBV3	5020	12231	0.47%	0.113%
39	16.075	2186	2191	2197	rVB10	3213	5462	0.21%	0.050%
40	16.204	2211	2213	2217	rBV5	2562	2974	0.11%	0.027%
41	16.451	2249	2255	2257	rBV7	3104	4943	0.19%	0.046%
42	16.733	2298	2303	2308	rBV2	8736	17462	0.67%	0.161%
43	16.986	2343	2346	2349	rBV5	2044	3157	0.12%	0.029%
44	17.128	2366	2370	2379	rVV3	17355	30777	1.18%	0.284%
45	17.257	2390	2392	2395	rVV4	3823	5534	0.21%	0.051%
46	17.286	2395	2397	2401	rVB5	3939	5272	0.20%	0.049%
47	17.469	2422	2428	2434	rBV	1234696	1817250	69.58%	16.788%
48	17.569	2441	2445	2451	rVB2	41959	61116	2.34%	0.565%
49	17.875	2492	2497	2503	rBV	73574	108263	4.15%	1.000%
50	18.039	2521	2525	2529	rBV2	9509	14509	0.56%	0.134%
51	18.292	2566	2568	2570	rBV3	3167	2816	0.11%	0.026%
52	18.451	2593	2595	2598	rBV4	3639	3646	0.14%	0.034%
53	19.792	2819	2823	2828	rBV	67353	88759	3.40%	0.820%
54	21.545	3116	3121	3128	rBV	1850468	2485160	95.15%	22.958%
55	24.086	3546	3553	3568	rVB	1248138	2611762	100.00%	24.128%




Sum of corrected areas: 10824771

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013996.D
Acq On : 09 Mar 2023 01:44
Operator : CG/JU
Sample : 01746-01DL2 50X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAC1DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

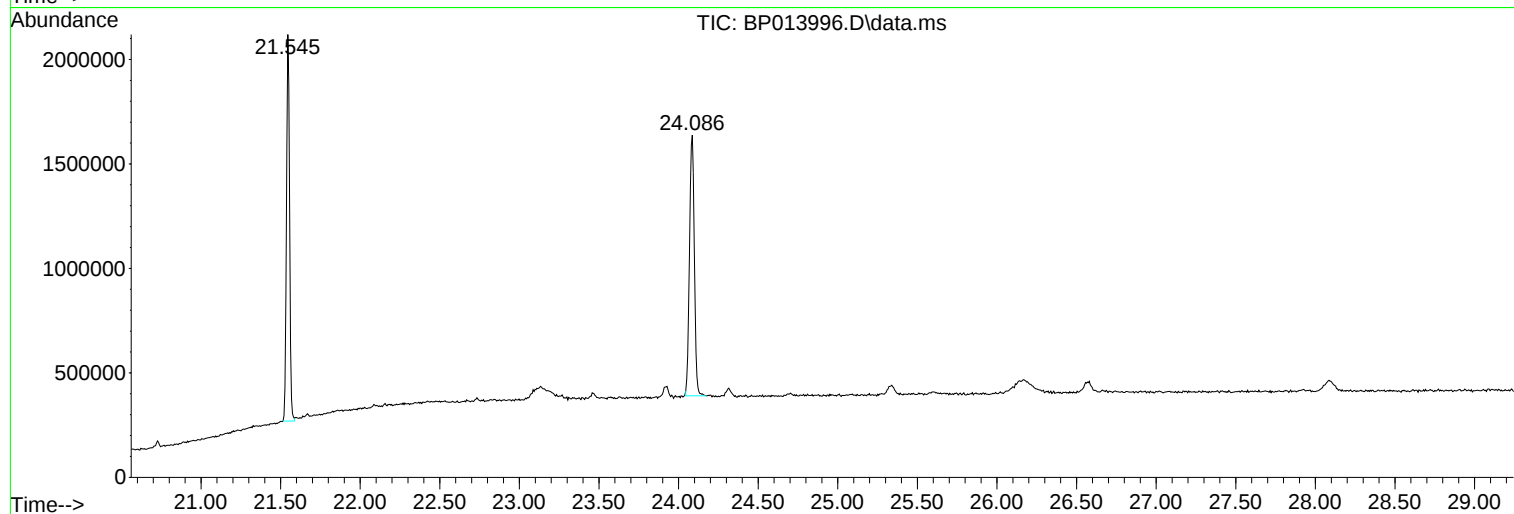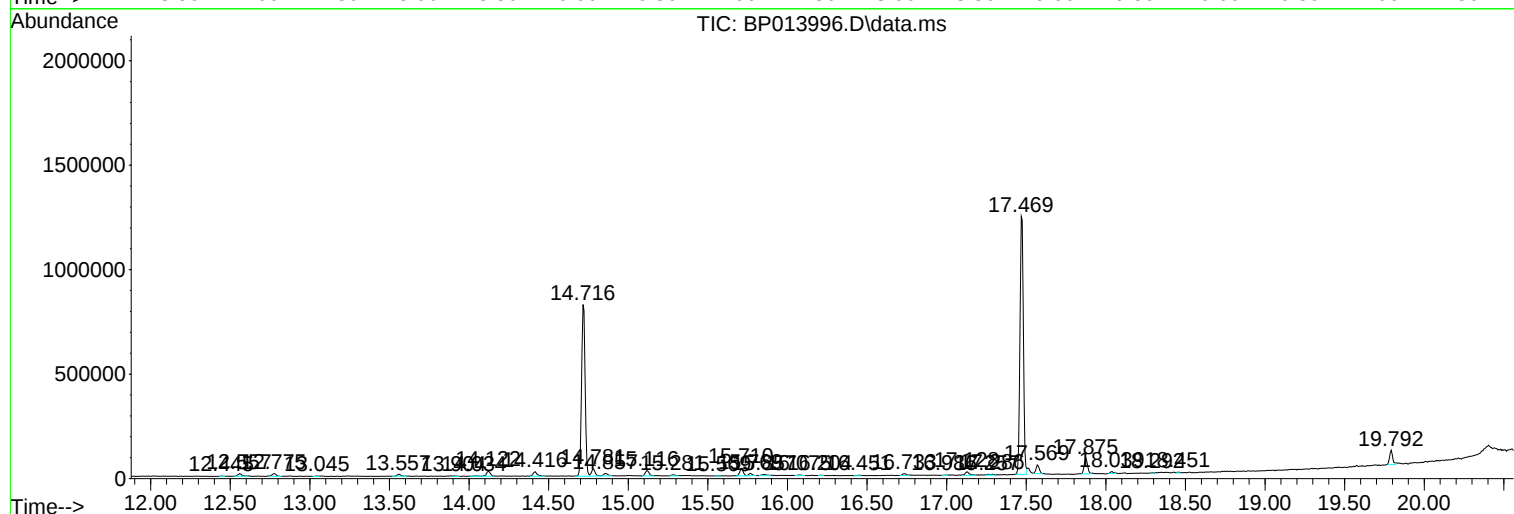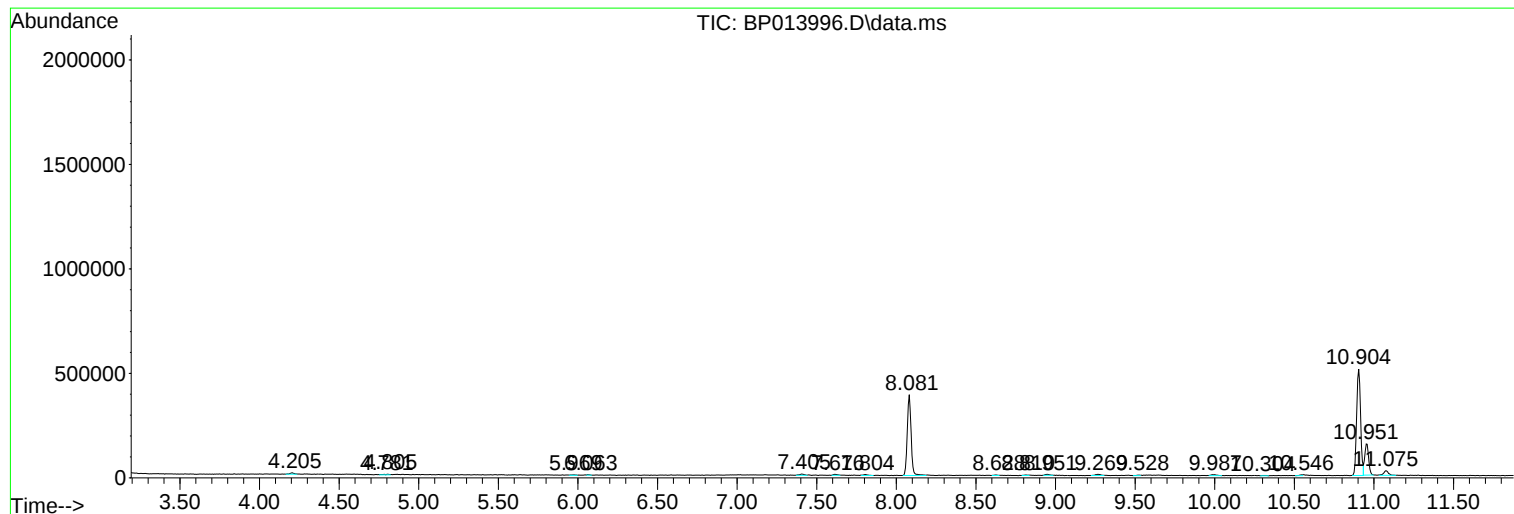

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013996.D
Acq On : 09 Mar 2023 01:44
Operator : CG/JU
Sample : 01746-01DL2 50X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAC1DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013996.D
Acq On : 09 Mar 2023 01:44
Operator : CG/JU
Sample : 01746-01DL2 50X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAC1DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc