

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP013999.D
 Acq On : 09 Mar 2023 03:25
 Operator : CG/JU
 Sample : PB151195BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	39	42	49	rVB	37320	53166	0.98%	0.119%
2	3.870	112	116	135	rBV	458213	762712	14.00%	1.706%
3	4.199	168	172	178	rBV	9666	14303	0.26%	0.032%
4	7.228	677	687	699	rBV	598765	984104	18.06%	2.201%
5	7.399	710	716	726	rVB	450959	710974	13.05%	1.590%
6	7.605	744	751	766	rBV	607131	981089	18.01%	2.194%
7	8.081	825	832	844	rBV	521358	833127	15.29%	1.863%
8	8.787	944	952	967	rBV	732996	1229656	22.57%	2.750%
9	9.252	1024	1031	1041	rBV	580349	968722	17.78%	2.166%
10	9.981	1147	1155	1166	rBV	528113	881453	16.18%	1.971%
11	10.522	1240	1247	1260	rBV	726634	1282074	23.53%	2.867%
12	10.905	1304	1312	1323	rVB	709637	1171363	21.50%	2.619%
13	11.040	1327	1335	1354	rBV	686199	1246833	22.89%	2.788%
14	12.493	1574	1582	1588	rBV4	8821	18954	0.35%	0.042%
15	14.122	1852	1859	1873	rBV	1495518	2059353	37.80%	4.605%
16	14.410	1901	1908	1925	rBV	1447317	2133250	39.16%	4.771%
17	14.716	1952	1960	1970	rBV	1102370	1617920	29.70%	3.618%
18	14.910	1987	1993	2018	rBV	583900	1051159	19.30%	2.351%
19	15.710	2117	2129	2140	rBV	2046934	2909010	53.40%	6.505%
20	15.822	2142	2148	2163	rVV	764162	1129003	20.72%	2.525%
21	15.951	2166	2170	2179	rVB3	12457	21044	0.39%	0.047%
22	17.145	2369	2373	2380	rBV10	3530	7183	0.13%	0.016%
23	17.263	2389	2393	2396	rBV4	3938	5892	0.11%	0.013%
24	17.469	2421	2428	2438	rBV	1598735	2331960	42.81%	5.215%
25	17.569	2439	2445	2456	rVV	2432150	3477079	63.83%	7.776%
26	19.369	2747	2751	2757	rBV3	36651	53482	0.98%	0.120%
27	19.439	2759	2763	2768	rVV	31658	48399	0.89%	0.108%
28	19.792	2817	2823	2832	rBV	3713331	4731175	86.85%	10.580%
29	21.545	3116	3121	3129	rBV	2364284	3201125	58.76%	7.159%
30	23.921	3517	3525	3538	rVB	2664834	5447784	100.00%	12.183%
31	24.086	3546	3553	3567	rVB2	1540514	3353794	61.56%	7.500%




Sum of corrected areas: 44717142

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013999.D
Acq On : 09 Mar 2023 03:25
Operator : CG/JU
Sample : PB151195BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

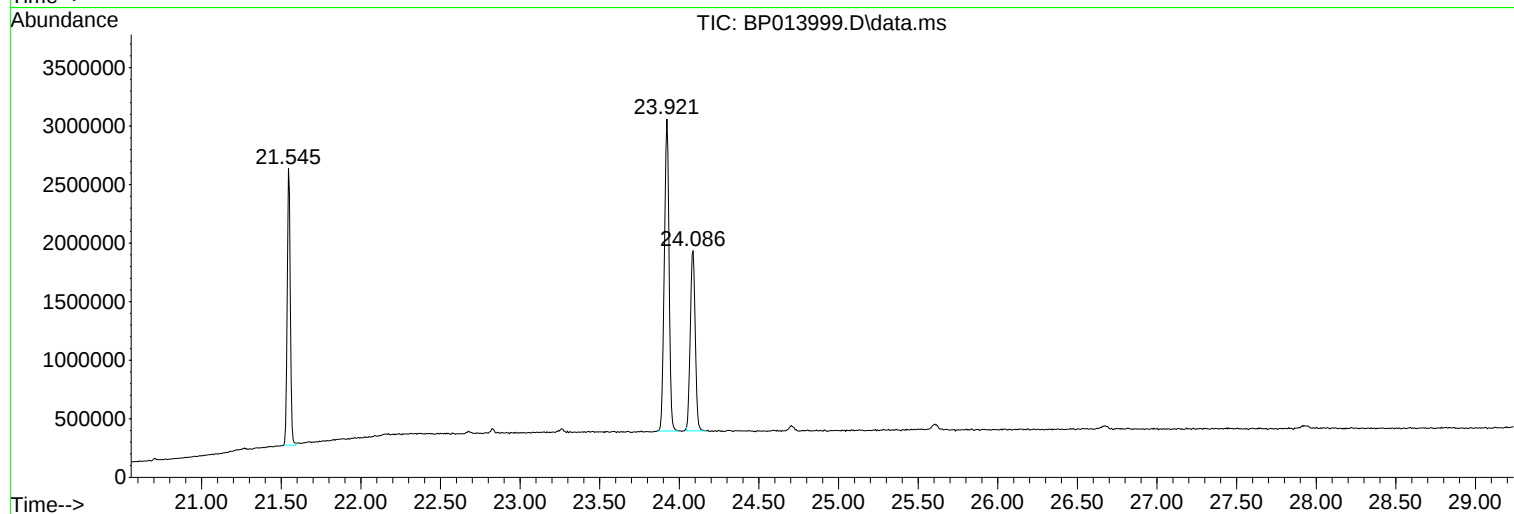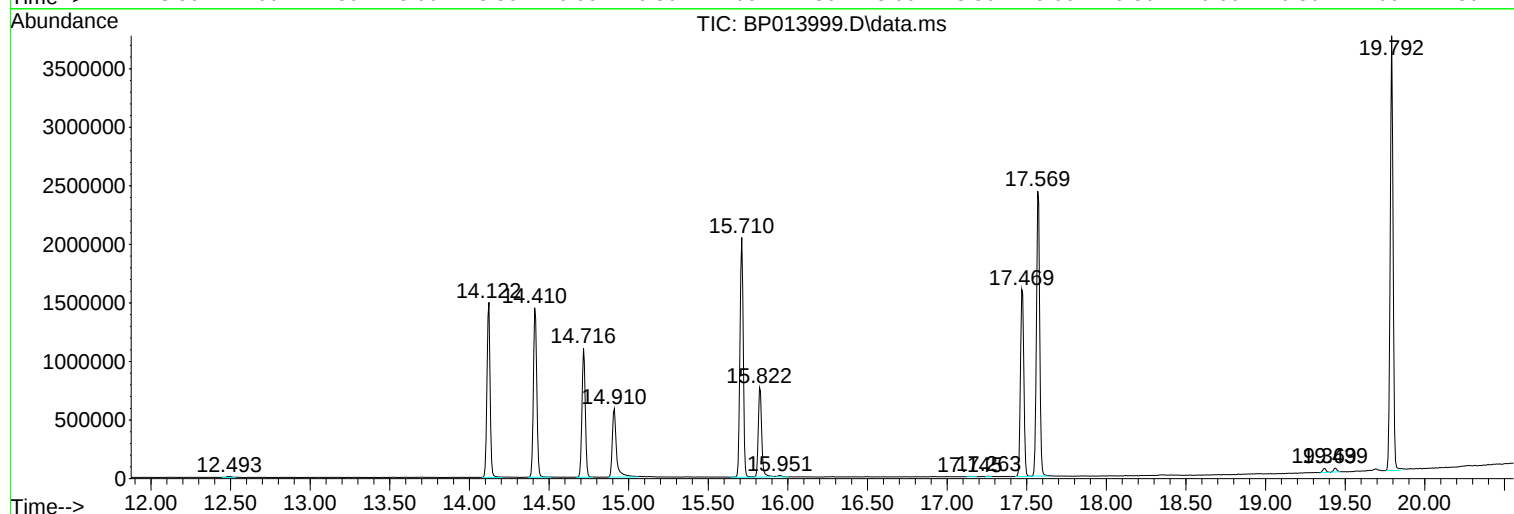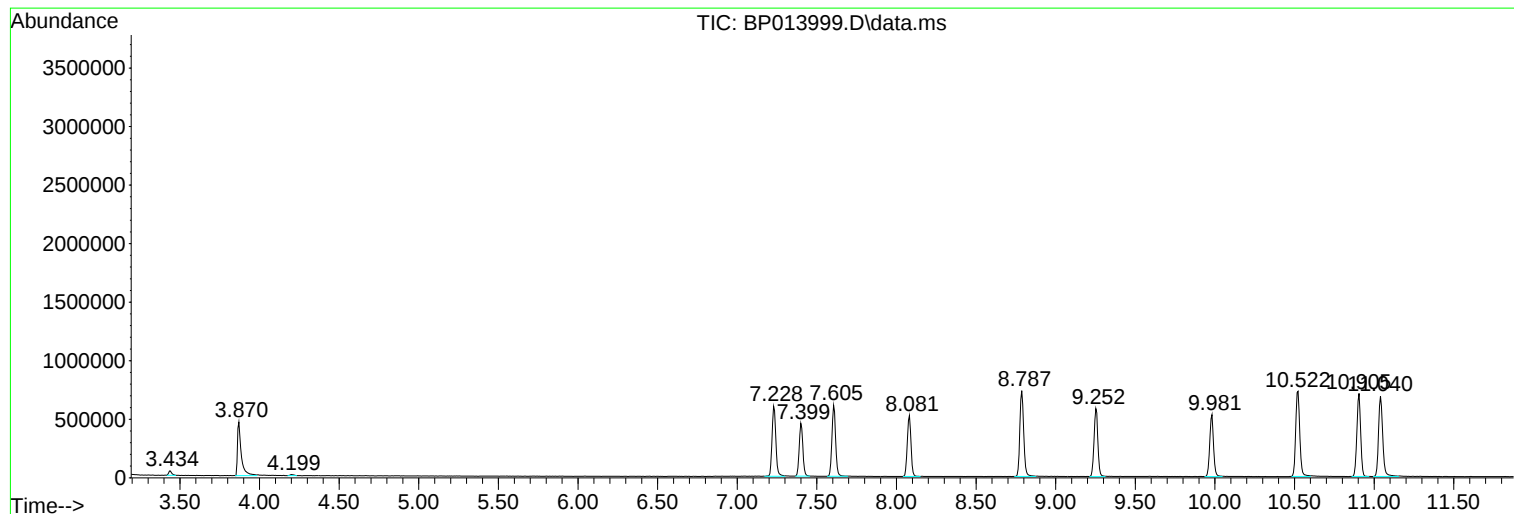

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013999.D
Acq On : 09 Mar 2023 03:25
Operator : CG/JU
Sample : PB151195BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP013999.D
Acq On : 09 Mar 2023 03:25
Operator : CG/JU
Sample : PB151195BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc