

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014001.D
 Acq On : 09 Mar 2023 09:48
 Operator : CG/JU
 Sample : PB151235BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	39	43	52	rVB	34920	47048	1.14%	0.123%
2	3.875	114	117	135	rBV	388447	669430	16.25%	1.753%
3	4.210	170	174	179	rBV4	8623	14462	0.35%	0.038%
4	7.240	682	689	705	rVB	524161	869379	21.10%	2.277%
5	7.410	709	718	727	rBV	405851	652819	15.85%	1.709%
6	7.616	745	753	765	rBV	528016	884319	21.47%	2.316%
7	8.087	826	833	843	rBV	455395	753420	18.29%	1.973%
8	8.792	946	953	965	rBV	634615	1076119	26.12%	2.818%
9	9.263	1024	1033	1046	rBV	516304	848885	20.61%	2.223%
10	9.987	1147	1156	1172	rBV	423847	744777	18.08%	1.950%
11	10.528	1240	1248	1261	rBV	627779	1091933	26.51%	2.859%
12	10.916	1306	1314	1326	rBV	613988	1036930	25.17%	2.715%
13	11.051	1330	1337	1354	rBV	602325	1076576	26.13%	2.819%
14	12.492	1577	1582	1588	rBV3	11133	20249	0.49%	0.053%
15	13.880	1811	1818	1819	rBV5	3564	7694	0.19%	0.020%
16	14.127	1853	1860	1874	rVB	1311495	1840074	44.67%	4.818%
17	14.422	1903	1910	1924	rBV	1273305	1948584	47.30%	5.102%
18	14.727	1955	1962	1972	rVB	1052714	1516174	36.81%	3.970%
19	14.916	1988	1994	2020	rBV	505978	916855	22.26%	2.401%
20	15.139	2030	2032	2036	rVB5	4322	4915	0.12%	0.013%
21	15.457	2080	2086	2095	rBV5	5402	15404	0.37%	0.040%
22	15.639	2110	2117	2119	rBV5	12379	25942	0.63%	0.068%
23	15.721	2124	2131	2138	rVV	1796289	2557834	62.09%	6.698%
24	15.833	2144	2150	2166	rBV	653217	909428	22.08%	2.381%
25	15.963	2168	2172	2177	rVB3	7673	11661	0.28%	0.031%
26	16.086	2186	2193	2200	rBV6	8445	18846	0.46%	0.049%
27	16.292	2224	2228	2233	rVB5	5198	6987	0.17%	0.018%
28	16.504	2260	2264	2270	rBV9	4192	6476	0.16%	0.017%
29	16.739	2299	2304	2309	rBV8	7076	11790	0.29%	0.031%
30	16.921	2330	2335	2342	rBV2	17386	27390	0.66%	0.072%
31	16.992	2343	2347	2351	rVV5	4416	6542	0.16%	0.017%
32	17.157	2369	2375	2380	rBV10	4254	8052	0.20%	0.021%
33	17.286	2392	2397	2404	rBV7	12103	23272	0.56%	0.061%
34	17.486	2423	2431	2440	rBV	1428760	2070039	50.25%	5.420%
35	17.580	2441	2447	2459	rVV2	2109356	3016061	73.22%	7.898%
36	17.845	2488	2492	2496	rBV6	7195	12103	0.29%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014001.D
 Acq On : 09 Mar 2023 09:48
 Operator : CG/JU
 Sample : PB151235BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	17.998	2514	2518	2522	rVB2	15042	18681	0.45%	0.049%
38	18.315	2568	2572	2575	rBV5	5156	8732	0.21%	0.023%
39	18.774	2648	2650	2654	rVB4	6792	7671	0.19%	0.020%
40	18.898	2669	2671	2677	rVB4	14836	16657	0.40%	0.044%
41	19.380	2750	2753	2758	rVB3	28304	37667	0.91%	0.099%
42	19.451	2761	2765	2770	rBV	29847	44447	1.08%	0.116%
43	19.804	2819	2825	2838	rBV	3149186	4037963	98.02%	10.574%
44	21.562	3119	3124	3135	rBV	1838249	2578444	62.59%	6.752%
45	23.939	3521	3528	3540	rVB2	2006309	4119357	100.00%	10.787%
46	24.103	3549	3556	3568	rVB2	1205966	2571066	62.41%	6.732%




Sum of corrected areas: 38189154

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014001.D
Acq On : 09 Mar 2023 09:48
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

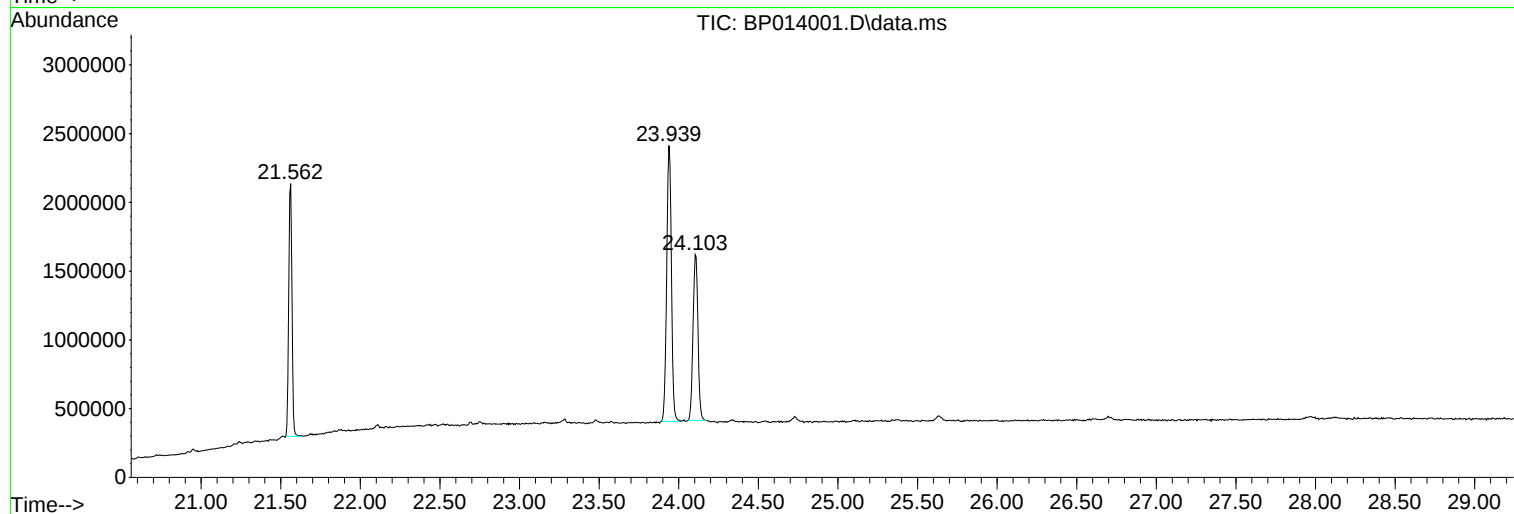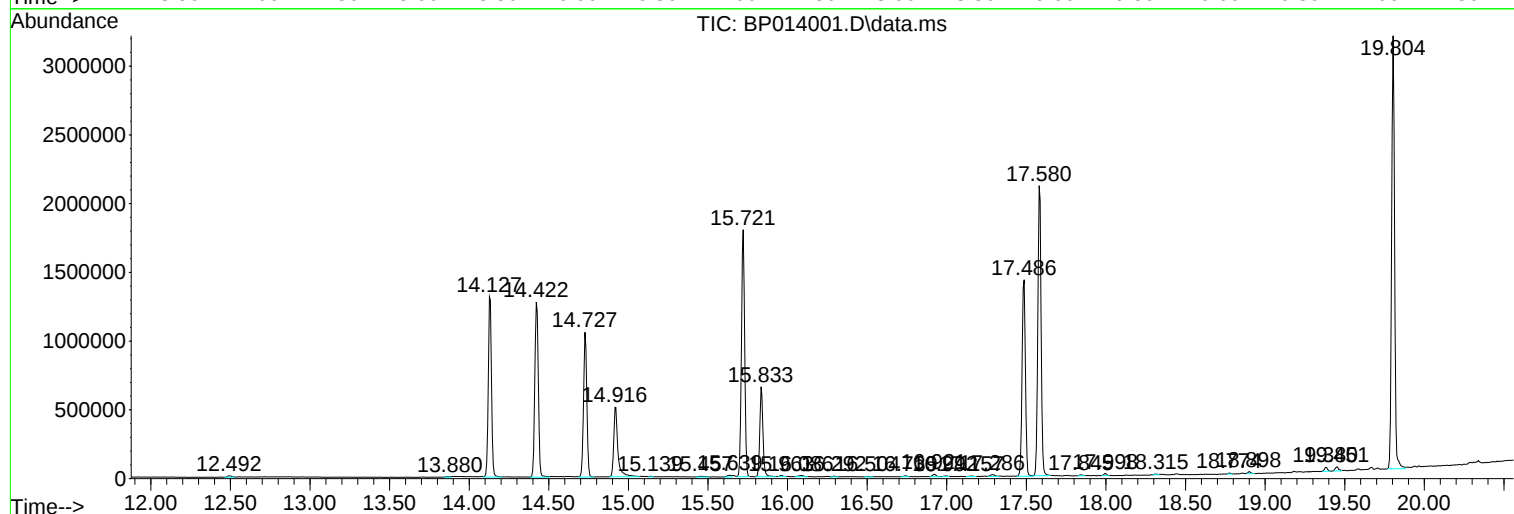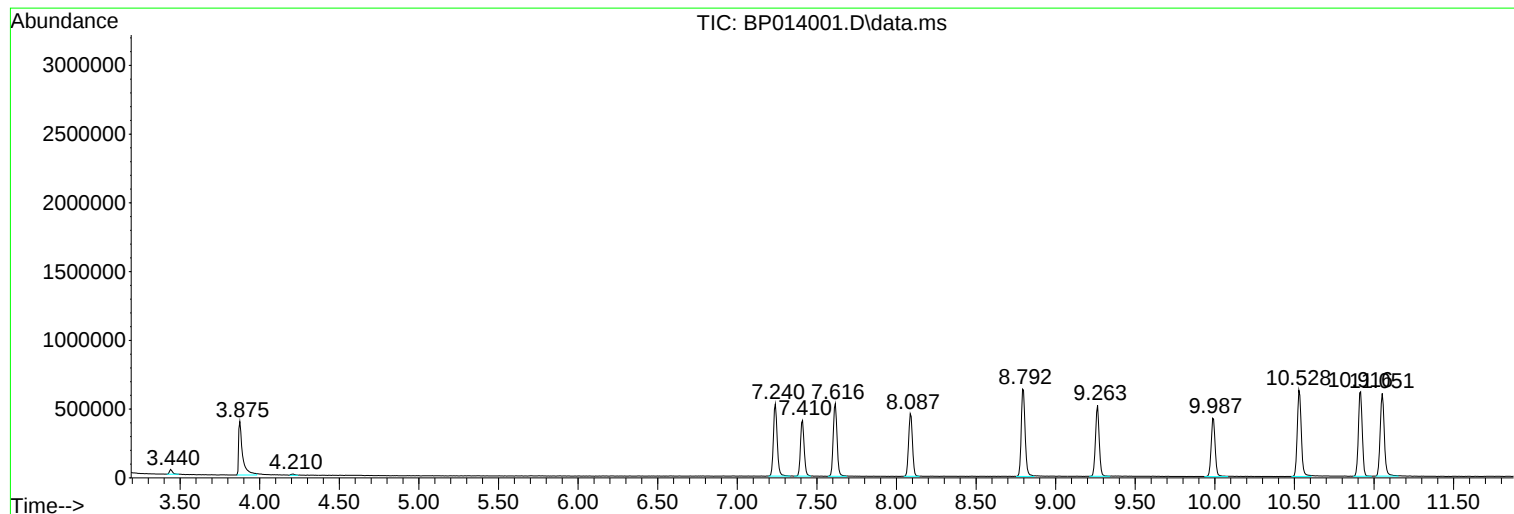

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014001.D
Acq On : 09 Mar 2023 09:48
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014001.D
Acq On : 09 Mar 2023 09:48
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------