

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014010.D
 Acq On : 09 Mar 2023 14:57
 Operator : CG/JU
 Sample : PB151235BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	49	rBV	32384	41655	1.08%	0.119%
2	3.870	112	116	138	rBV	372349	627593	16.30%	1.785%
3	4.199	169	172	177	rVB	6909	8760	0.23%	0.025%
4	7.228	680	687	703	rBV	487492	814555	21.15%	2.317%
5	7.399	710	716	727	rBV	374686	582748	15.13%	1.658%
6	7.605	744	751	766	rBV	490654	807071	20.96%	2.296%
7	8.081	824	832	843	rBV	421010	686760	17.83%	1.954%
8	8.787	944	952	965	rBV	613742	1016394	26.39%	2.892%
9	9.252	1021	1031	1045	rBV	467354	780414	20.26%	2.220%
10	9.981	1148	1155	1170	rBV	401357	701860	18.22%	1.997%
11	10.522	1238	1247	1262	rBV	576809	1038196	26.96%	2.954%
12	10.904	1304	1312	1322	rVB	572483	956309	24.83%	2.721%
13	11.040	1328	1335	1349	rBV	558548	1007348	26.16%	2.866%
14	12.487	1576	1581	1587	rBV3	8083	16400	0.43%	0.047%
15	14.122	1852	1859	1870	rBV	1181567	1689090	43.86%	4.805%
16	14.228	1875	1877	1885	rVB9	2634	4162	0.11%	0.012%
17	14.410	1900	1908	1922	rBV	1222250	1843648	47.87%	5.245%
18	14.716	1953	1960	1968	rBV	943635	1433686	37.23%	4.079%
19	14.910	1986	1993	2020	rBV	473598	860890	22.35%	2.449%
20	15.710	2121	2129	2142	rBV	1662935	2397061	62.24%	6.819%
21	15.822	2142	2148	2163	rVV	612854	891032	23.14%	2.535%
22	15.951	2166	2170	2177	rVB6	9912	17042	0.44%	0.048%
23	16.281	2223	2226	2231	rVB7	2541	3881	0.10%	0.011%
24	17.263	2389	2393	2395	rBV5	3139	3894	0.10%	0.011%
25	17.475	2421	2429	2439	rBV	1278884	1894003	49.18%	5.388%
26	17.569	2439	2445	2457	rBV	1920681	2779079	72.16%	7.906%
27	19.369	2747	2751	2757	rVB3	28511	37727	0.98%	0.107%
28	19.439	2759	2763	2768	rBV2	21585	35536	0.92%	0.101%
29	19.792	2817	2823	2833	rBV	2780129	3641247	94.55%	10.359%
30	21.551	3117	3122	3130	rBV	1706169	2316183	60.14%	6.589%
31	23.921	3518	3525	3537	rVB	1802151	3851156	100.00%	10.956%
32	24.086	3547	3553	3562	rVB2	1182495	2364863	61.41%	6.728%




Sum of corrected areas: 35150243

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014010.D
Acq On : 09 Mar 2023 14:57
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

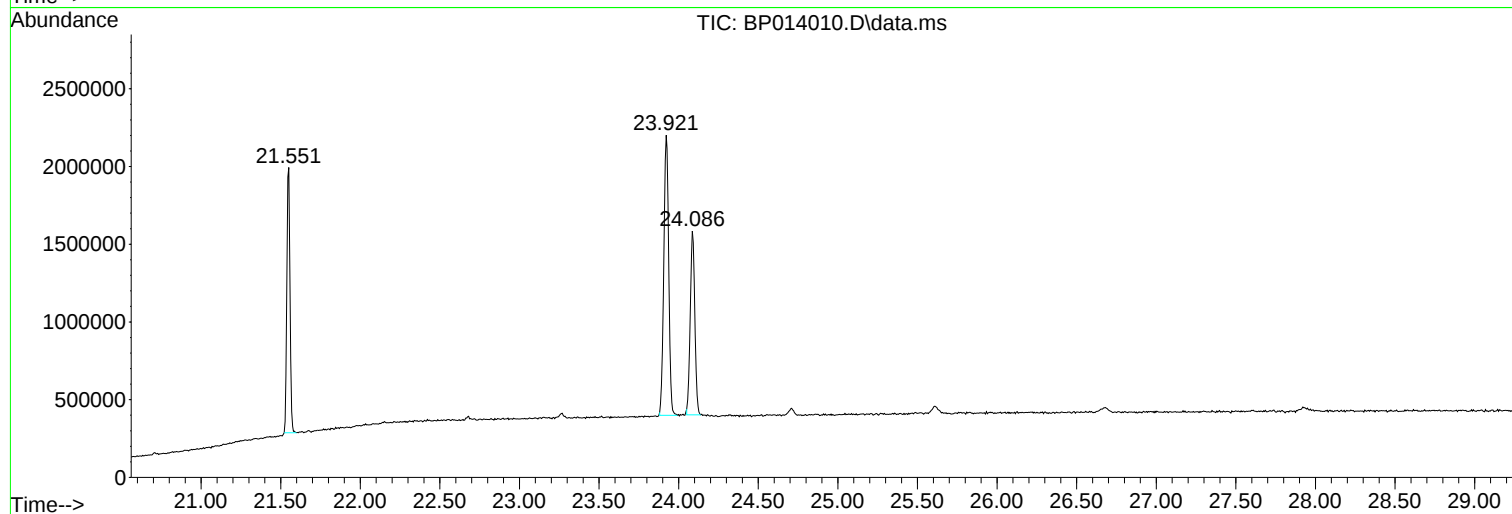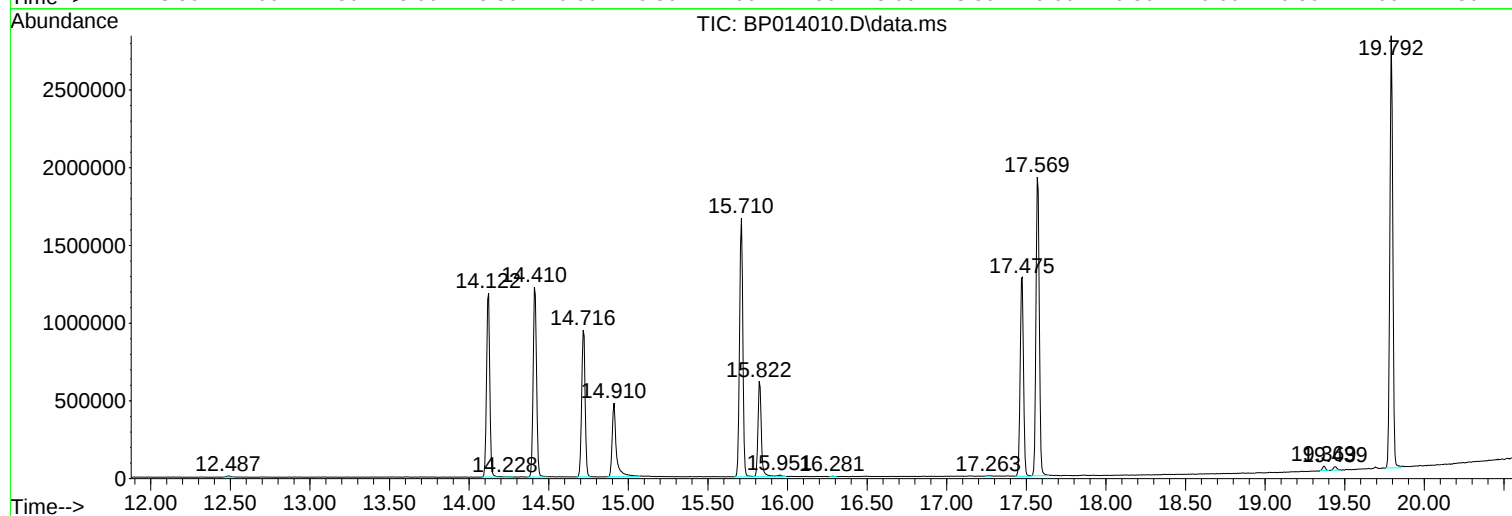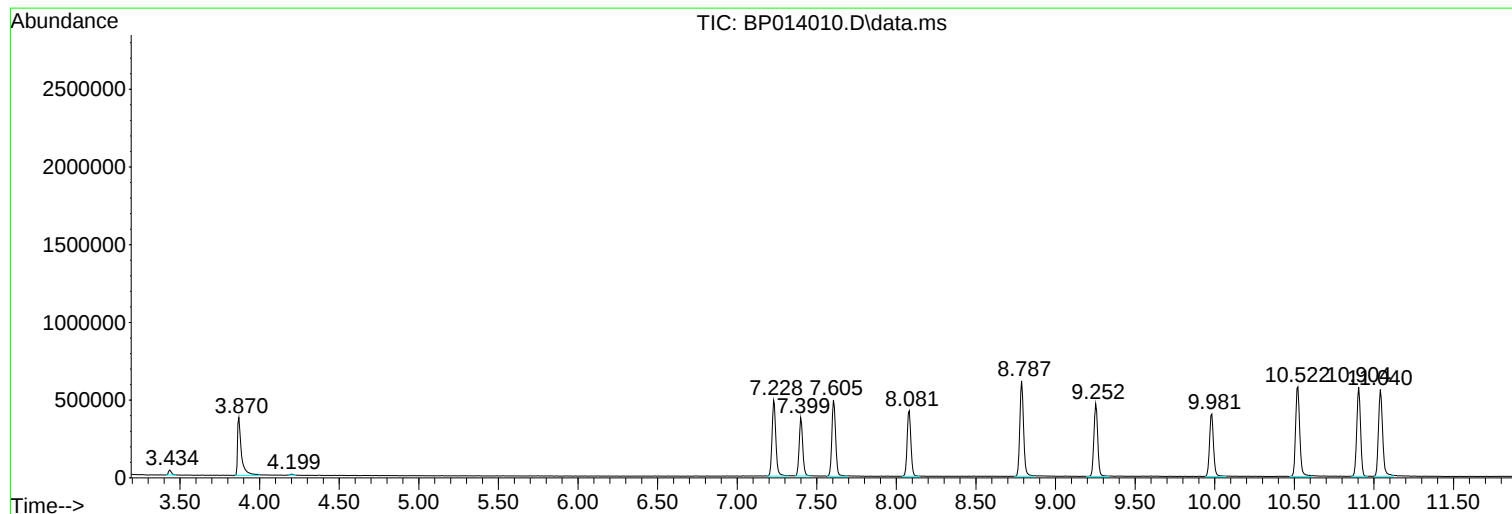

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014010.D
Acq On : 09 Mar 2023 14:57
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014010.D
Acq On : 09 Mar 2023 14:57
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc