

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014012.D
 Acq On : 09 Mar 2023 16:06
 Operator : CG/JU
 Sample : 01746-17DL 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.899	119	121	132	rBV	15589	31207	1.15%	0.148%
2	4.105	152	156	161	rVB4	3820	6411	0.24%	0.030%
3	4.205	169	173	180	rVB	9018	14930	0.55%	0.071%
4	4.311	187	191	197	rVB7	3675	7601	0.28%	0.036%
5	6.070	485	490	496	rVB4	5880	12205	0.45%	0.058%
6	6.546	564	571	574	rBV9	2255	5026	0.18%	0.024%
7	7.234	682	688	696	rBV	16940	35119	1.29%	0.167%
8	7.399	709	716	723	rBV	80866	133537	4.91%	0.634%
9	7.605	745	751	762	rBV	75940	136455	5.02%	0.648%
10	7.716	767	770	776	rVB3	5239	7614	0.28%	0.036%
11	7.799	776	784	790	rBV3	7824	14659	0.54%	0.070%
12	8.081	824	832	846	rBV	472248	780247	28.68%	3.704%
13	8.193	846	851	859	rVB2	4534	8628	0.32%	0.041%
14	8.622	920	924	931	rVB2	8121	12088	0.44%	0.057%
15	8.793	946	953	966	rVV2	57984	108628	3.99%	0.516%
16	8.934	971	977	983	rBV	26262	45756	1.68%	0.217%
17	9.252	1025	1031	1045	rVV	100906	189132	6.95%	0.898%
18	9.446	1055	1064	1070	rVV6	7384	15934	0.59%	0.076%
19	9.516	1070	1076	1080	rVV6	6247	11837	0.44%	0.056%
20	9.575	1080	1086	1091	rVV4	14438	32725	1.20%	0.155%
21	9.640	1092	1097	1103	rVB6	6640	13256	0.49%	0.063%
22	9.981	1146	1155	1167	rBV2	78502	150081	5.52%	0.712%
23	10.099	1170	1175	1178	rVV5	4160	5878	0.22%	0.028%
24	10.181	1183	1189	1194	rVB9	2813	6256	0.23%	0.030%
25	10.293	1203	1208	1213	rBV9	3660	7898	0.29%	0.037%
26	10.522	1238	1247	1260	rBV	112552	220848	8.12%	1.048%
27	10.905	1300	1312	1316	rBV	676242	1148581	42.21%	5.452%
28	10.952	1316	1320	1329	rVV	758460	1245099	45.76%	5.911%
29	11.046	1329	1336	1337	rVV	88379	128347	4.72%	0.609%
30	11.075	1338	1341	1352	rVB	114181	190502	7.00%	0.904%
31	11.287	1370	1377	1383	rVB	3460	8118	0.30%	0.039%
32	11.493	1407	1412	1419	rVB9	3660	7010	0.26%	0.033%
33	12.016	1491	1501	1508	rBV9	4516	13162	0.48%	0.062%
34	12.299	1546	1549	1556	rVB8	3954	5866	0.22%	0.028%
35	12.446	1568	1574	1578	rBV3	7630	15386	0.57%	0.073%
36	12.552	1587	1592	1600	rBV	61535	99418	3.65%	0.472%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014012.D
 Acq On : 09 Mar 2023 16:06
 Operator : CG/JU
 Sample : 01746-17DL 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	12.675	1606	1613	1618	rBV8	3909	8754	0.32%	0.042%
38	12.769	1620	1629	1637	rVB	62491	109445	4.02%	0.520%
39	12.869	1642	1646	1651	rVB7	5881	9268	0.34%	0.044%
40	12.928	1651	1656	1661	rBV9	3202	7507	0.28%	0.036%
41	13.199	1696	1702	1705	rVV8	3975	8910	0.33%	0.042%
42	13.240	1705	1709	1710	rVV4	5623	8741	0.32%	0.041%
43	13.269	1710	1714	1720	rVV8	7633	17419	0.64%	0.083%
44	13.440	1738	1743	1751	rBV8	6296	15843	0.58%	0.075%
45	13.551	1751	1762	1767	rVV2	38620	81800	3.01%	0.388%
46	13.593	1767	1769	1776	rVB7	8053	13846	0.51%	0.066%
47	13.751	1791	1796	1798	rBV5	5448	6951	0.26%	0.033%
48	13.875	1810	1817	1818	rBV7	6339	10548	0.39%	0.050%
49	14.034	1837	1844	1850	rBV5	10520	21087	0.78%	0.100%
50	14.116	1850	1858	1864	rBV	312683	436377	16.04%	2.072%
51	14.204	1870	1873	1881	rVB4	7188	13913	0.51%	0.066%
52	14.269	1881	1884	1889	rBV6	6184	11660	0.43%	0.055%
53	14.410	1902	1908	1922	rVB	302117	469344	17.25%	2.228%
54	14.593	1933	1939	1943	rBV	18607	25941	0.95%	0.123%
55	14.675	1943	1953	1954	rVV10	6469	11594	0.43%	0.055%
56	14.716	1954	1960	1966	rVV	1149147	1699585	62.47%	8.068%
57	14.781	1966	1971	1977	rVB	187684	267481	9.83%	1.270%
58	14.851	1977	1983	1989	rBV2	44864	69830	2.57%	0.331%
59	14.940	1992	1998	2001	rBV8	8815	16058	0.59%	0.076%
60	14.993	2004	2007	2011	rBV5	4496	5755	0.21%	0.027%
61	15.116	2022	2028	2037	rVB	110259	173009	6.36%	0.821%
62	15.210	2039	2044	2049	rVB8	4351	7679	0.28%	0.036%
63	15.275	2050	2055	2059	rVB8	7079	13135	0.48%	0.062%
64	15.328	2060	2064	2065	rBV4	4406	5425	0.20%	0.026%
65	15.540	2096	2100	2106	rBV	29393	38883	1.43%	0.185%
66	15.704	2123	2128	2134	rBV	431518	621198	22.83%	2.949%
67	15.763	2134	2138	2144	rVB	116872	160381	5.89%	0.761%
68	15.822	2144	2148	2157	rBV	110029	179649	6.60%	0.853%
69	15.951	2164	2170	2174	rBV5	10858	18653	0.69%	0.089%
70	16.069	2183	2190	2195	rBV2	37731	57011	2.10%	0.271%
71	16.204	2209	2213	2219	rVB7	9086	15779	0.58%	0.075%
72	16.410	2243	2248	2250	rBV	36176	52518	1.93%	0.249%
73	16.640	2281	2287	2296	rBV9	7667	22002	0.81%	0.104%
74	16.728	2297	2302	2313	rVV	21418	50221	1.85%	0.238%
75	16.916	2331	2334	2339	rVB7	5616	7089	0.26%	0.034%
76	16.981	2339	2345	2349	rBV9	8426	18581	0.68%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
 Data File : BP014012.D
 Acq On : 09 Mar 2023 16:06
 Operator : CG/JU
 Sample : 01746-17DL 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

77	17.122	2365	2369	2375	rVB3	25663	41743	1.53%	0.198%
78	17.204	2379	2383	2387	rBV	33126	40193	1.48%	0.191%
79	17.257	2387	2392	2395	rVV5	20946	31372	1.15%	0.149%
80	17.292	2395	2398	2402	rVB2	16323	22184	0.82%	0.105%
81	17.363	2405	2410	2414	rBV8	6720	11276	0.41%	0.054%
82	17.422	2417	2420	2422	rBV4	5765	6951	0.26%	0.033%
83	17.469	2422	2428	2433	rVV	1643212	2317946	85.19%	11.003%
84	17.510	2433	2435	2440	rVV	129136	183214	6.73%	0.870%
85	17.569	2440	2445	2459	rVB2	525035	791743	29.10%	3.758%
86	17.869	2491	2496	2502	rVV	307265	417983	15.36%	1.984%
87	17.939	2505	2508	2514	rVB	31360	38982	1.43%	0.185%
88	18.028	2519	2523	2527	rBV	24483	35292	1.30%	0.168%
89	18.110	2533	2537	2542	rVB2	19977	25645	0.94%	0.122%
90	18.292	2565	2568	2572	rBV5	9884	12858	0.47%	0.061%
91	18.334	2572	2575	2577	rBV3	14192	16134	0.59%	0.077%
92	18.510	2603	2605	2612	rVB6	8144	12357	0.45%	0.059%
93	18.604	2616	2621	2627	rBV3	36629	59318	2.18%	0.282%
94	19.210	2719	2724	2726	rBV4	39844	55031	2.02%	0.261%
95	19.233	2726	2728	2735	rVB6	36906	45927	1.69%	0.218%
96	19.363	2747	2750	2755	rVB5	16902	21835	0.80%	0.104%
97	19.792	2817	2823	2832	rBV	711849	1004352	36.91%	4.768%
98	21.545	3116	3121	3128	rBV	1979338	2720824	100.00%	12.916%
99	23.916	3519	3524	3534	rVB2	453775	933633	34.31%	4.432%
100	24.086	3546	3553	3561	rVB	1268379	2554599	93.89%	12.127%




Sum of corrected areas: 21065707

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014012.D
Acq On : 09 Mar 2023 16:06
Operator : CG/JU
Sample : 01746-17DL 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAG0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

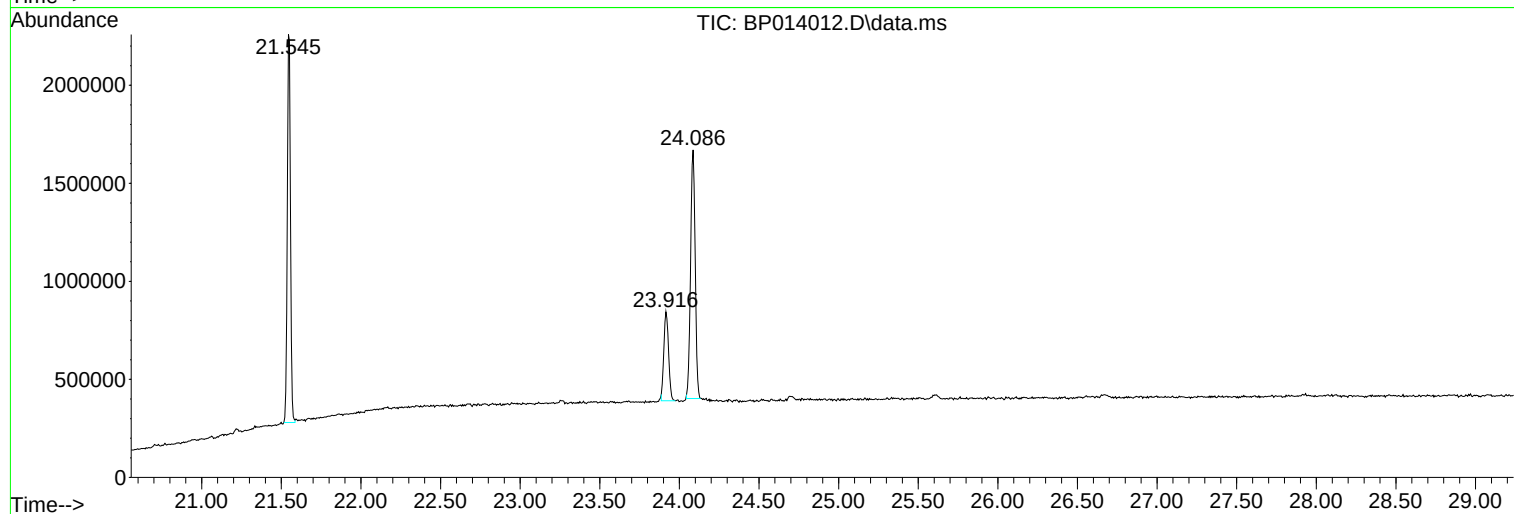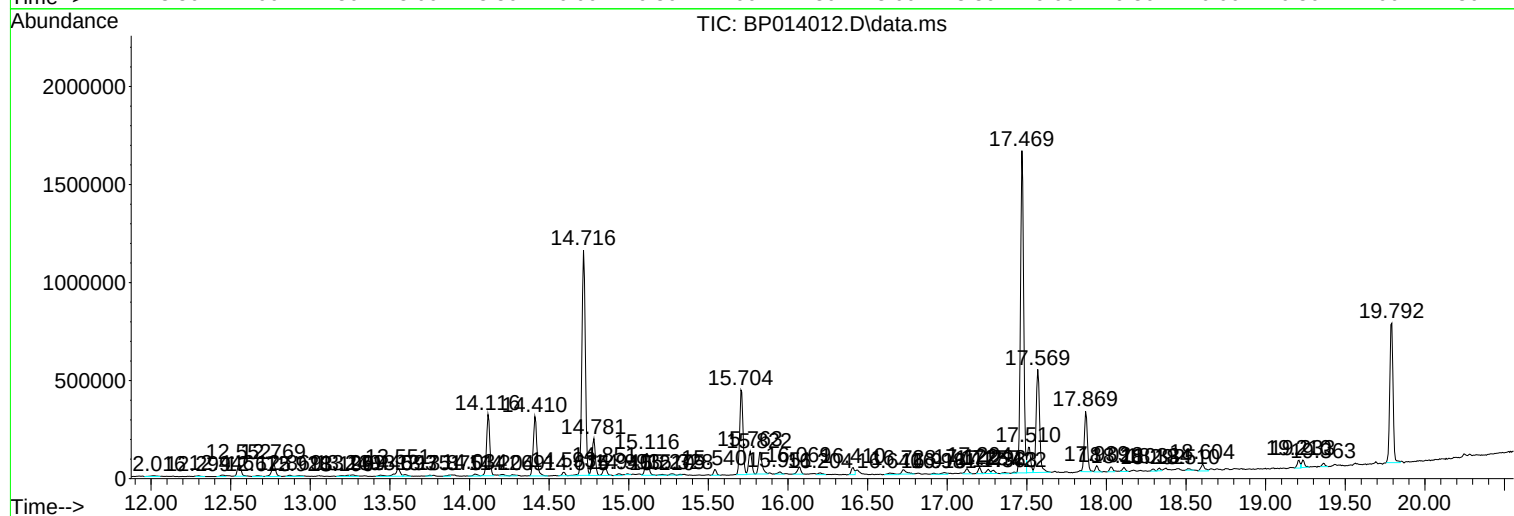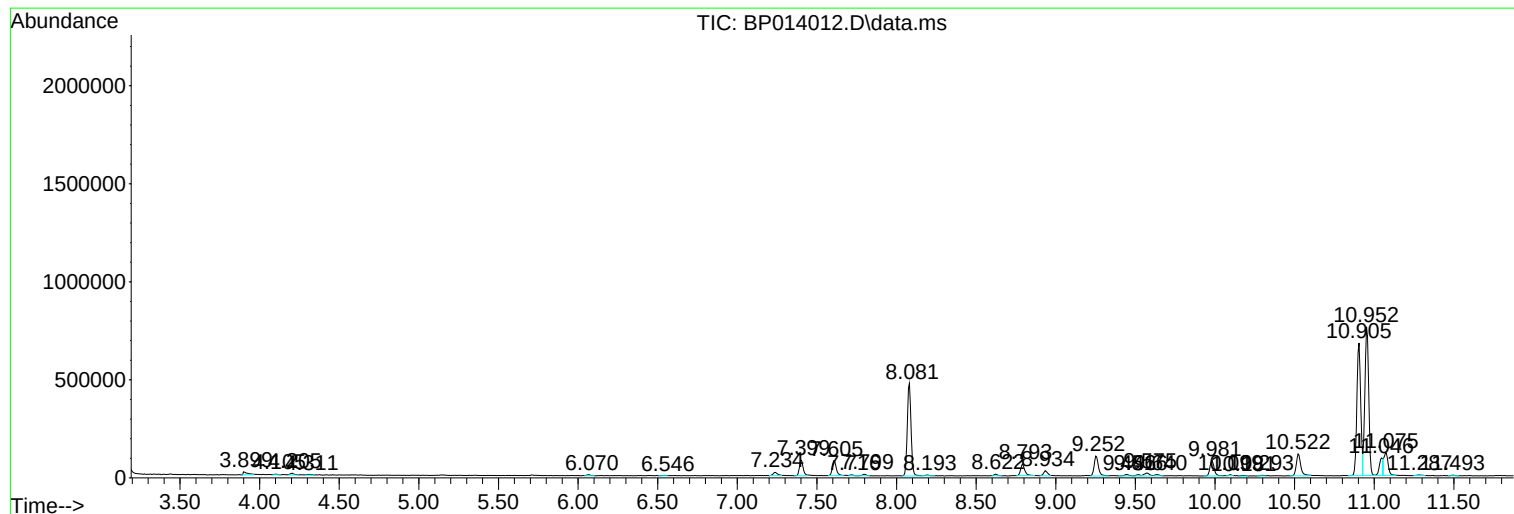

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014012.D
Acq On : 09 Mar 2023 16:06
Operator : CG/JU
Sample : 01746-17DL 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAG0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030823\
Data File : BP014012.D
Acq On : 09 Mar 2023 16:06
Operator : CG/JU
Sample : 01746-17DL 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAG0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc