

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
 Data File : BP009421.D
 Acq On : 16 Mar 2022 13:51
 Operator : CG/JU
 Sample : PB142486BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142486BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.417	406	413	433	rBV	4759591	7802930	44.31%	9.753%
2	7.005	674	683	710	rBV	4346761	7837430	44.50%	9.796%
3	7.805	812	819	834	rBV	980736	1714100	9.73%	2.142%
4	8.963	1007	1016	1036	rBV	2849722	5234510	29.72%	6.543%
5	10.605	1285	1295	1315	rBV	1141625	2324385	13.20%	2.905%
6	13.069	1706	1714	1731	rBV	7776589	12875053	73.11%	16.092%
7	14.451	1941	1949	1967	rBV	1795337	3120920	17.72%	3.901%
8	15.945	2196	2203	2233	rBV	6042766	10043716	57.03%	12.554%
9	17.210	2411	2418	2433	rBV	2082931	3623121	20.57%	4.529%
10	19.498	2803	2807	2815	rBV	227378	304946	1.73%	0.381%
11	19.786	2850	2856	2870	rBV	13340648	17611172	100.00%	22.012%
12	20.528	2978	2982	2986	rBV2	186889	227046	1.29%	0.284%
13	21.322	3112	3117	3127	rBV	2516174	3625663	20.59%	4.532%
14	23.727	3520	3526	3539	rVB2	1572969	3661720	20.79%	4.577%




Sum of corrected areas: 80006712

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009421.D
Acq On : 16 Mar 2022 13:51
Operator : CG/JU
Sample : PB142486BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142486BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

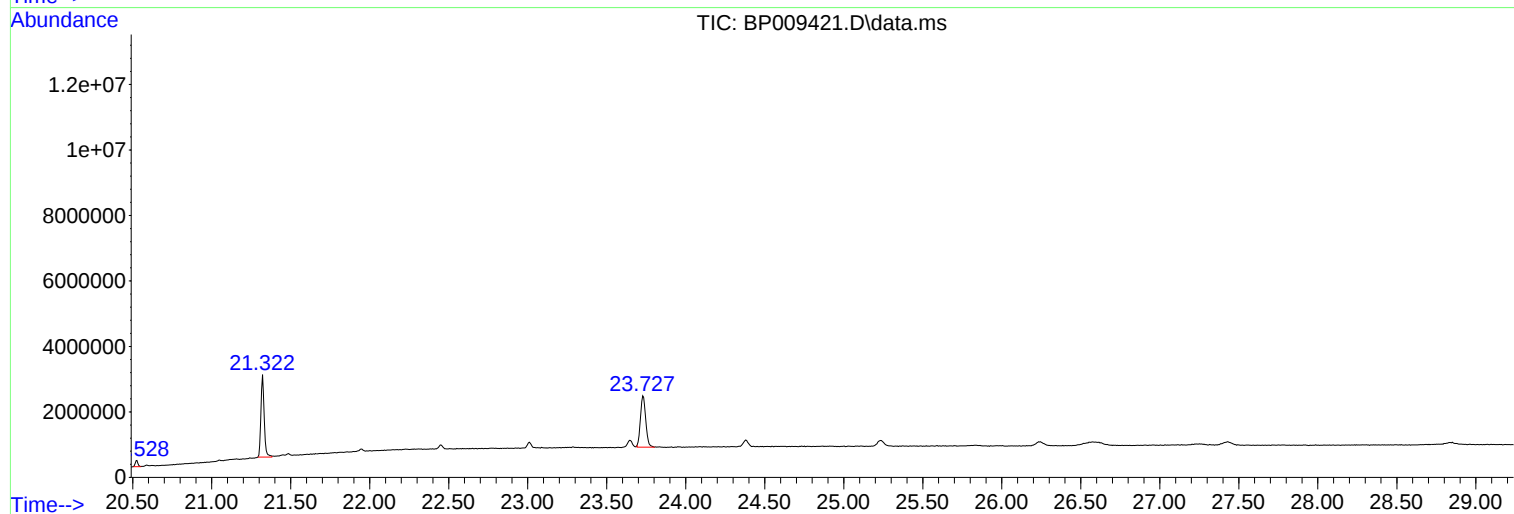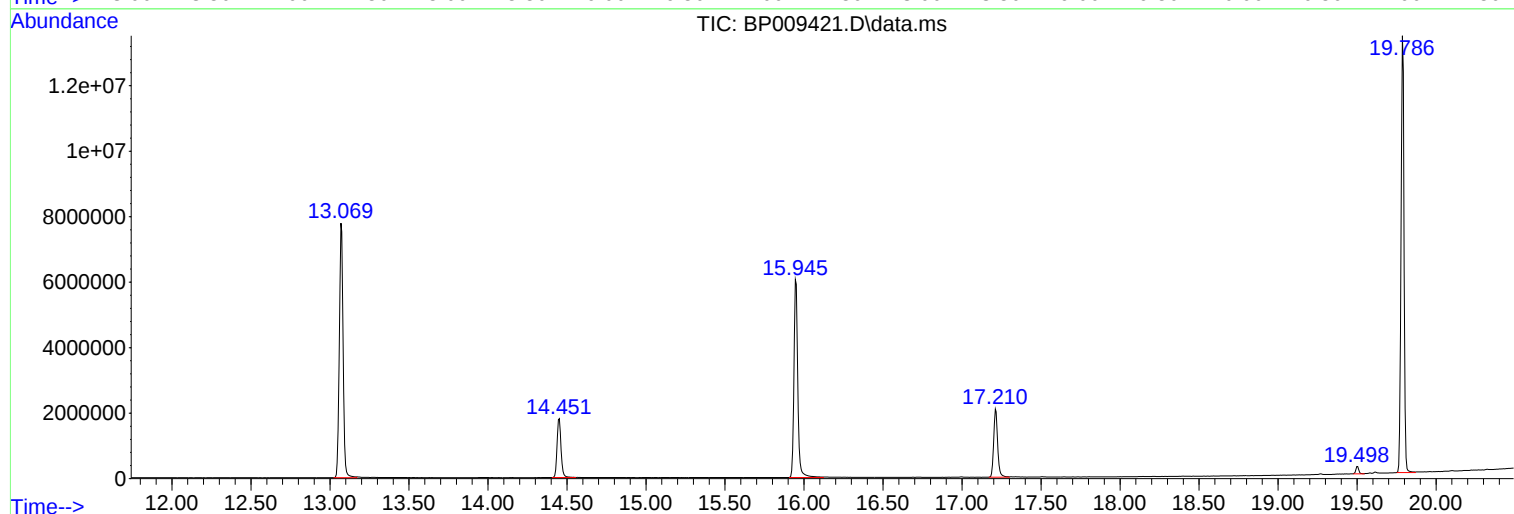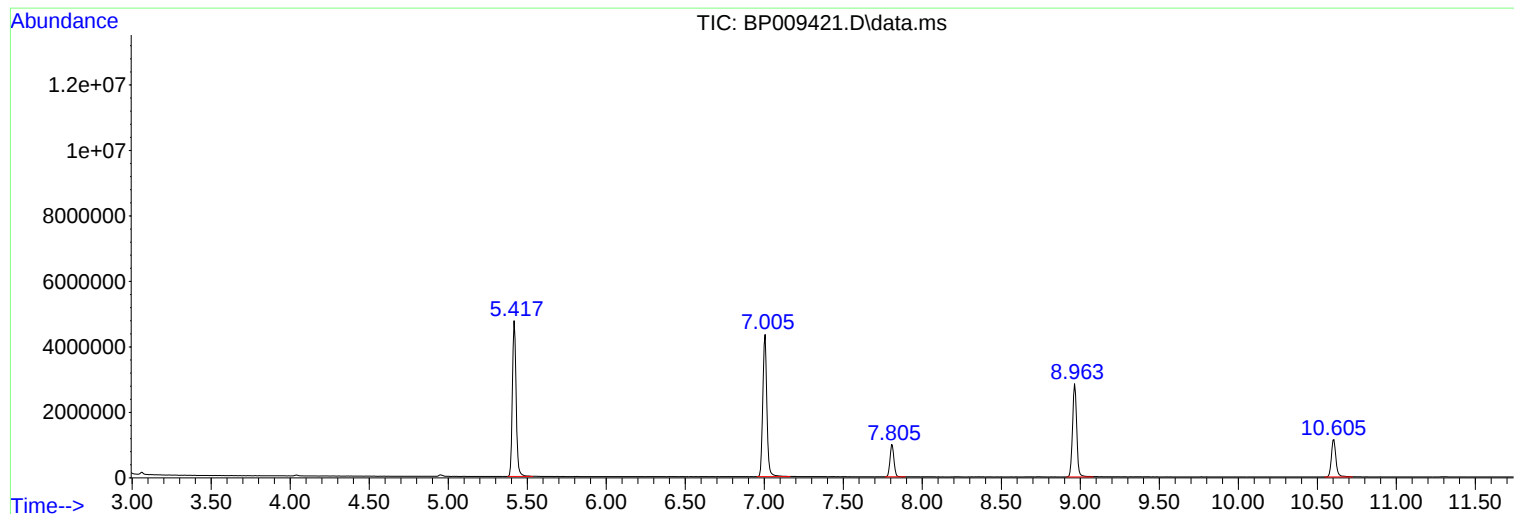

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009421.D
Acq On : 16 Mar 2022 13:51
Operator : CG/JU
Sample : PB142486BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142486BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009421.D
Acq On : 16 Mar 2022 13:51
Operator : CG/JU
Sample : PB142486BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142486BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------