

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
 Data File : BP009436.D
 Acq On : 16 Mar 2022 22:50
 Operator : CG/JU
 Sample : N1954-01 2X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CL-02-031522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	7	11	30	rVB	220887	486136	6.05%	0.548%
2	5.416	406	413	430	rBV	2070001	3804945	47.32%	4.286%
3	7.010	672	684	695	rBV	1936936	3840118	47.76%	4.326%
4	7.110	696	701	712	rVB	150654	300307	3.73%	0.338%
5	7.810	811	820	829	rBV	1636544	2820880	35.08%	3.178%
6	8.963	1004	1016	1028	rBV	1160664	2207985	27.46%	2.487%
7	10.604	1287	1295	1301	rBV	2276410	4285635	53.30%	4.828%
8	10.651	1301	1303	1311	rVB	138876	227043	2.82%	0.256%
9	12.275	1571	1579	1588	rVB	94521	189042	2.35%	0.213%
10	12.493	1610	1616	1620	rBV	78641	144209	1.79%	0.162%
11	13.075	1707	1715	1727	rBV	3875802	6374968	79.28%	7.182%
12	13.287	1746	1751	1758	rVB	88699	142456	1.77%	0.160%
13	13.775	1828	1834	1839	rBV2	77935	154209	1.92%	0.174%
14	13.828	1839	1843	1848	rVB2	50732	86086	1.07%	0.097%
15	14.175	1896	1902	1910	rBV	110332	191997	2.39%	0.216%
16	14.363	1931	1934	1941	rVB	76921	114446	1.42%	0.129%
17	14.451	1941	1949	1956	rBV	3874259	6140783	76.37%	6.918%
18	14.516	1956	1960	1969	rVB	310179	520287	6.47%	0.586%
19	14.663	1981	1985	1995	rVB3	29586	82488	1.03%	0.093%
20	14.851	2012	2017	2023	rBV2	191520	328368	4.08%	0.370%
21	15.075	2049	2055	2060	rBV4	41660	93446	1.16%	0.105%
22	15.322	2094	2097	2102	rVB2	79525	106179	1.32%	0.120%
23	15.504	2123	2128	2141	rVB	399562	683414	8.50%	0.770%
24	15.722	2161	2165	2175	rVV5	57237	151310	1.88%	0.170%
25	15.804	2175	2179	2188	rVB	91814	165043	2.05%	0.186%
26	15.951	2197	2204	2212	rBV	3051344	4798952	59.68%	5.406%
27	16.186	2240	2244	2248	rBV2	132416	228484	2.84%	0.257%
28	16.945	2370	2373	2377	rBV3	51108	101877	1.27%	0.115%
29	16.986	2377	2380	2384	rVV3	100437	165991	2.06%	0.187%
30	17.033	2384	2388	2399	rVB2	171732	317367	3.95%	0.358%
31	17.216	2413	2419	2423	rBV	4535559	7158890	89.03%	8.065%
32	17.257	2423	2426	2433	rVV	2770591	3786157	47.09%	4.265%
33	17.351	2437	2442	2448	rVB	831037	1318486	16.40%	1.485%
34	17.628	2485	2489	2493	rBV	147536	219919	2.74%	0.248%
35	17.733	2504	2507	2513	rVB4	127383	170170	2.12%	0.192%
36	18.092	2563	2568	2570	rBV	291818	440785	5.48%	0.497%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009436.D
Acq On : 16 Mar 2022 22:50
Operator : CG/JU
Sample : N1954-01 2X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-031522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.133	2570	2575	2582	rVB2	575752	1103568	13.72%	1.243%
38	18.210	2585	2588	2593	rVB	189638	278418	3.46%	0.314%
39	18.275	2594	2599	2604	rBV2	617656	1128655	14.04%	1.271%
40	18.575	2647	2650	2654	rBV	226987	261363	3.25%	0.294%
41	19.239	2757	2763	2770	rBV	4008817	5854491	72.81%	6.595%
42	19.592	2814	2823	2831	rBV	3342672	5881659	73.15%	6.626%
43	19.792	2852	2857	2861	rVB	5893041	7759929	96.51%	8.742%
44	20.074	2903	2905	2914	rVB	547414	739674	9.20%	0.833%
45	20.174	2919	2922	2926	rVB	457240	583667	7.26%	0.658%
46	21.327	3112	3118	3122	rBV2	4495548	8040907	100.00%	9.058%
47	23.745	3524	3529	3535	rVB	2422325	4786115	59.52%	5.392%




Sum of corrected areas: 88767304

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009436.D
Acq On : 16 Mar 2022 22:50
Operator : CG/JU
Sample : N1954-01 2X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-031522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

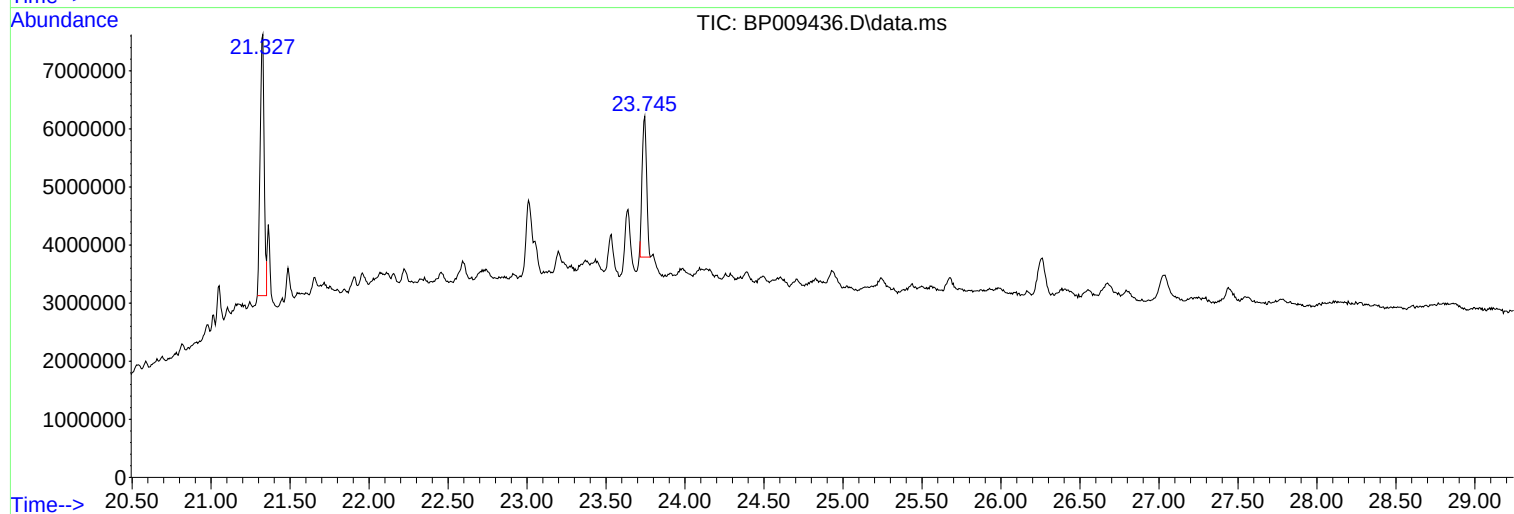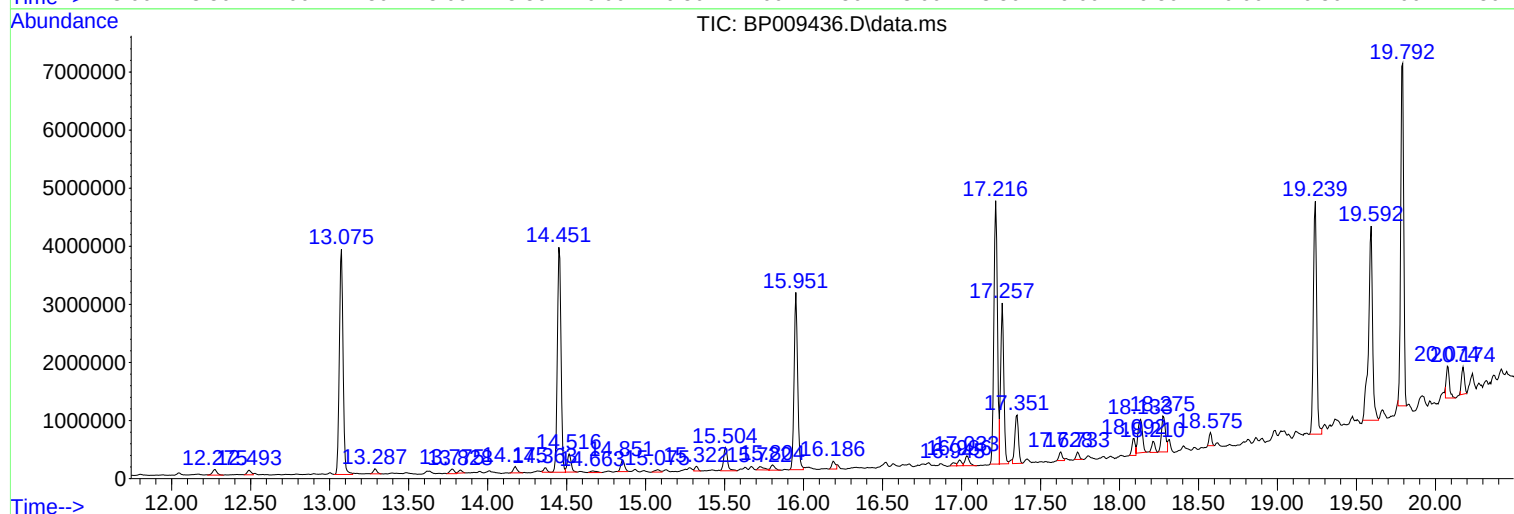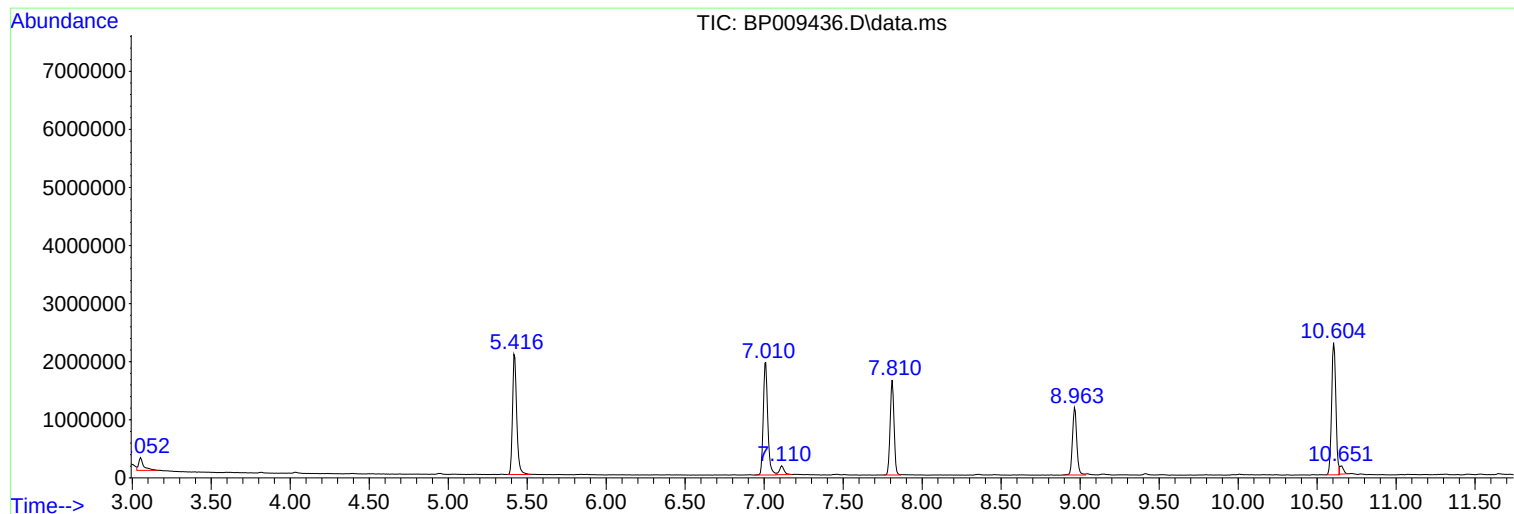

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009436.D
Acq On : 16 Mar 2022 22:50
Operator : CG/JU
Sample : N1954-01 2X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-031522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009436.D
Acq On : 16 Mar 2022 22:50
Operator : CG/JU
Sample : N1954-01 2X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-031522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------