


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
 Data File : BP009419.D
 Acq On : 16 Mar 2022 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

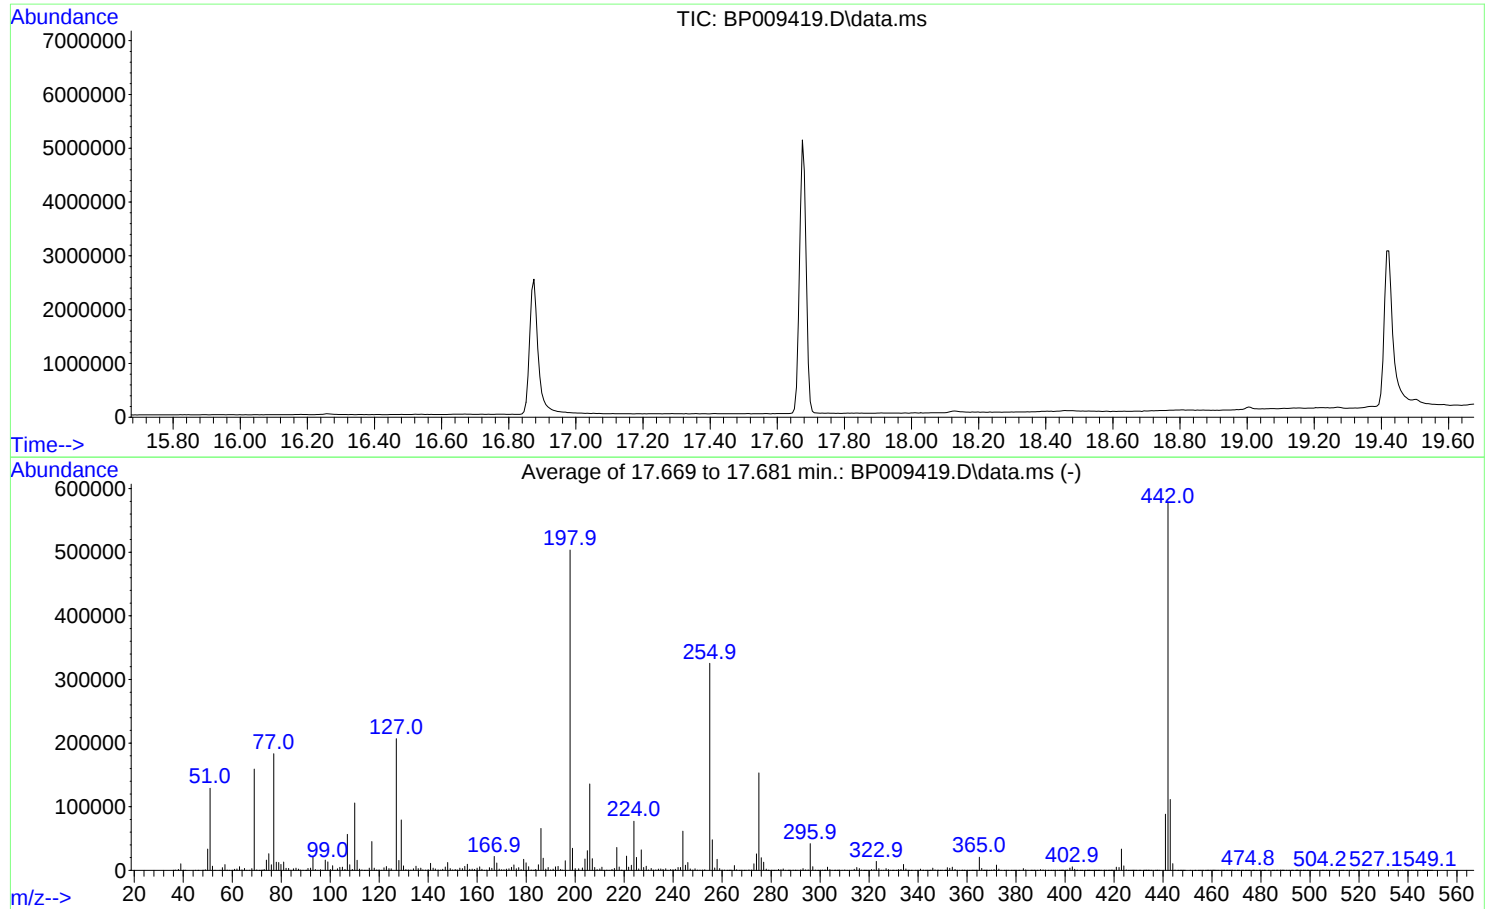




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	128922	PASS
68	69	0.00	2	1.8	2796	PASS
69	198	0.00	100	31.6	159106	PASS
70	69	0.00	2	0.5	863	PASS
127	198	10	80	41.1	207096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	503378	PASS
199	198	5	9	6.9	34682	PASS
275	198	10	60	30.4	153232	PASS
365	198	1	100	4.1	20588	PASS
441	198	0.01	100	17.5	88331	PASS
442	442	100	100	100.0	578155	PASS
443	442	15	24	19.3	111529	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
Data File : BP009419.D
Acq On : 16 Mar 2022 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 16 15:25:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

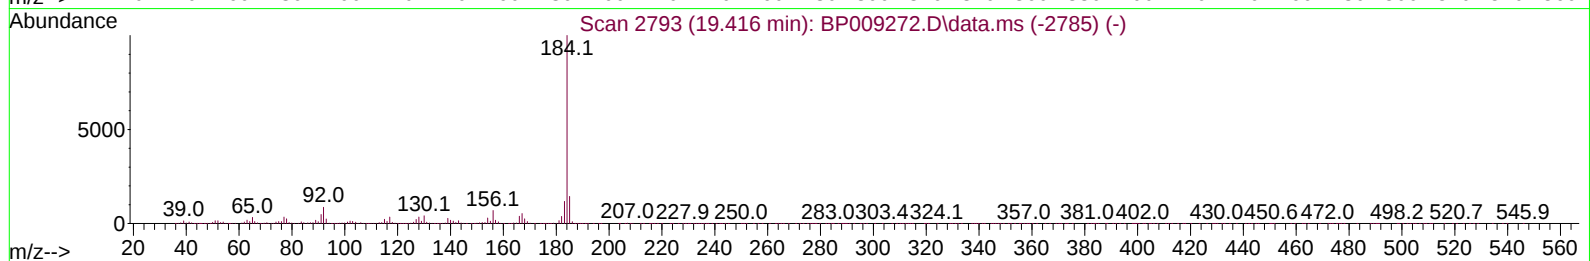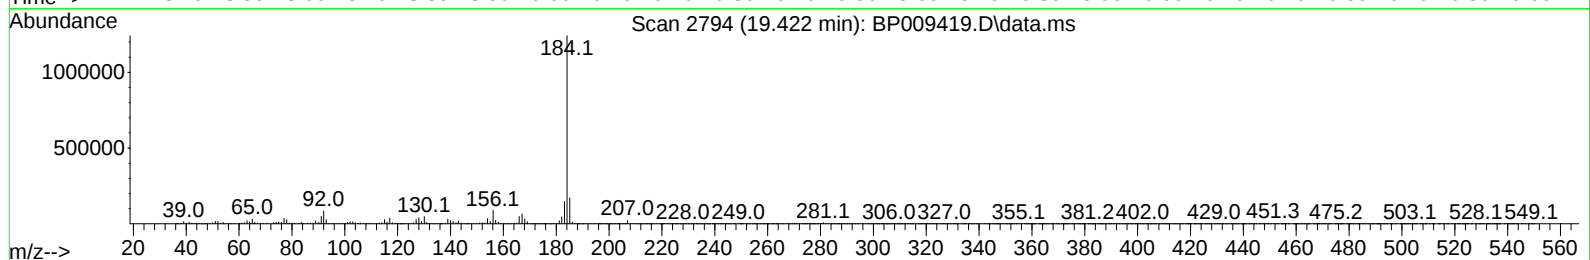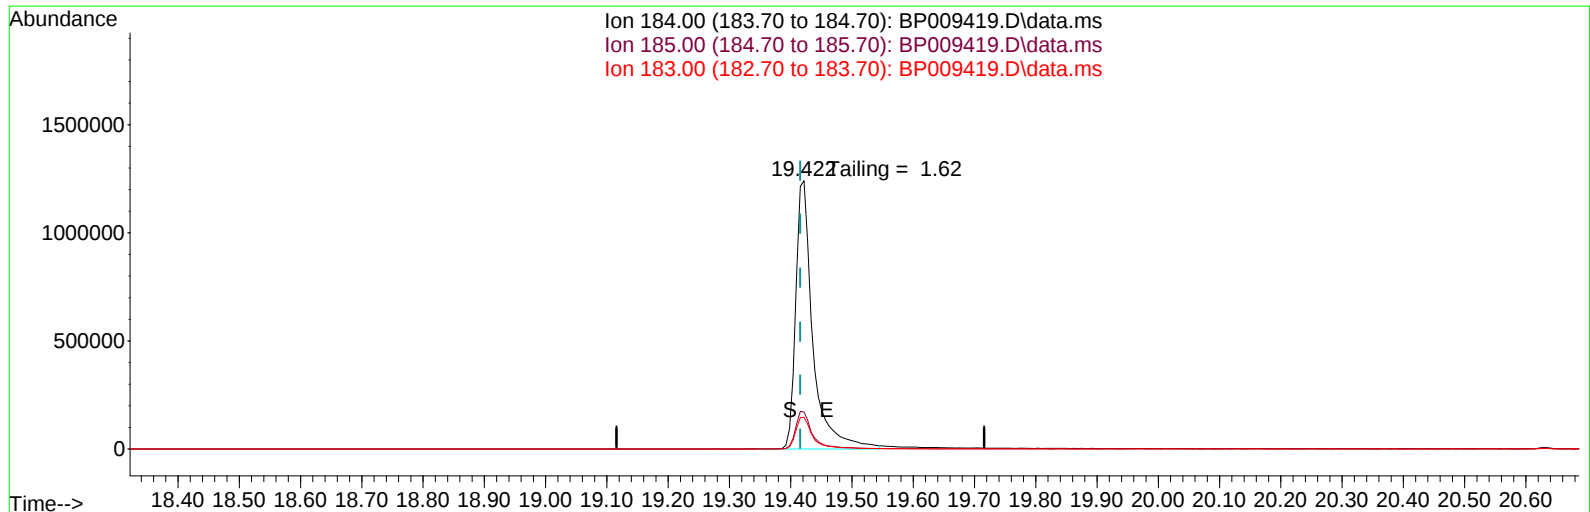

TIC: BP009419.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 52624.66 ng




response 2479687

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.79
183.00	11.70	11.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031622\
 Data File : BP009419.D
 Acq On : 16 Mar 2022 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 16 15:25:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

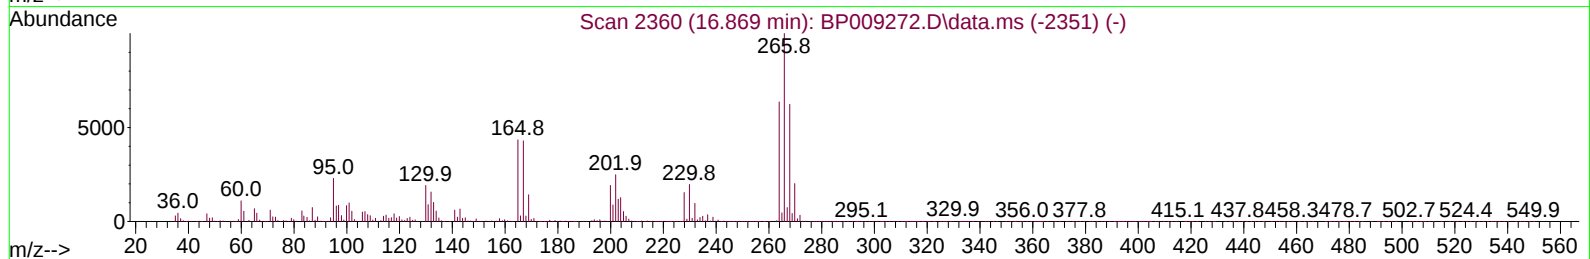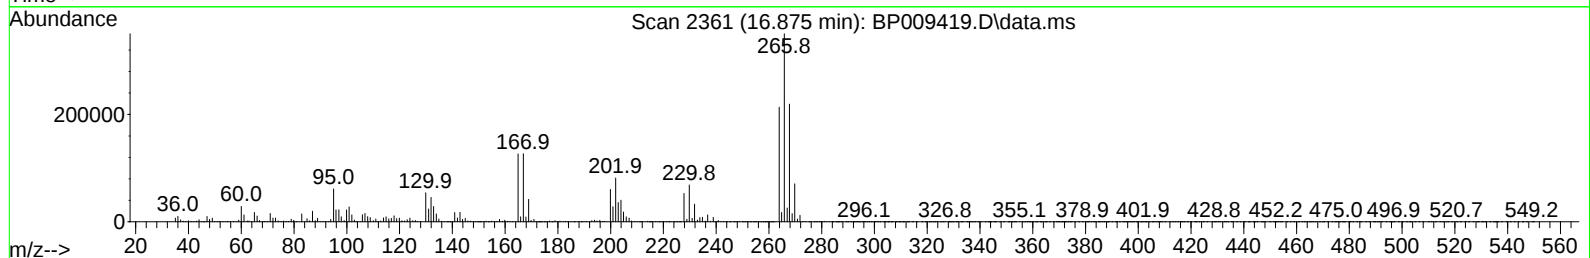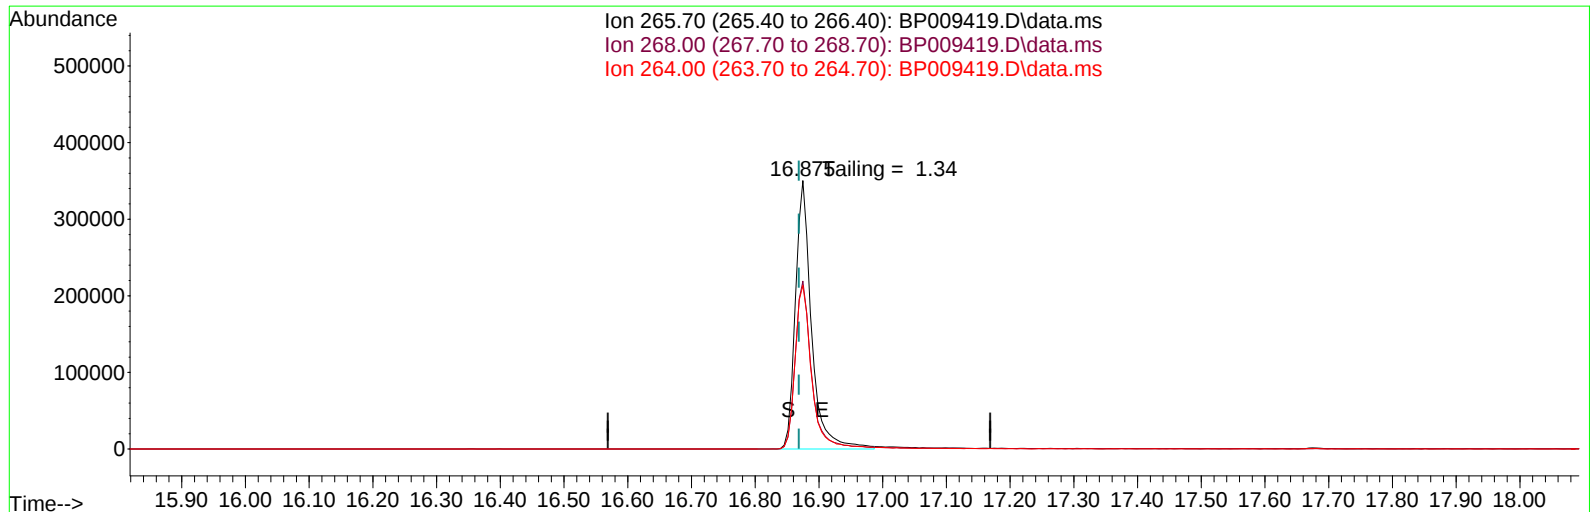

TIC: BP009419.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.006) 443572.83 ng

response 628390

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.52
264.00	63.60	60.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2022	BNA_P	<u>BP009419.D</u>
Compound Name	Response	Retention Time
DDT	1835071	20.63
DDD	28108	20.19
DDE	3177	19.7
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31285	1866356	1.68

Instrument :
BNA_P
ClientSampleId :
DFTPP