

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014136.D
 Acq On : 20 Mar 2023 12:12
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020779

Quant Time: Mar 21 00:44:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	168972	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	747715	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.698	164	529184	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.457	188	1256247	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1261973	20.000	ng/u1	# 0.00
88) Perylene-d12	24.062	264	1234396	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	32506	7.268	ng/uL	0.00
4) Pyridine-d5	3.846	84	230064	18.580	ng/u1	0.00
7) Phenol-d5	7.210	99	302787	20.306	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	183541	21.106	ng/u1	0.00
11) 2-Chlorophenol-d4	7.581	132	234614	20.651	ng/u1	0.00
15) 4-Methylphenol-d8	8.769	113	256711	21.076	ng/u1	0.00
21) Nitrobenzene-d5	9.234	128	121060	20.292	ng/u1	0.00
24) 2-Nitrophenol-d4	9.957	143	146234	20.476	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.498	165	266224	19.812	ng/u1	0.00
31) 4-Chloroaniline-d4	11.016	131	347460	19.539	ng/u1	0.00
46) Dimethylphthalate-d6	14.098	166	875228	19.488	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	965090	20.286	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	145493	18.384	ng/u1	0.00
60) Fluorene-d10	15.692	176	735296	19.319	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	174881	18.419	ng/u1	0.00
73) Anthracene-d10	17.557	188	1213572	19.900	ng/u1	0.00
81) Pyrene-d10	19.774	212	1460963	20.990	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.892	264	1315242	20.031	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	33942	7.030	ng/uL#	88
5) Pyridine	3.869	79	232005	18.476	ng/u1	97
6) Benzaldehyde	7.193	77	184422	24.856	ng/u1	98
8) Phenol	7.240	94	309856	20.150	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.469	93	250176	21.236	ng/u1	99
12) 2-Chlorophenol	7.616	128	239094	20.889	ng/u1	98
13) 2-Methylphenol	8.504	108	241476	21.118	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.587	45	300051	23.584	ng/u1	100
16) Acetophenone	8.887	105	416557	21.170	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.869	70	224457	22.298	ng/u1	99
18) 4-Methylphenol	8.834	108	267252	21.249	ng/u1	97
19) Hexachloroethane	9.146	117	107151	21.374	ng/u1	97
22) Nitrobenzene	9.275	77	324832	20.354	ng/u1	98
23) Isophorone	9.804	82	633745	20.621	ng/u1	98
25) 2-Nitrophenol	9.987	139	150376	20.430	ng/u1	95
26) 2,4-Dimethylphenol	10.046	107	322912	20.043	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.281	93	370611	20.848	ng/u1	99
29) 2,4-Dichlorophenol	10.528	162	260094	19.622	ng/u1	99
30) Naphthalene	10.928	128	816787	19.893	ng/u1	99
32) 4-Chloroaniline	11.040	127	351142	19.623	ng/u1	96
33) Hexachlorobutadiene	11.204	225	197795	18.752	ng/u1	97
34) Caprolactam	11.834	113	47680	11.078	ng/u1	93
35) 4-Chloro-3-methylphenol	12.157	107	313050	20.424	ng/u1	96
36) 2-Methylnaphthalene	12.528	142	570399	19.806	ng/u1	98


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014136.D
 Acq On : 20 Mar 2023 12:12
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020779

Quant Time: Mar 21 00:44:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.745	142	565794	19.546	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.892	216	364781	19.062	ng/ul	100
40) Hexachlorocyclopentadiene	12.869	237	208760	15.235	ng/ul	98
41) 2,4,6-Trichlorophenol	13.134	196	239560	19.928	ng/ul	99
42) 2,4,5-Trichlorophenol	13.210	196	263661	19.985	ng/ul	98
43) 1,1'-Biphenyl	13.534	154	816025	20.029	ng/ul	99
44) 2-Chloronaphthalene	13.575	162	654809	20.237	ng/ul	99
45) 2-Nitroaniline	13.787	65	203159	21.228	ng/ul	97
47) Dimethylphthalate	14.151	163	867743	19.520	ng/ul	99
48) 2,6-Dinitrotoluene	14.275	165	180767	20.568	ng/ul	99
50) Acenaphthylene	14.422	152	1009447	20.218	ng/ul	100
51) 3-Nitroaniline	14.610	138	163848	21.056	ng/ul	95
52) Acenaphthene	14.763	153	698528	20.013	ng/ul	100
53) 2,4-Dinitrophenol	14.816	184	105060	16.007	ng/ul	96
55) 4-Nitrophenol	14.916	109	142427	16.660	ng/ul	86
56) Dibenzofuran	15.098	168	999367	19.681	ng/ul	98
57) 2,4-Dinitrotoluene	15.063	165	266444	20.291	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.322	232	243971	19.330	ng/ul	99
59) Diethylphthalate	15.504	149	897869	19.914	ng/ul	99
61) Fluorene	15.745	166	827528	19.660	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.733	204	446898	19.237	ng/ul	99
63) 4-Nitroaniline	15.775	138	171692	21.465	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.828	198	167578	18.500	ng/ul	98
67) N-Nitrosodiphenylamine	15.951	169	712475	20.081	ng/ul	99
68) 4-Bromophenyl-phenylether	16.633	248	296060	19.495	ng/ul	97
69) Hexachlorobenzene	16.751	284	346619	19.368	ng/ul	97
70) Atrazine	16.904	200	301479	19.701	ng/ul	99
71) Pentachlorophenol	17.104	266	205498	17.567	ng/ul	98
72) Phenanthrene	17.498	178	1357045	19.805	ng/ul	100
74) Anthracene	17.586	178	1395242	20.083	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.498	216	386959	20.071	ng/ul	98
76) Pentachlorobenzene	15.016	250	393876	19.667	ng/ul	99
77) Carbazole	17.857	167	1238851	20.216	ng/ul	99
78) Di-n-butylphthalate	18.386	149	1634182	21.338	ng/ul	100
80) Fluoranthene	19.451	202	1707096	21.518	ng/ul#	96
82) Pyrene	19.804	202	1770370	21.392	ng/ul	96
83) Butylbenzylphthalate	20.657	149	765019	22.926	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.445	252	627556	19.425	ng/ul	99
85) Benzo(a)anthracene	21.516	228	1763316	19.866	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.410	149	1134550	22.741	ng/ul	99
87) Chrysene	21.574	228	1657372	19.592	ng/ul	100
89) Di-n-octyl phthalate	22.374	149	1935615	24.851	ng/ul	100
90) Benzo(b)fluoranthene	23.280	252	1712039	20.814	ng/ul	98
91) Benzo(k)fluoranthene	23.333	252	1609496	20.521	ng/ul	99
93) Benzo(a)pyrene	23.945	252	1430092	19.989	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.715	276	1664968	17.580	ng/ul	98
95) Dibenzo(a,h)anthracene	26.733	278	1400138	17.787	ng/ul	98
96) Benzo(g,h,i)perylene	27.539	276	1338939	17.687	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed

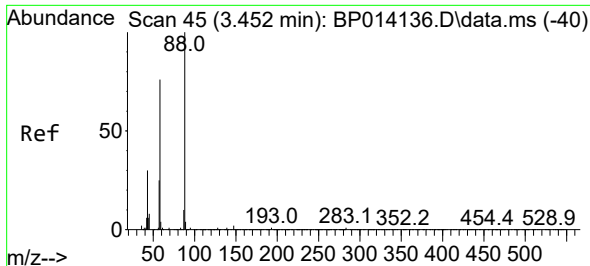

#2
 1,4-Dioxane
 Concen: 7.030 ng/uL
 RT: 3.452 min Scan# 45
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12




Instrument :
 BNA_P
 ClientSampleId :
 SST020779


Tgt Ion: 88 Resp: 33942
 Ion Ratio Lower Upper
 88 100
 43 31.1 23.9 35.9
 58 76.0 50.2 75.2#

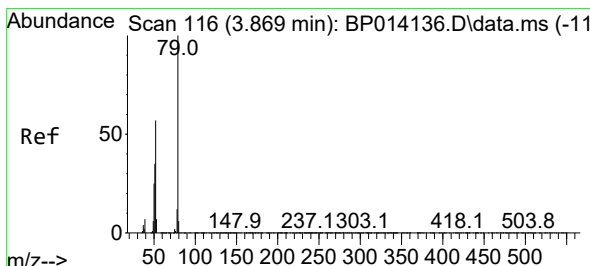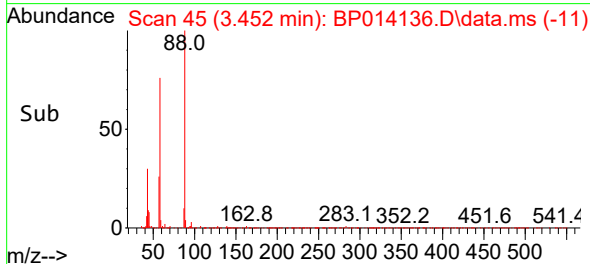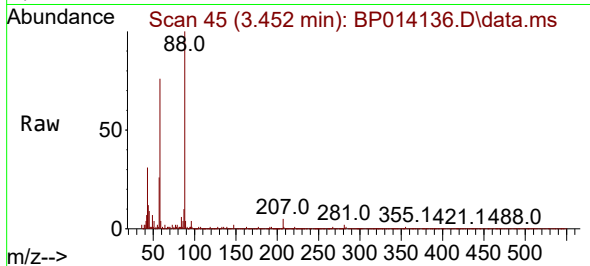

#5
 Pyridine
 Concen: 18.476 ng/uL
 RT: 3.869 min Scan# 116
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12

Tgt Ion: 79 Resp: 232005
 Ion Ratio Lower Upper
 79 100
 52 72.5 55.1 82.7
 51 35.8 28.9 43.3


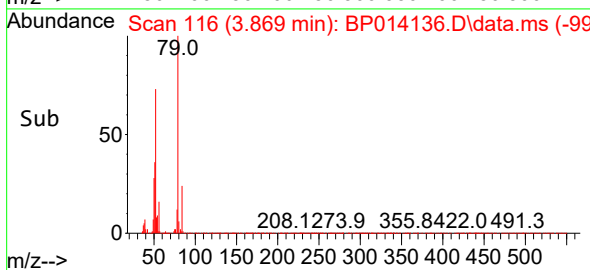

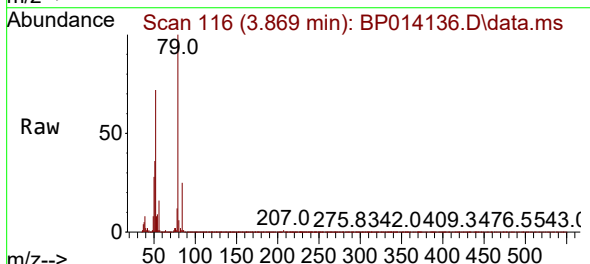




#6
Benzaldehyde
Concen: 24.856 ng/ul
RT: 7.193 min Scan# 681
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion: 77 Resp: 184422
Ion Ratio Lower Upper
77 100
105 94.6 74.2 111.2
106 89.3 69.8 104.8



#8
Phenol
Concen: 20.150 ng/ul
RT: 7.240 min Scan# 689
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion: 94 Resp: 309856
Ion Ratio Lower Upper
94 100
65 31.6 25.2 37.8
66 45.5 37.2 55.8



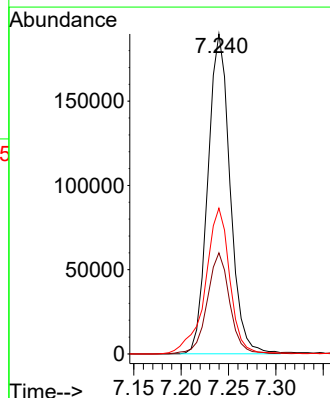
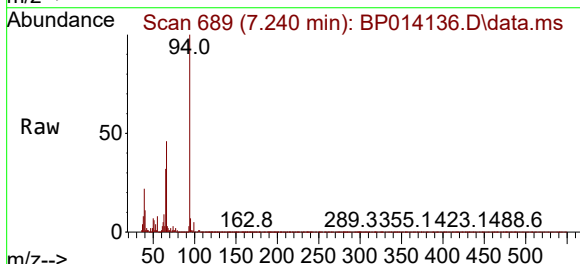




#10
Bis(2-Chloroethyl)ether
Concen: 21.236 ng/ul
RT: 7.469 min Scan# 728
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion: 93 Resp: 250176
Ion Ratio Lower Upper
93 100
63 72.6 58.8 88.2
95 31.5 25.8 38.6



#12
2-Chlorophenol
Concen: 20.889 ng/ul
RT: 7.616 min Scan# 753
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:128 Resp: 239094
Ion Ratio Lower Upper
128 100
64 49.8 38.3 57.5
130 31.8 25.7 38.5





#13

2-Methylphenol

Concen: 21.118 ng/ul

RT: 8.504 min Scan# 904

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :





SSTD020779

Tgt Ion:108 Resp: 241476

Ion Ratio Lower Upper

108 100

107 90.4 70.5 105.7

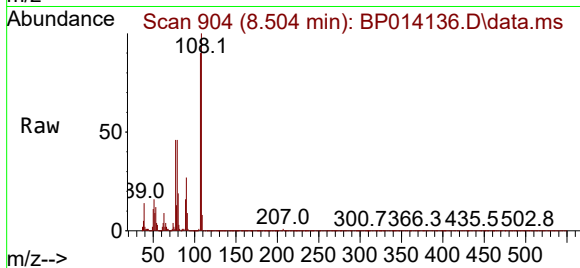

#14

2,2'-oxybis(1-Chloropropane)

Concen: 23.584 ng/ul

RT: 8.587 min Scan# 918

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion: 45 Resp: 300051


Ion Ratio Lower Upper

45 100

77 17.4 14.2 21.2

79 13.2 10.6 15.8









#16
Acetophenone
Concen: 21.170 ng/ul
RT: 8.887 min Scan# 969
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:105 Resp: 416557
Ion Ratio Lower Upper
105 100
77 81.1 65.4 98.2
51 26.7 21.8 32.8



#17
N-Nitroso-di-n-propylamine
Concen: 22.298 ng/ul
RT: 8.869 min Scan# 966
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion: 70 Resp: 224457
Ion Ratio Lower Upper
70 100
42 50.8 40.9 61.3
101 9.8 7.9 11.9
130 19.2 16.6 25.0



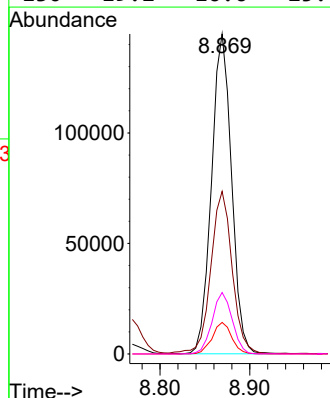





#18
4-Methylphenol
Concen: 21.249 ng/ul
RT: 8.834 min Scan# 960
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:108 Resp: 267252
Ion Ratio Lower Upper
108 100
107 108.9 89.8 134.6



#19
Hexachloroethane
Concen: 21.374 ng/ul
RT: 9.146 min Scan# 1013
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:117 Resp: 107151
Ion Ratio Lower Upper
117 100
201 119.4 91.7 137.5
199 72.9 59.1 88.7



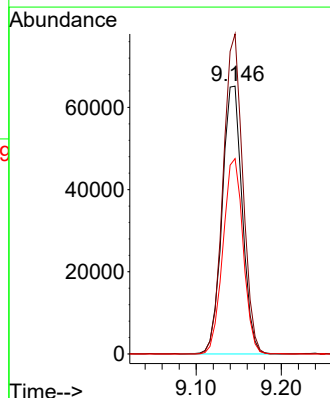
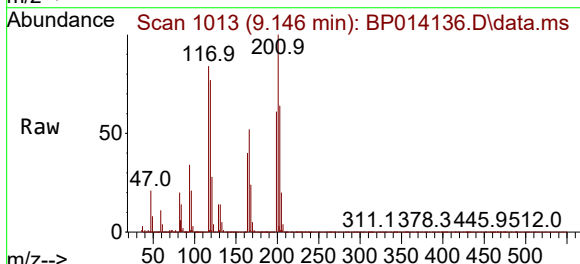




#22
Nitrobenzene
Concen: 20.354 ng/ul
RT: 9.275 min Scan# 1035
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion: 77 Resp: 324832
Ion Ratio Lower Upper
77 100
123 41.9 32.6 48.8
65 13.6 11.2 16.8



#23
Isophorone
Concen: 20.621 ng/ul
RT: 9.804 min Scan# 1125
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion: 82 Resp: 633745
Ion Ratio Lower Upper
82 100
95 8.0 7.1 10.7
138 17.2 13.3 19.9









#25
2-Nitrophenol
Concen: 20.430 ng/ul
RT: 9.987 min Scan# 1156
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:139 Resp: 150376
Ion Ratio Lower Upper
139 100
65 57.4 46.6 70.0
109 37.0 34.5 51.7



#26
2,4-Dimethylphenol
Concen: 20.043 ng/ul
RT: 10.046 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:107 Resp: 322912
Ion Ratio Lower Upper
107 100
121 48.2 37.1 55.7
122 76.1 61.2 91.8









#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.848 ng/ul
 RT: 10.281 min Scan# 1206
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020779


Tgt Ion: 93 Resp: 370611
 Ion Ratio Lower Upper
 93 100
 95 32.4 25.6 38.4
 123 10.3 8.5 12.7



#29
 2,4-Dichlorophenol
 Concen: 19.622 ng/ul
 RT: 10.528 min Scan# 1248
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12

Tgt Ion: 162 Resp: 260094
 Ion Ratio Lower Upper
 162 100
 164 66.4 52.0 78.0
 98 36.5 29.1 43.7


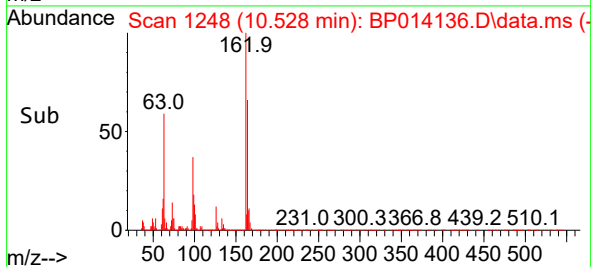

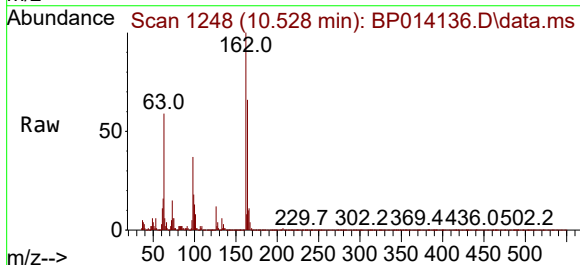




#30
Naphthalene
Concen: 19.893 ng/ul
RT: 10.928 min Scan# 1316
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:128 Resp: 816787
Ion Ratio Lower Upper
128 100
129 10.6 8.5 12.7
127 13.2 11.0 16.4



#32
4-Chloroaniline
Concen: 19.623 ng/ul
RT: 11.040 min Scan# 1335
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:127 Resp: 351142
Ion Ratio Lower Upper
127 100
129 33.3 24.9 37.3









#33
Hexachlorobutadiene
Concen: 18.752 ng/ul
RT: 11.204 min Scan# 1363
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:225 Resp: 197795
Ion Ratio Lower Upper
225 100
223 63.1 48.0 72.0
227 64.6 50.3 75.5



#34
Caprolactam
Concen: 11.078 ng/ul
RT: 11.834 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:113 Resp: 47680
Ion Ratio Lower Upper
113 100
55 146.6 124.0 186.0
56 117.5 102.0 153.0




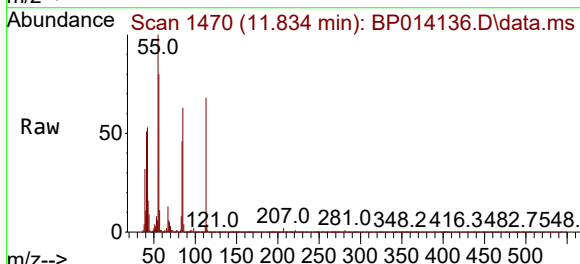




#35
4-Chloro-3-methylphenol
Concen: 20.424 ng/ul
RT: 12.157 min Scan# 1525
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:107 Resp: 313050
Ion Ratio Lower Upper
107 100
144 22.9 19.4 29.0
142 70.4 59.6 89.4

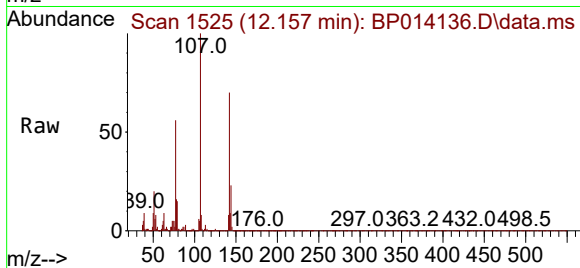

#36
2-Methylnaphthalene
Concen: 19.806 ng/ul
RT: 12.528 min Scan# 1588
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:142 Resp: 570399
Ion Ratio Lower Upper
142 100
141 91.9 71.7 107.5



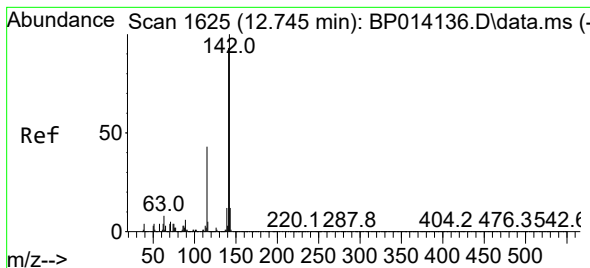

#37

1-Methylnaphthalene

Concen: 19.546 ng/ul

RT: 12.745 min Scan# 1625

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:142 Resp: 565794

Ion Ratio Lower Upper

142 100

141 93.0 73.8 110.6

116 4.7 3.7 5.5

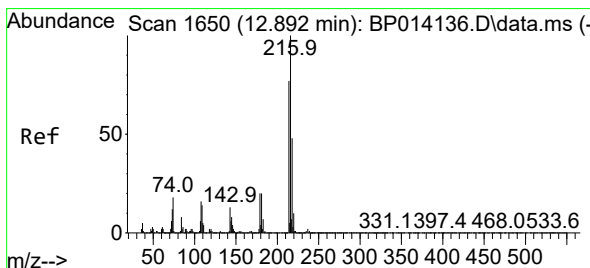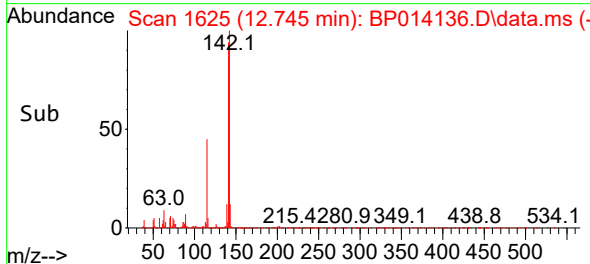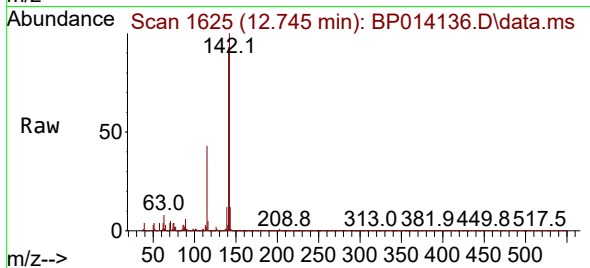

#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.062 ng/ul

RT: 12.892 min Scan# 1650

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Tgt Ion:216 Resp: 364781




Ion Ratio Lower Upper


216 100

214 76.9 61.7 92.5

179 20.4 16.2 24.4

108 15.9 13.2 19.8


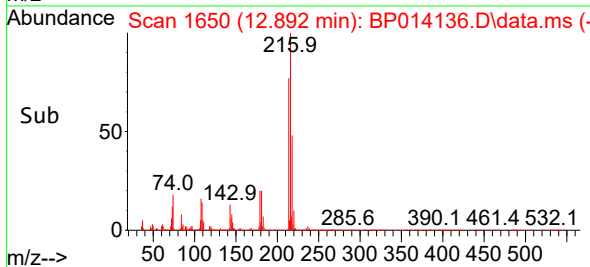

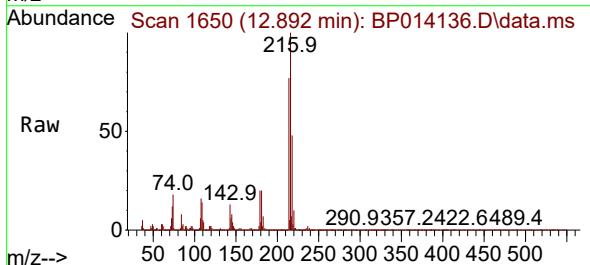




#40
Hexachlorocyclopentadiene
Concen: 15.235 ng/ul
RT: 12.869 min Scan# 1646
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:237 Resp: 208760
Ion Ratio Lower Upper
237 100
235 62.3 49.0 73.6
272 13.3 9.6 14.4



#41
2,4,6-Trichlorophenol
Concen: 19.928 ng/ul
RT: 13.134 min Scan# 1691
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:196 Resp: 239560
Ion Ratio Lower Upper
196 100
198 98.4 78.5 117.7
200 30.9 25.4 38.0






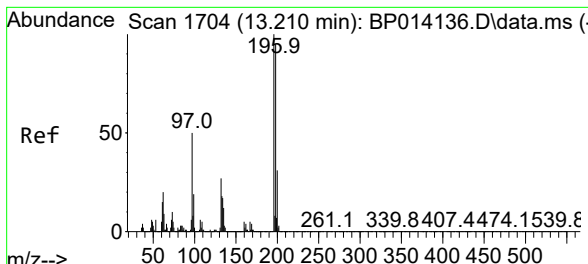


#42
 2,4,5-Trichlorophenol
 Concen: 19.985 ng/ul
 RT: 13.210 min Scan# 1704
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020779

Tgt Ion:196 Resp: 263661




Ion	Ratio	Lower	Upper
196	100		
198	95.0	77.6	116.4
200	31.3	25.3	37.9

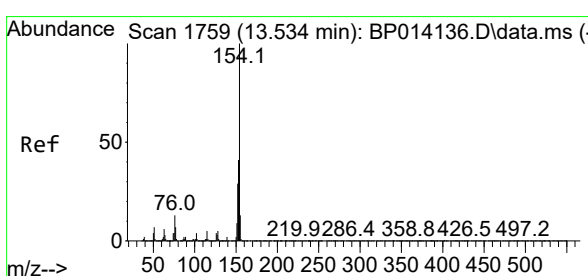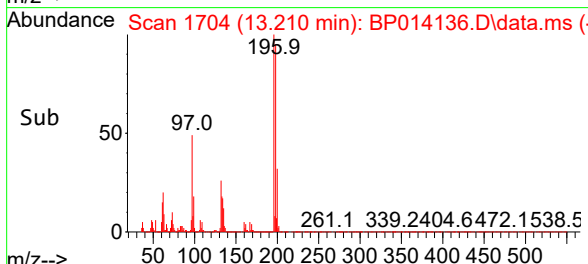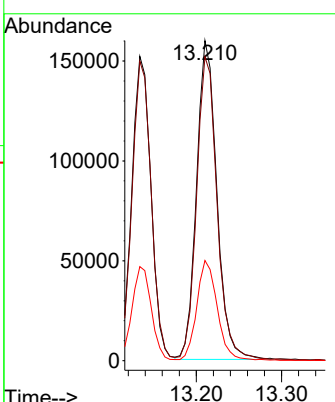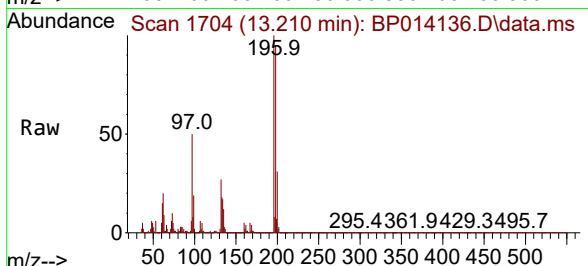


#43
 1,1'-Biphenyl
 Concen: 20.029 ng/ul
 RT: 13.534 min Scan# 1759
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12

Tgt Ion:154 Resp: 816025

Ion	Ratio	Lower	Upper
154	100		
153	41.4	32.6	49.0
76	12.7	9.4	14.0

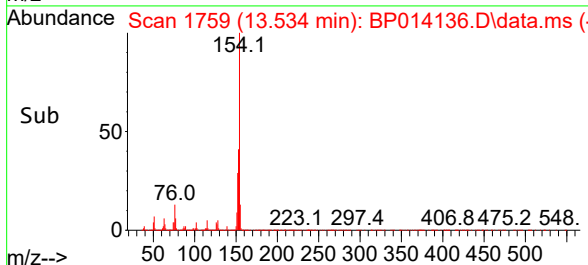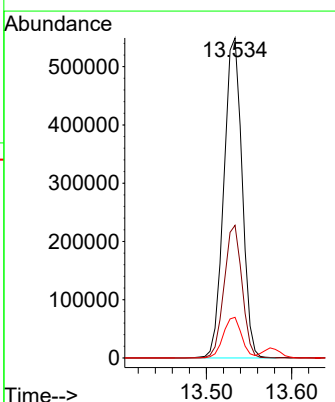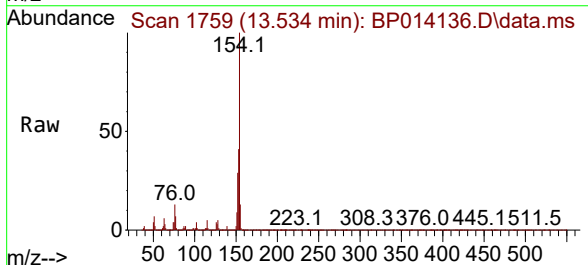



#44

2-Chloronaphthalene

Concen: 20.237 ng/ul

RT: 13.575 min Scan# 1766

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:162 Resp: 654809

Ion Ratio Lower Upper

162 100

164 32.4 26.0 39.0

127 40.4 31.3 46.9

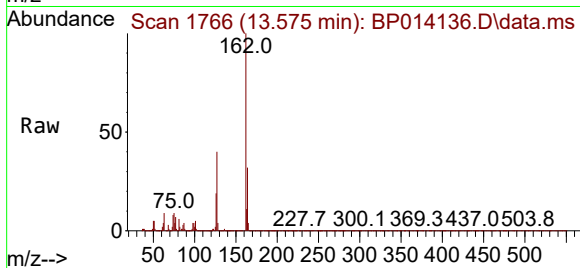

#45

2-Nitroaniline

Concen: 21.228 ng/ul

RT: 13.787 min Scan# 1802

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion: 65 Resp: 203159


Ion Ratio Lower Upper

65 100

92 69.0 56.3 84.5

138 97.3 81.4 122.2









#47
Dimethylphthalate
Concen: 19.520 ng/ul
RT: 14.151 min Scan# 1864
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:163 Resp: 867743
Ion Ratio Lower Upper
163 100
194 4.3 3.6 5.4
164 9.9 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 20.568 ng/ul
RT: 14.275 min Scan# 1885
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:165 Resp: 180767
Ion Ratio Lower Upper
165 100
89 63.6 51.7 77.5
121 20.9 17.5 26.3

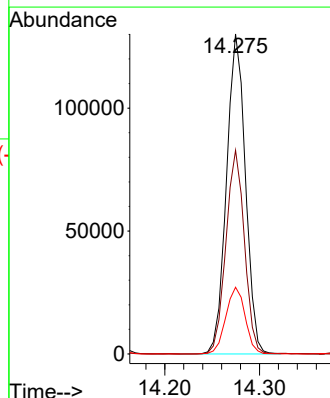



#50

Acenaphthylene

Concen: 20.218 ng/ul

RT: 14.422 min Scan# 1910

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:152 Resp: 1009447

Ion Ratio Lower Upper

152 100

151 20.1 16.2 24.2

153 13.1 10.4 15.6

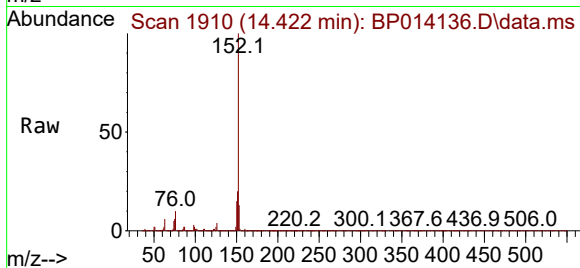

#51

3-Nitroaniline

Concen: 21.056 ng/ul

RT: 14.610 min Scan# 1942

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:138 Resp: 163848


Ion Ratio Lower Upper

138 100

108 12.2 10.5 15.7

92 129.6 98.5 147.7









#52
Acenaphthene
Concen: 20.013 ng/ul
RT: 14.763 min Scan# 1968
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:153 Resp: 698528
Ion Ratio Lower Upper
153 100
152 47.3 37.7 56.5
154 87.8 70.4 105.6



#53
2,4-Dinitrophenol
Concen: 16.007 ng/ul
RT: 14.816 min Scan# 1977
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:184 Resp: 105060
Ion Ratio Lower Upper
184 100
63 68.1 51.9 77.9
154 69.6 58.8 88.2









#55
4-Nitrophenol
Concen: 16.660 ng/ul
RT: 14.916 min Scan# 1994
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:109 Resp: 142427
Ion Ratio Lower Upper
109 100
139 107.8 74.5 111.7
65 121.1 86.6 130.0



#56
Dibenzofuran
Concen: 19.681 ng/ul
RT: 15.098 min Scan# 2025
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:168 Resp: 999367
Ion Ratio Lower Upper
168 100
139 38.7 31.8 47.6




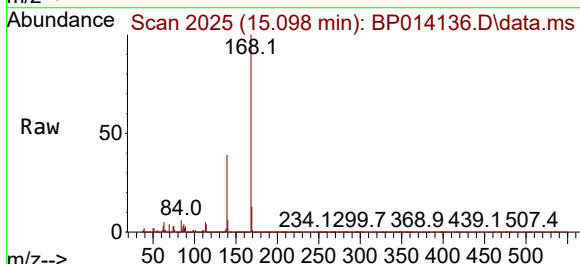




#57
2,4-Dinitrotoluene
Concen: 20.291 ng/ul
RT: 15.063 min Scan# 2019
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:165 Resp: 266444
Ion Ratio Lower Upper
165 100
63 43.4 34.6 52.0
182 2.8 2.2 3.2

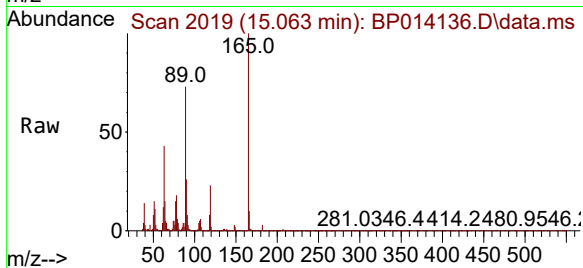

#58
2,3,4,6-Tetrachlorophenol
Concen: 19.330 ng/ul
RT: 15.322 min Scan# 2063
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:232 Resp: 243971
Ion Ratio Lower Upper
232 100
131 42.3 34.1 51.1
130 2.4 2.1 3.1
166 30.1 23.0 34.6



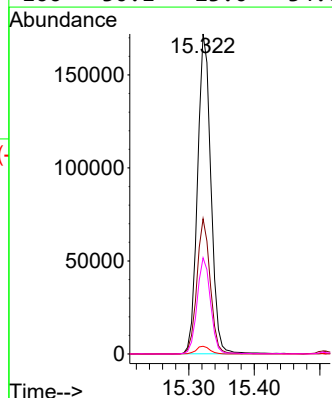
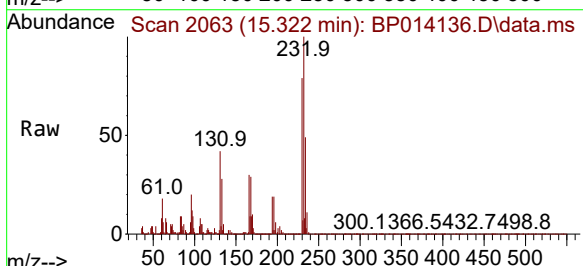




#59
Diethylphthalate
Concen: 19.914 ng/ul
RT: 15.504 min Scan# 2094
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:149 Resp: 897869
Ion Ratio Lower Upper
149 100
177 21.8 18.2 27.2
150 12.4 10.0 15.0



#61
Fluorene
Concen: 19.660 ng/ul
RT: 15.745 min Scan# 2135
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:166 Resp: 827528
Ion Ratio Lower Upper
166 100
165 99.3 78.9 118.3
167 13.5 11.0 16.6




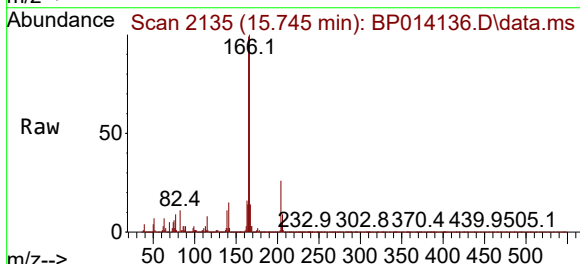




#62
4-Chlorophenyl-phenylether
Concen: 19.237 ng/ul
RT: 15.733 min Scan# 2133
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:204 Resp: 446898
Ion Ratio Lower Upper
204 100
206 33.2 26.6 39.8
141 60.7 49.2 73.8



#63
4-Nitroaniline
Concen: 21.465 ng/ul
RT: 15.775 min Scan# 2140
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:138 Resp: 171692
Ion Ratio Lower Upper
138 100
92 58.2 44.5 66.7
108 101.2 87.2 130.8









#66
4,6-Dinitro-2-methylphenol
Concen: 18.500 ng/ul
RT: 15.828 min Scan# 2149
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:198 Resp: 167578
Ion Ratio Lower Upper
198 100
182 4.3 3.0 4.6
77 26.5 20.3 30.5

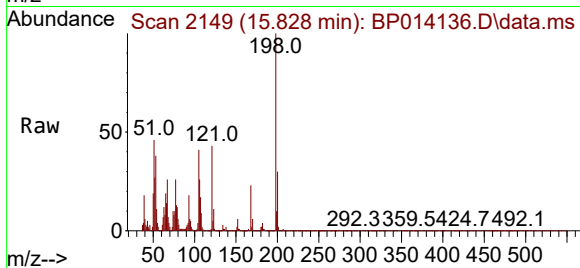

#67
N-Nitrosodiphenylamine
Concen: 20.081 ng/ul
RT: 15.951 min Scan# 2170
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:169 Resp: 712475
Ion Ratio Lower Upper
169 100
168 66.2 53.7 80.5
167 36.6 28.6 43.0









#68
4-Bromophenyl-phenylether
Concen: 19.495 ng/ul
RT: 16.633 min Scan# 2286
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:248 Resp: 296060
Ion Ratio Lower Upper
248 100
250 96.8 78.8 118.2
141 72.9 60.8 91.2

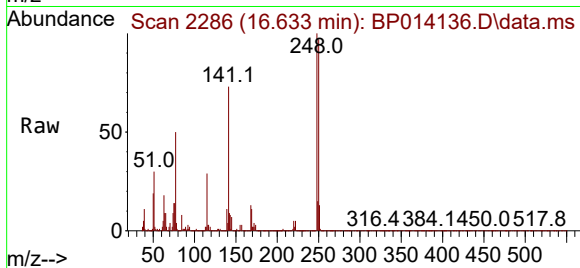

#69
Hexachlorobenzene
Concen: 19.368 ng/ul
RT: 16.751 min Scan# 2306
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:284 Resp: 346619
Ion Ratio Lower Upper
284 100
142 31.9 23.2 34.8
249 32.8 25.7 38.5

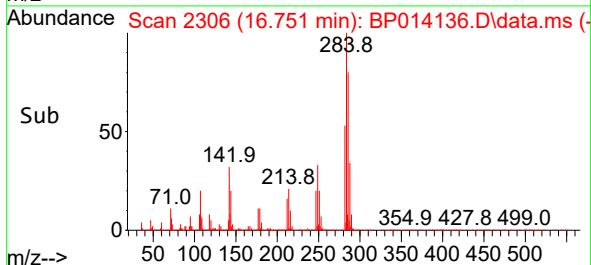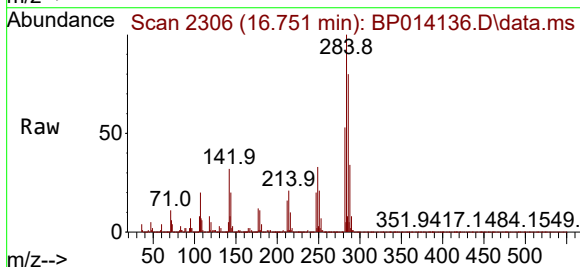



#70

Atrazine

Concen: 19.701 ng/ul

RT: 16.904 min Scan# 2332

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:200 Resp: 301479

Ion Ratio Lower Upper

200 100

173 24.5 19.0 28.4

215 47.8 38.5 57.7

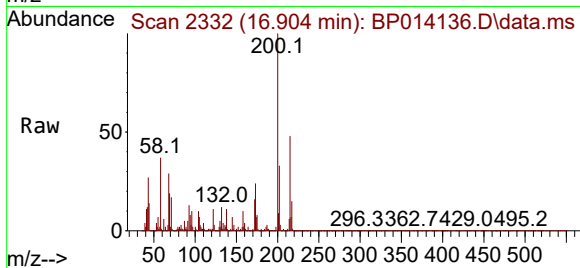

#71

Pentachlorophenol

Concen: 17.567 ng/ul

RT: 17.104 min Scan# 2366

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:266 Resp: 205498


Ion Ratio Lower Upper

266 100

264 61.1 48.4 72.6

268 65.5 50.4 75.6

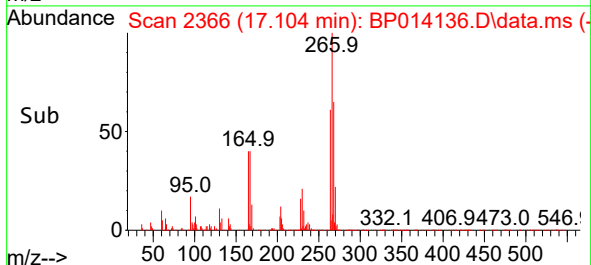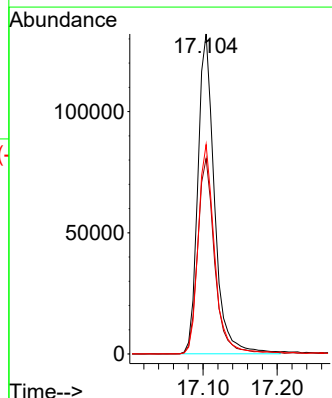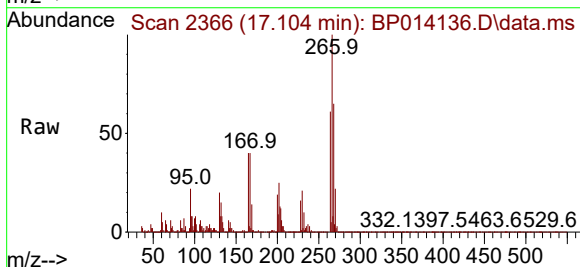



#72

Phenanthrene

Concen: 19.805 ng/ul

RT: 17.498 min Scan# 2433

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:178 Resp: 1357045

Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.4

176 19.2 15.4 23.0

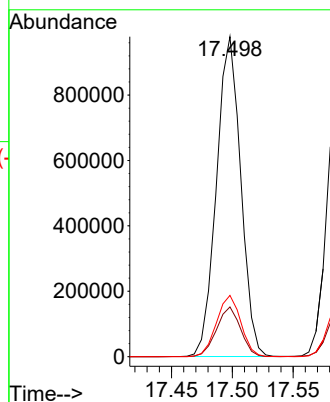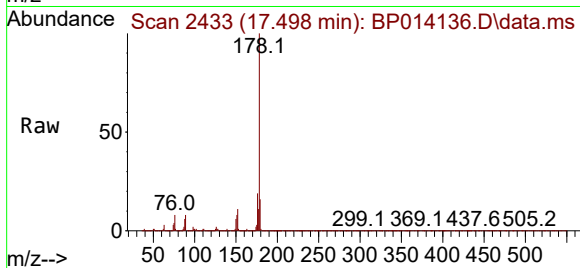

#74

Anthracene

Concen: 20.083 ng/ul

RT: 17.586 min Scan# 2448

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:178 Resp: 1395242


Ion Ratio Lower Upper

178 100

179 15.3 12.5 18.7

176 18.5 15.1 22.7





#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.071 ng/uL

RT: 13.498 min Scan# 1753

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:216 Resp: 386959

Ion Ratio Lower Upper

216 100

214 78.9 61.4 92.2

218 48.1 39.1 58.7

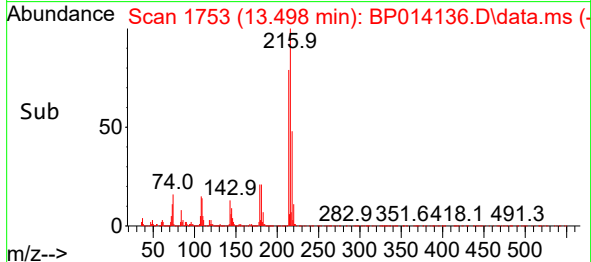

#76

Pentachlorobenzene

Concen: 19.667 ng/uL

RT: 15.016 min Scan# 2011

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:250 Resp: 393876


Ion Ratio Lower Upper

250 100

248 62.8 51.0 76.4

252 63.7 50.8 76.2

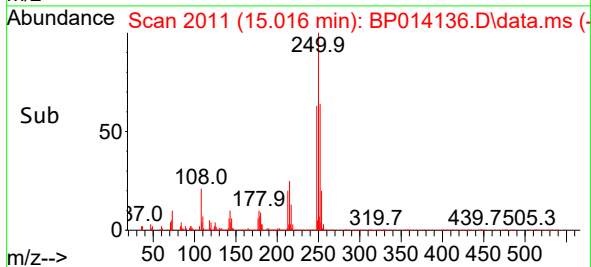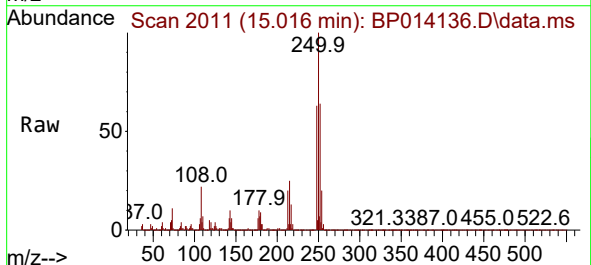







#77
 Carbazole
 Concen: 20.216 ng/ul
 RT: 17.857 min Scan# 2494
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020779

Tgt Ion:167 Resp: 1238851




Ion	Ratio	Lower	Upper
167	100		
166	21.3	17.5	26.3
139	13.1	10.5	15.7




#78
 Di-n-butylphthalate
 Concen: 21.338 ng/ul
 RT: 18.386 min Scan# 2584
 Delta R.T. 0.000 min
 Lab File: BP014136.D
 Acq: 20 Mar 2023 12:12

Tgt Ion:149 Resp: 1634182

Ion	Ratio	Lower	Upper
149	100		
150	9.3	7.4	11.2
104	5.4	4.6	6.8




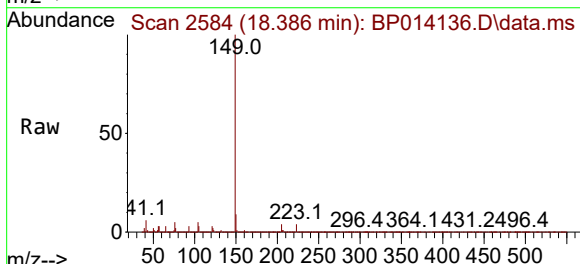




#80
Fluoranthene
Concen: 21.518 ng/ul
RT: 19.451 min Scan# 2765
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:202 Resp: 1707096
Ion Ratio Lower Upper
202 100
101 9.8 6.6 10.0
100 7.5 5.0 7.4#



#82
Pyrene
Concen: 21.392 ng/ul
RT: 19.804 min Scan# 2825
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:202 Resp: 1770370
Ion Ratio Lower Upper
202 100
101 11.3 7.8 11.8
100 9.5 6.5 9.7

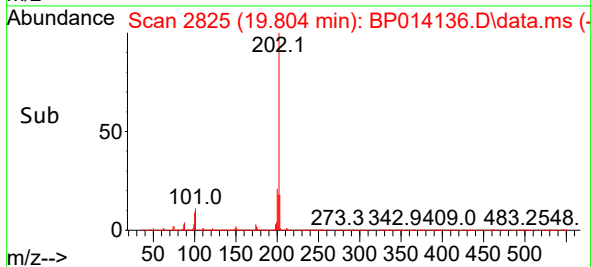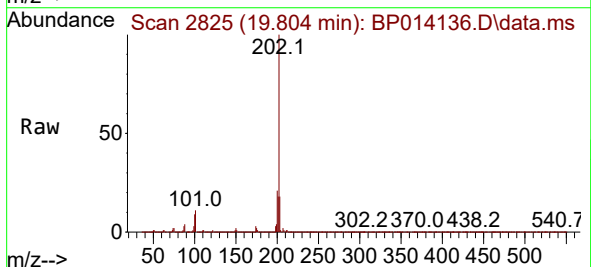



#83

Butylbenzylphthalate

Concen: 22.926 ng/ul

RT: 20.657 min Scan# 2970

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:149 Resp: 765019

Ion Ratio Lower Upper

149 100

91 75.1 57.9 86.9

206 22.0 17.9 26.9

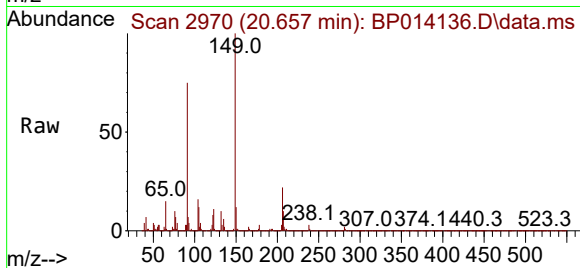

#84

3,3'-Dichlorobenzidine

Concen: 19.425 ng/ul

RT: 21.445 min Scan# 3104

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:252 Resp: 627556


Ion Ratio Lower Upper

252 100

254 64.6 51.3 76.9

126 8.8 6.9 10.3





#85

Benzo(a)anthracene

Concen: 19.866 ng/ul

RT: 21.516 min Scan# 3116

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:228 Resp: 1763316

Ion Ratio Lower Upper

228 100

229 19.7 15.5 23.3

226 26.8 22.1 33.1



#86

Bis(2-ethylhexyl)phthalate

Concen: 22.741 ng/ul

RT: 21.410 min Scan# 3098

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:149 Resp: 1134550


Ion Ratio Lower Upper

149 100

167 28.1 22.3 33.5

279 4.6 4.3 6.5





#87

Chrysene

Concen: 19.592 ng/ul

RT: 21.574 min Scan# 3126

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:228 Resp: 1657372

Ion Ratio Lower Upper

228 100

226 30.0 24.2 36.2

229 19.5 15.7 23.5



#89

Di-n-octyl phthalate

Concen: 24.851 ng/ul




RT: 22.374 min Scan# 3262


Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Tgt Ion:149 Resp: 1935615


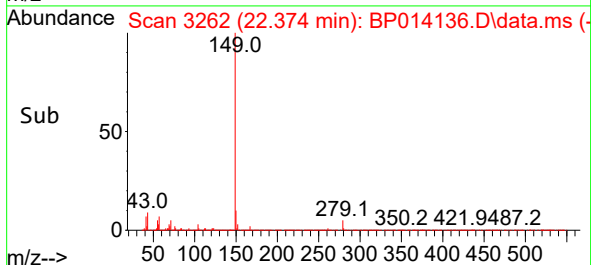
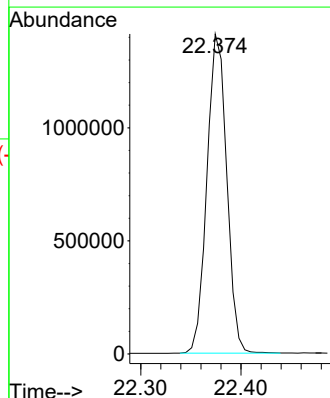
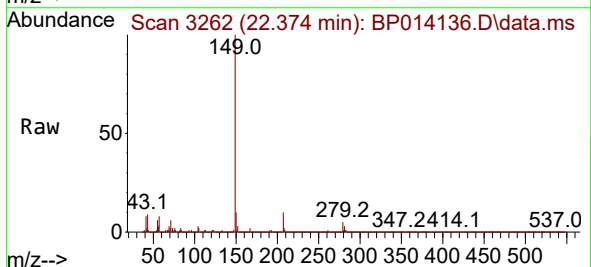




#90
Benzo(b)fluoranthene
Concen: 20.814 ng/ul
RT: 23.280 min Scan# 3416
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12




Instrument :
BNA_P
ClientSampleId :
SSTD020779


Tgt Ion:252 Resp: 1712039
Ion Ratio Lower Upper
252 100
253 22.1 17.3 25.9
125 7.8 5.4 8.2

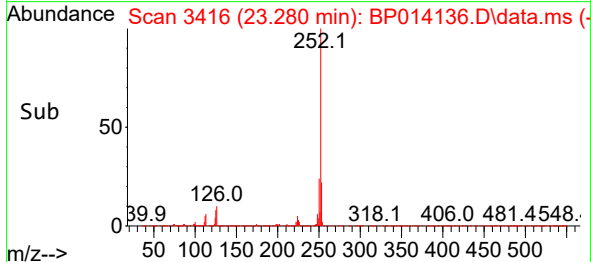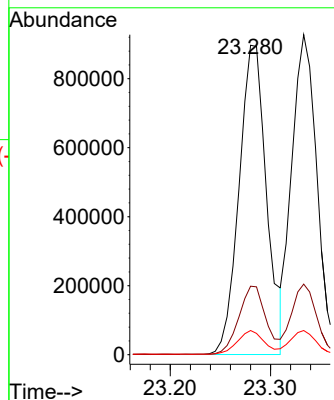

#91
Benzo(k)fluoranthene
Concen: 20.521 ng/ul
RT: 23.333 min Scan# 3425
Delta R.T. 0.000 min
Lab File: BP014136.D
Acq: 20 Mar 2023 12:12

Tgt Ion:252 Resp: 1609496
Ion Ratio Lower Upper
252 100
253 22.1 17.4 26.0
125 7.6 5.5 8.3

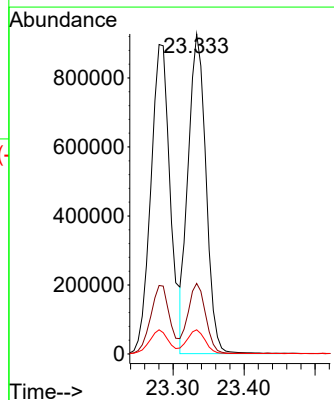



#93

Benzo(a)pyrene

Concen: 19.989 ng/ul

RT: 23.945 min Scan# 3529

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:252 Resp: 1430092

Ion Ratio Lower Upper

252 100

253 21.8 17.4 26.2

125 8.0 6.2 9.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 17.580 ng/ul

RT: 26.715 min Scan# 4000

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12




Tgt Ion:276 Resp: 1664968


Ion Ratio Lower Upper

276 100

138 17.4 13.1 19.7

277 26.0 20.2 30.2





#95

Dibenzo(a,h)anthracene

Concen: 17.787 ng/ul

RT: 26.733 min Scan# 4003

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Instrument :

BNA_P

ClientSampleId :

SSTD020779





Tgt Ion:278 Resp: 1400138

Ion Ratio Lower Upper

278 100

139 11.9 8.7 13.1

279 24.2 19.0 28.4

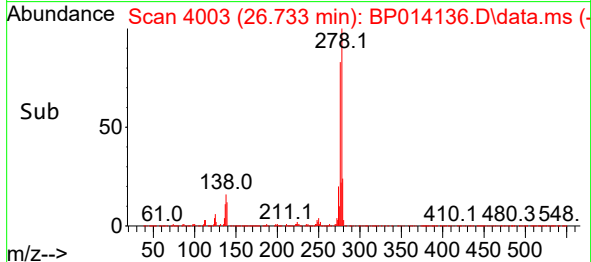

#96

Benzo(g,h,i)perylene

Concen: 17.687 ng/ul

RT: 27.539 min Scan# 4140

Delta R.T. 0.000 min

Lab File: BP014136.D

Acq: 20 Mar 2023 12:12

Tgt Ion:276 Resp: 1338939

Ion Ratio Lower Upper

276 100

138 15.1 11.9 17.9

277 23.7 18.7 28.1

