

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014150.D
 Acq On : 20 Mar 2023 20:44
 Operator : CG/JU
 Sample : 01927-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAQ6

Quant Time: Mar 21 00:49:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	177094	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	768635	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	530969	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1207886	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.528	240	1181601	20.000	ng/ul	0.00
88) Perylene-d12	24.051	264	1097417	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	13280	2.833	ng/uL	0.00
4) Pyridine-d5	3.852	84	463	0.036	ng/ul	0.00
7) Phenol-d5	7.211	99	254647	16.294	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	167812	18.412	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	203890	17.124	ng/ul	0.00
15) 4-Methylphenol-d8	8.764	113	187750	14.707	ng/ul	0.00
21) Nitrobenzene-d5	9.228	128	103873	16.937	ng/ul	0.00
24) 2-Nitrophenol-d4	9.952	143	122883	16.738	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	216463	15.670	ng/ul	0.00
31) 4-Chloroaniline-d4	11.016	131	151664	8.297	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	767937	17.042	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	839631	17.589	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	94927	11.954	ng/ul	0.00
60) Fluorene-d10	15.687	176	665663	17.430	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	120836	13.236	ng/ul	0.00
73) Anthracene-d10	17.545	188	1058852	18.058	ng/ul	-0.01
81) Pyrene-d10	19.769	212	1328825	20.390	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1100473	18.852	ng/ul	-0.01


Target Compounds					Qvalue
16) Acetophenone	8.887	105	22094	1.071 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014150.D
Acq On : 20 Mar 2023 20:44
Operator : CG/JU
Sample : 01927-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAQ6

Quant Time: Mar 21 00:49:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 20 13:12:59 2023
Response via : Initial Calibration

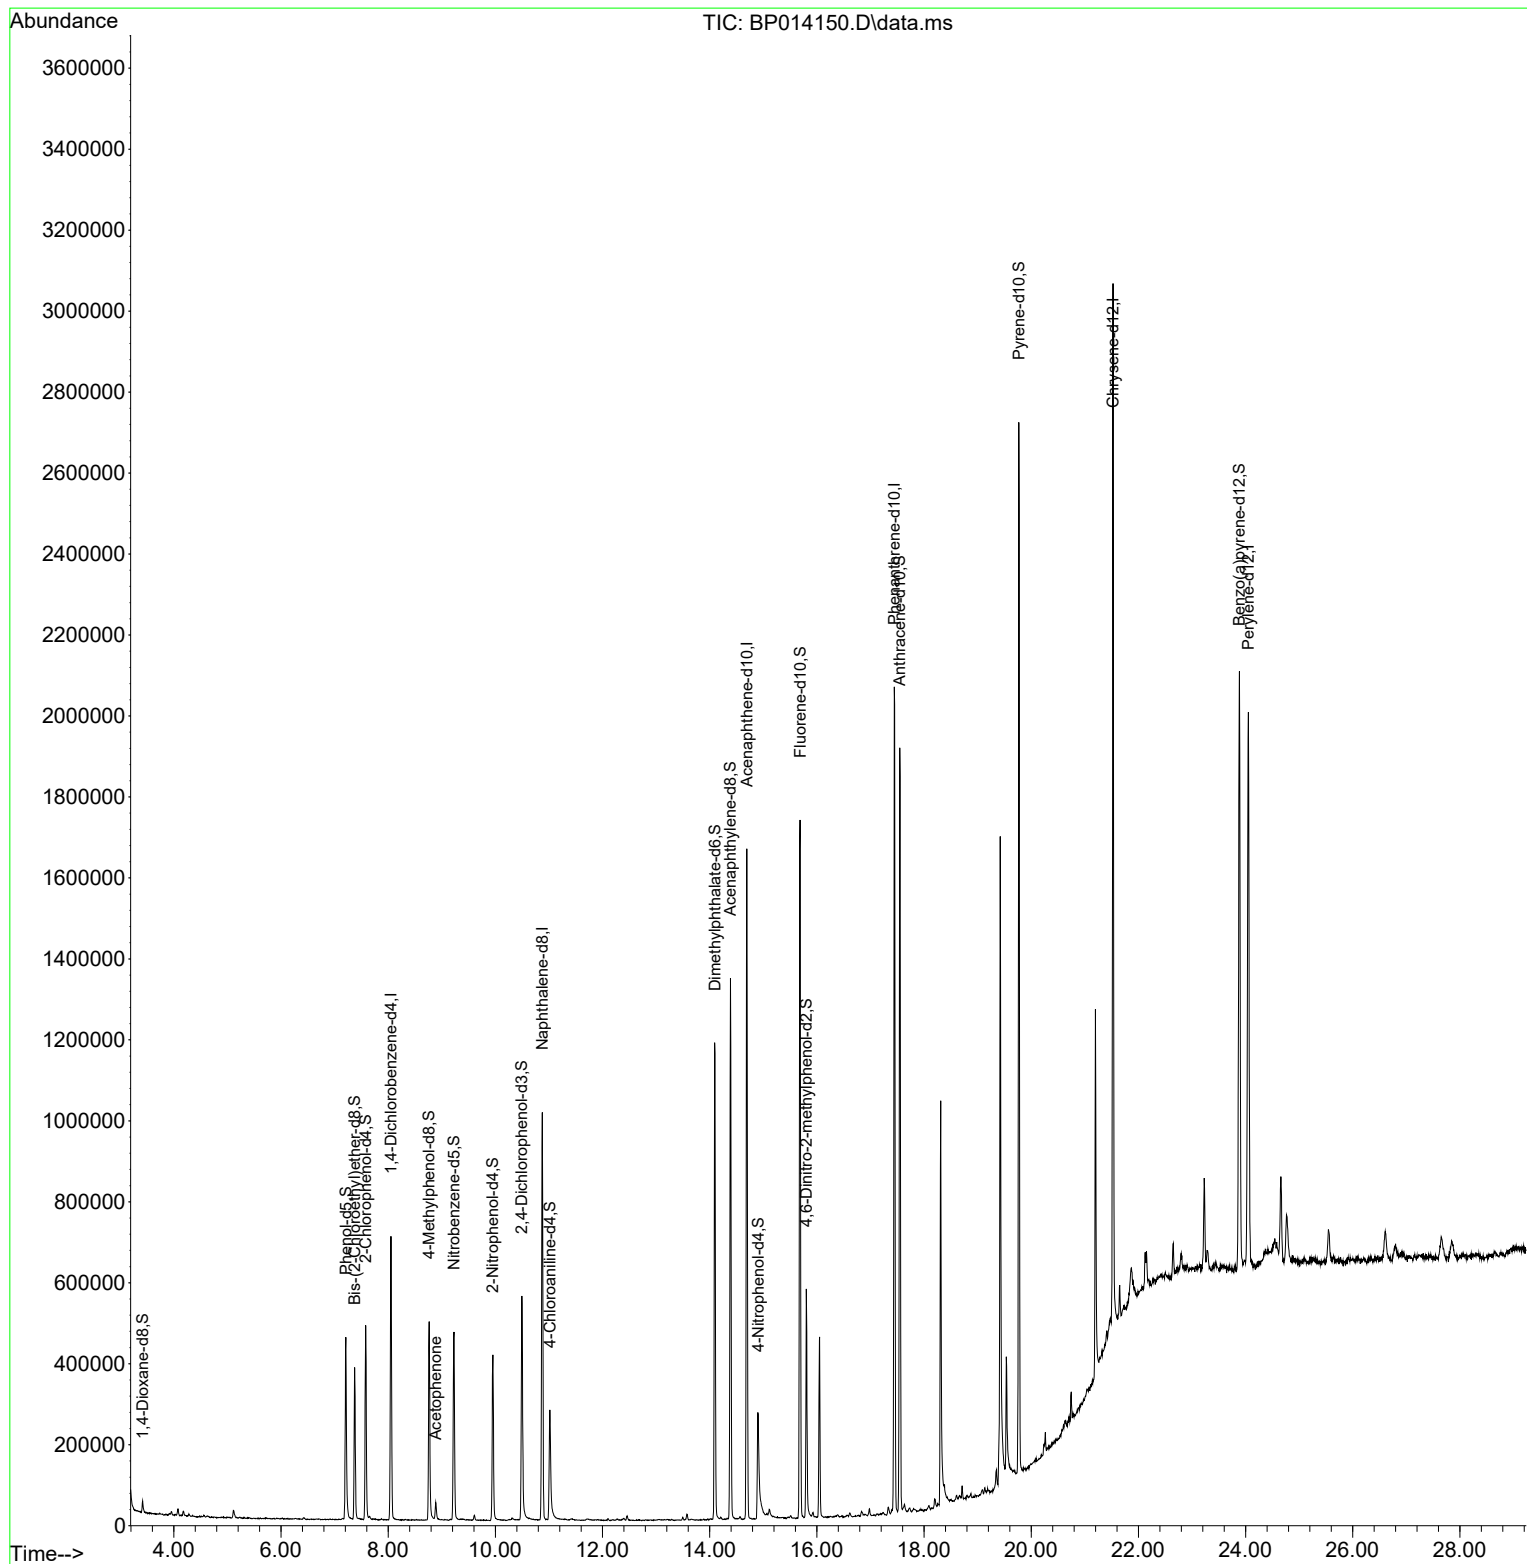

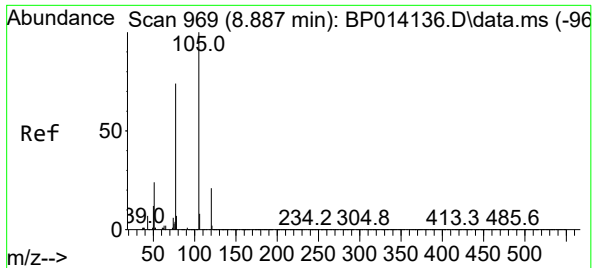

#16
 Acetophenone
 Concen: 1.071 ng/ul
 RT: 8.887 min Scan# 90
 Delta R.T. 0.000 min
 Lab File: BP014150.D
 Acq: 20 Mar 2023 20:44

Instrument :
 BNA_P
 ClientSampleId :
 DCAQ6

Tgt Ion:	105	Resp:	22094
Ion	Ratio	Lower	Upper
105	100		
77	81.2	65.4	98.2
51	31.3	21.8	32.8

