

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014151.D
 Acq On : 20 Mar 2023 21:19
 Operator : CG/JU
 Sample : 01927-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAQ2

Quant Time: Mar 21 00:49:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	173150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	756052	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.692	164	515305	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1161806	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.527	240	1147410	20.000	ng/ul	0.00
88) Perylene-d12	24.051	264	1044932	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	19446	4.243	ng/uL	0.00
4) Pyridine-d5	3.852	84	395	0.031	ng/ul	0.00
7) Phenol-d5	7.210	99	397351	26.005	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	256765	28.813	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	308007	26.458	ng/ul	0.00
15) 4-Methylphenol-d8	8.763	113	309082	24.764	ng/ul	0.00
21) Nitrobenzene-d5	9.228	128	161011	26.691	ng/ul	0.00
24) 2-Nitrophenol-d4	9.952	143	193813	26.839	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	339884	25.015	ng/ul	0.00
31) 4-Chloroaniline-d4	11.016	131	142281	7.913	ng/ul	0.00
46) Dimethylphthalate-d6	14.098	166	1187424	27.152	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1299105	28.042	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	153539	19.923	ng/ul	0.00
60) Fluorene-d10	15.687	176	989357	26.694	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	206219	23.485	ng/ul	0.00
73) Anthracene-d10	17.545	188	1579285	28.001	ng/ul	-0.01
81) Pyrene-d10	19.769	212	1937428	30.615	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.886	264	1585984	28.534	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.887	105	31576	1.566	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014151.D
Acq On : 20 Mar 2023 21:19
Operator : CG/JU
Sample : 01927-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAQ2

Quant Time: Mar 21 00:49:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 20 13:12:59 2023
Response via : Initial Calibration

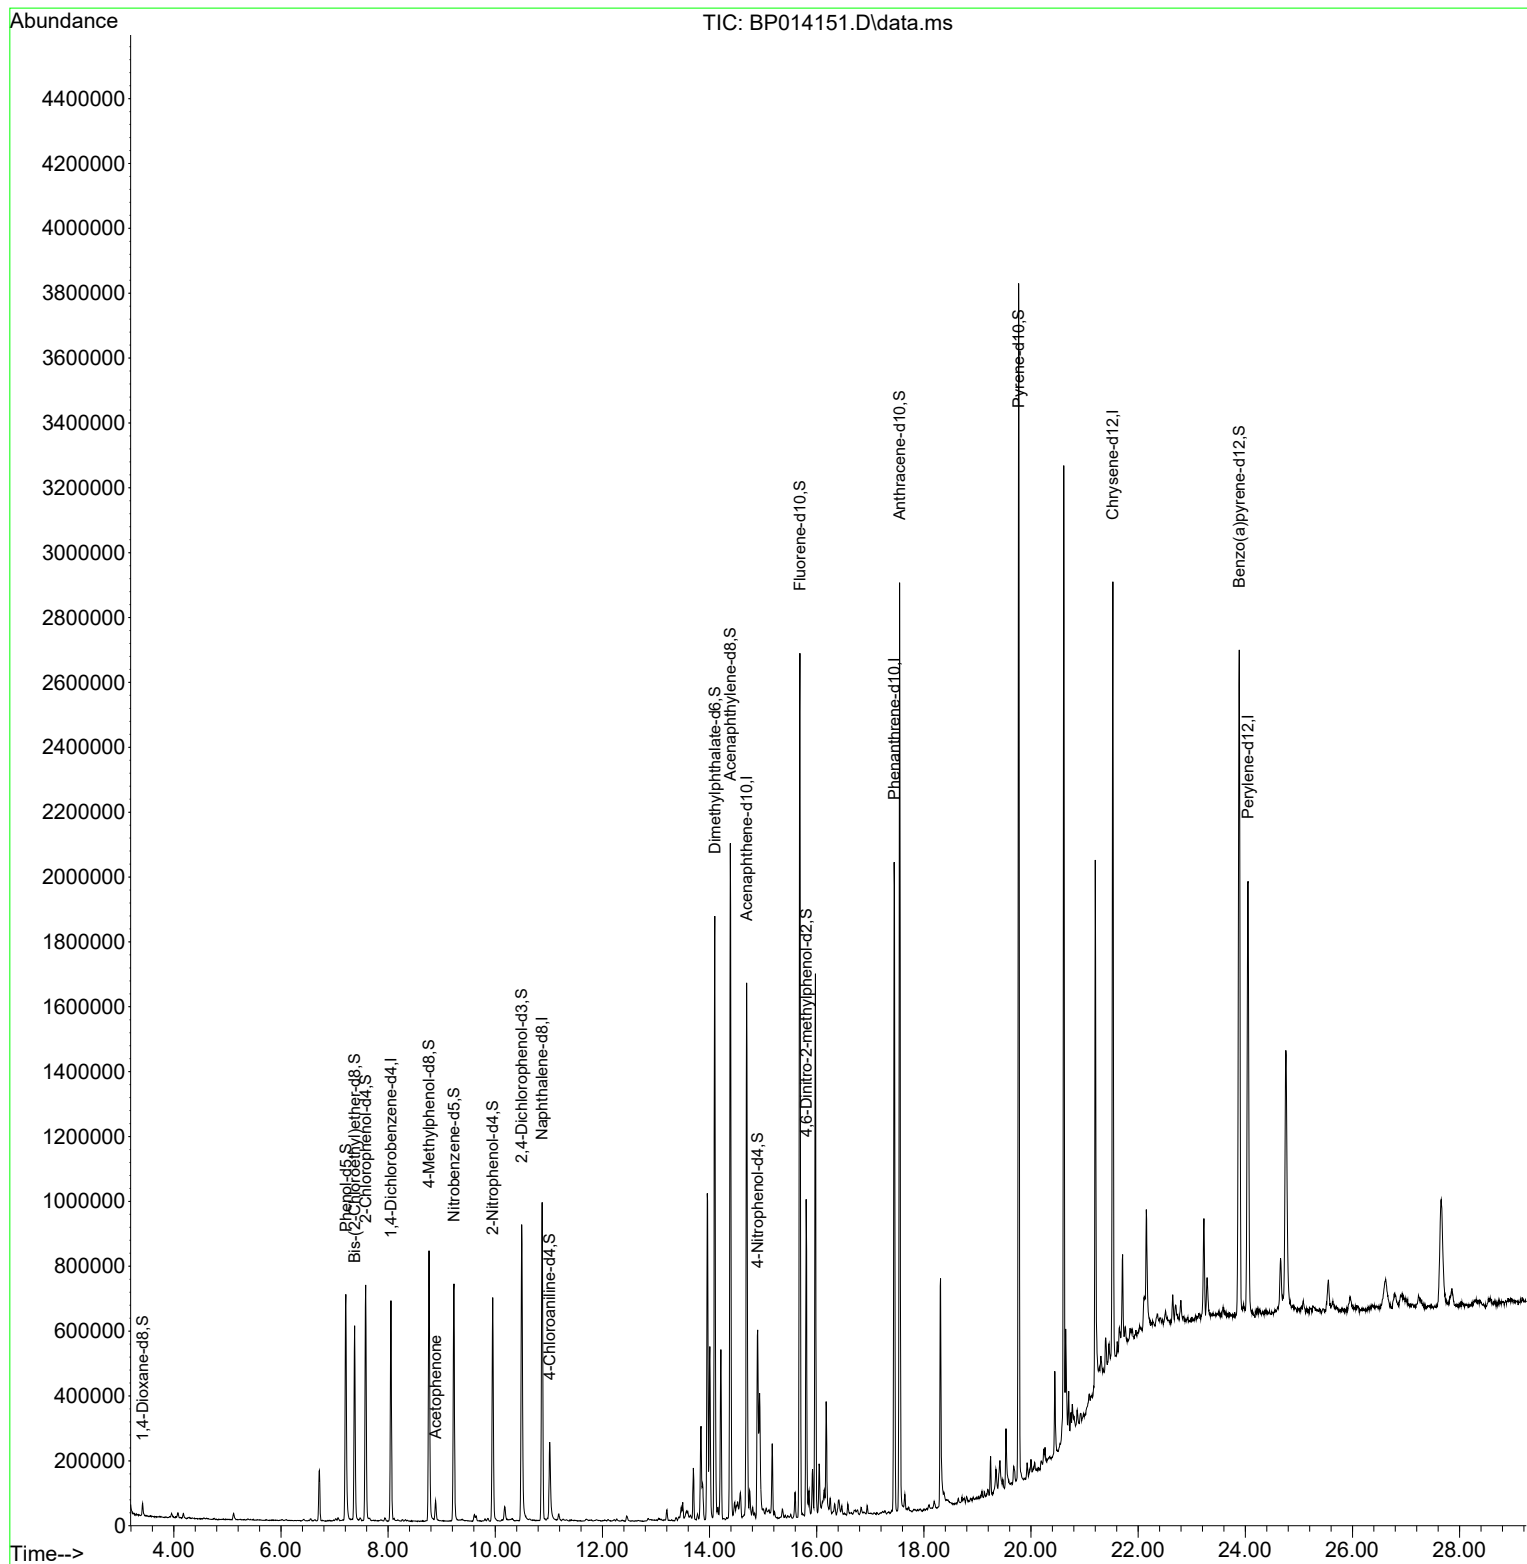

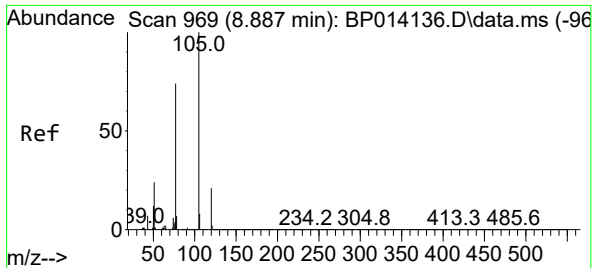

#16
 Acetophenone
 Concen: 1.566 ng/ul
 RT: 8.887 min Scan# 90
 Delta R.T. 0.000 min
 Lab File: BP014151.D
 Acq: 20 Mar 2023 21:19

Instrument :
 BNA_P
 ClientSampleId :
 DCAQ2

Tgt Ion:	105	Resp:	31576
Ion Ratio	Lower	Upper	
105	100		
77	84.9	65.4	98.2
51	29.7	21.8	32.8

