

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014155.D
 Acq On : 20 Mar 2023 23:36
 Operator : CG/JU
 Sample : 01885-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB907

Quant Time: Mar 21 00:50:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	207523	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	867542	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	583542	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1325587	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.527	240	1213458	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	1092778	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	21419	3.900	ng/uL	0.00
4) Pyridine-d5	3.852	84	136242	8.959	ng/ul	0.00
7) Phenol-d5	7.211	99	123632	6.751	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	354602	33.201	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	325197	23.307	ng/ul	0.00
15) 4-Methylphenol-d8	8.763	113	240239	16.060	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	226205	32.679	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.952	143	249222	30.077	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	420246	26.954	ng/ul	0.00
31) 4-Chloroaniline-d4	11.010	131	289941	14.052	ng/ul	0.00
46) Dimethylphthalate-d6	14.098	166	1608881	32.487	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1761680	33.580	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	46188	5.292	ng/ul	0.01
60) Fluorene-d10	15.687	176	1384206	32.980	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	281748	28.122	ng/ul	0.00
73) Anthracene-d10	17.545	188	2145394	33.339	ng/ul	-0.01
81) Pyrene-d10	19.769	212	2626612	39.246	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1968938	33.873	ng/ul	-0.01


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.452	88	20868	3.519	ng/uL#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014155.D
Acq On : 20 Mar 2023 23:36
Operator : CG/JU
Sample : 01885-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB907

Quant Time: Mar 21 00:50:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 20 13:12:59 2023
Response via : Initial Calibration

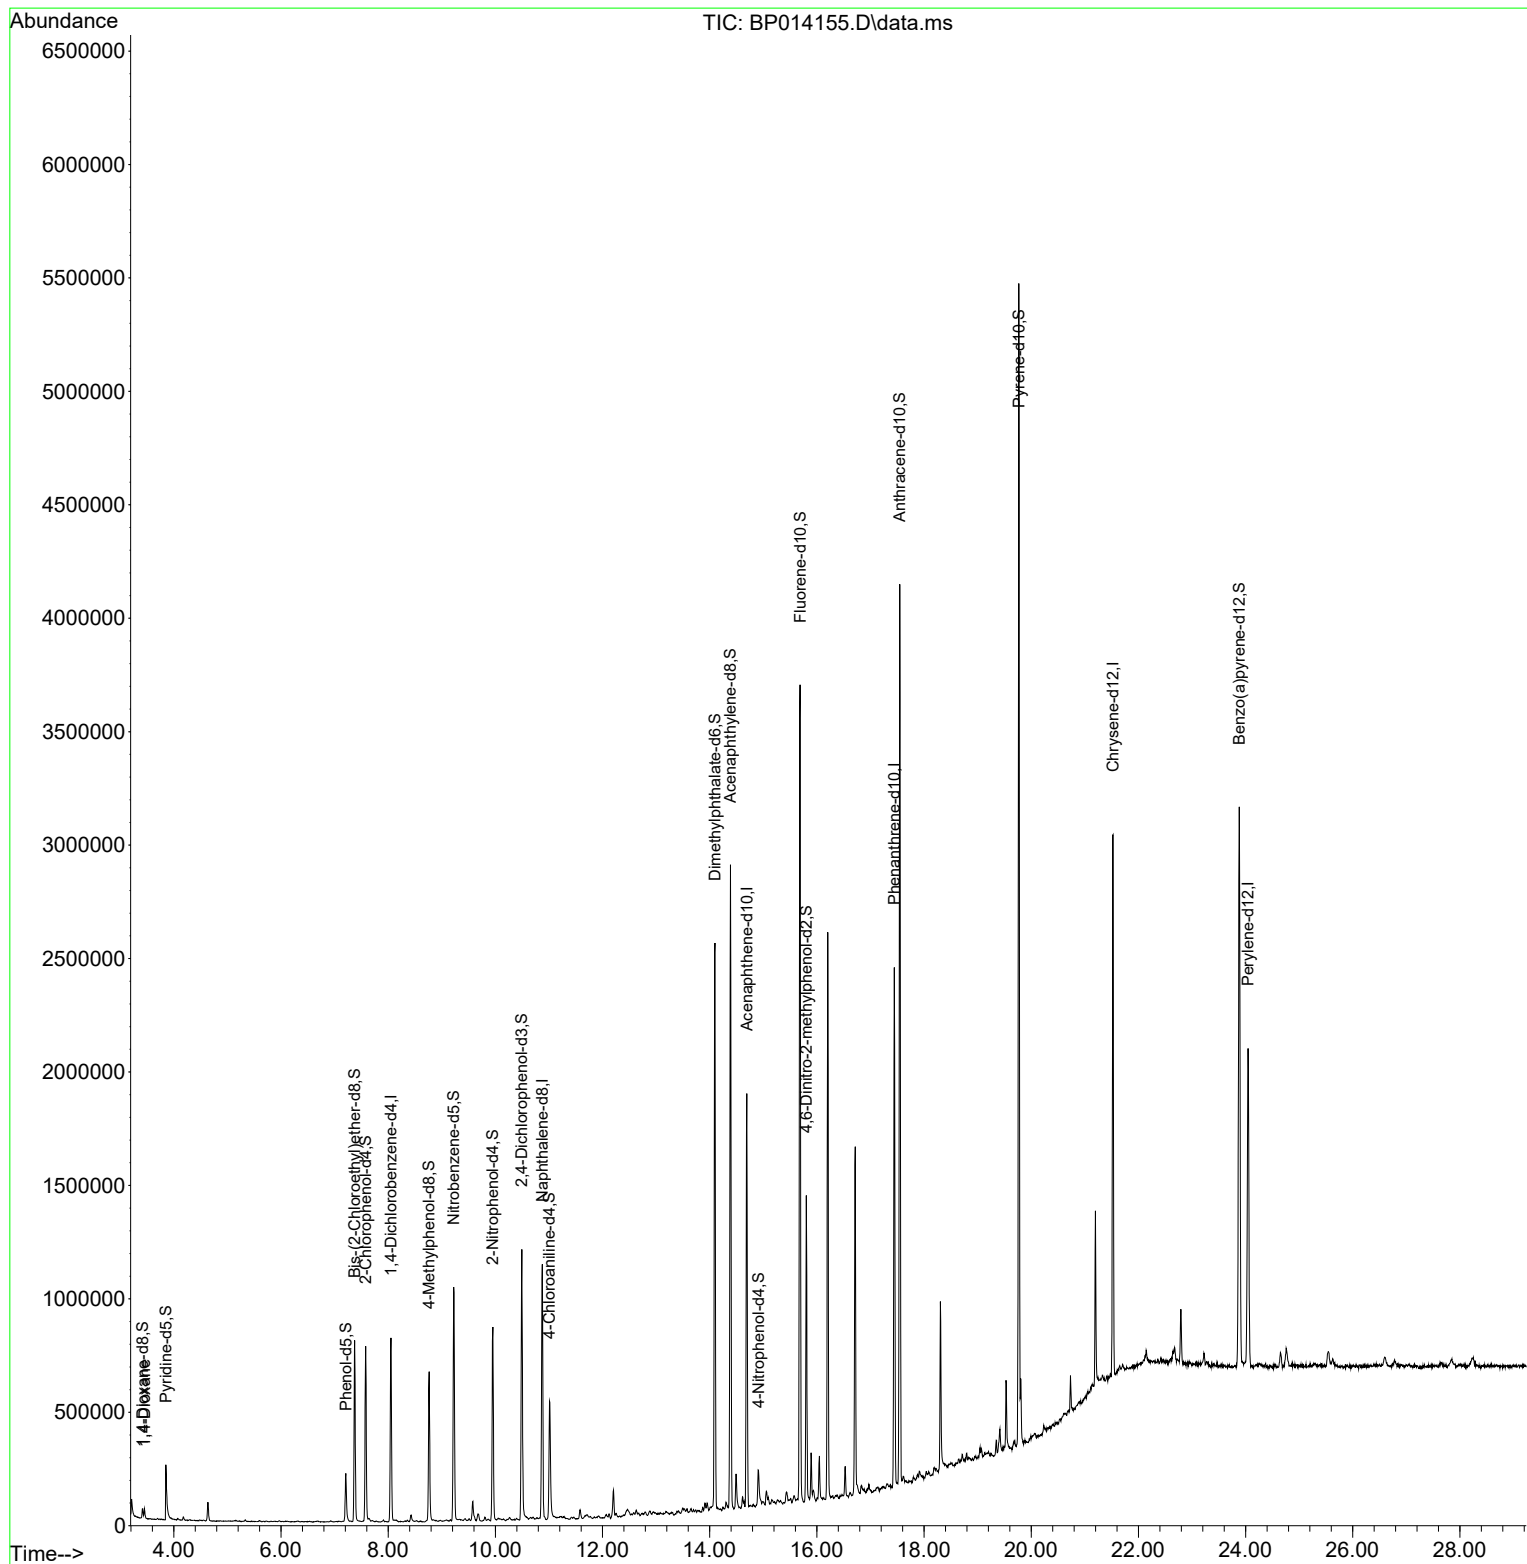

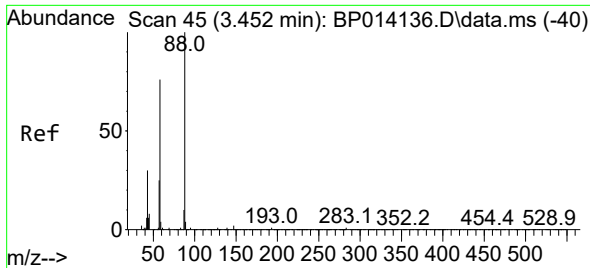

#2
 1,4-Dioxane
 Concen: 3.519 ng/uL
 RT: 3.452 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP014155.D
 Acq: 20 Mar 2023 23:36

Instrument :
 BNA_P
 ClientSampleId :
 CB907

Tgt Ion: 88 Resp: 20868
 Ion Ratio Lower Upper
 88 100
 43 36.2 23.9 35.9#
 58 72.6 50.2 75.2

