

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014195.D
 Acq On : 21 Mar 2023 23:28
 Operator : CG/JU
 Sample : 01949-04
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB935

Quant Time: Mar 22 01:23:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 21 04:47:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	199964	20.000	ng/u1	0.00
20) Naphthalene-d8	10.869	136	849382	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.686	164	569245	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.439	188	1300733	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.515	240	1146912	20.000	ng/u1	#-0.01
88) Perylene-d12	24.033	264	1013527	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	18227	3.444	ng/uL	0.00
4) Pyridine-d5	3.846	84	183344	12.512	ng/u1	0.00
7) Phenol-d5	7.204	99	104903	5.945	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	296581	28.818	ng/u1	0.00
11) 2-Chlorophenol-d4	7.575	132	292764	21.776	ng/u1	0.00
15) 4-Methylphenol-d8	8.757	113	212375	14.734	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	191617	28.274	ng/u1	0.00
24) 2-Nitrophenol-d4	9.945	143	218575	26.943	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	396346	25.965	ng/u1	0.00
31) 4-Chloroaniline-d4	11.004	131	537498	26.608	ng/u1	0.00
46) Dimethylphthalate-d6	14.092	166	1515996	31.380	ng/u1	0.00
49) Acenaphthylene-d8	14.380	160	1564753	30.575	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	38159	4.482	ng/u1	0.01
60) Fluorene-d10	15.675	176	1260192	30.779	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	221940	22.576	ng/u1	0.00
73) Anthracene-d10	17.539	188	2078274	32.913	ng/u1	0.00
81) Pyrene-d10	19.763	212	2427062	38.369	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.874	264	1807748	33.531	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.446	88	8339	1.460	ng/uL#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014195.D
Acq On : 21 Mar 2023 23:28
Operator : CG/JU
Sample : 01949-04
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB935


Quant Time: Mar 22 01:23:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 21 04:47:07 2023
Response via : Initial Calibration

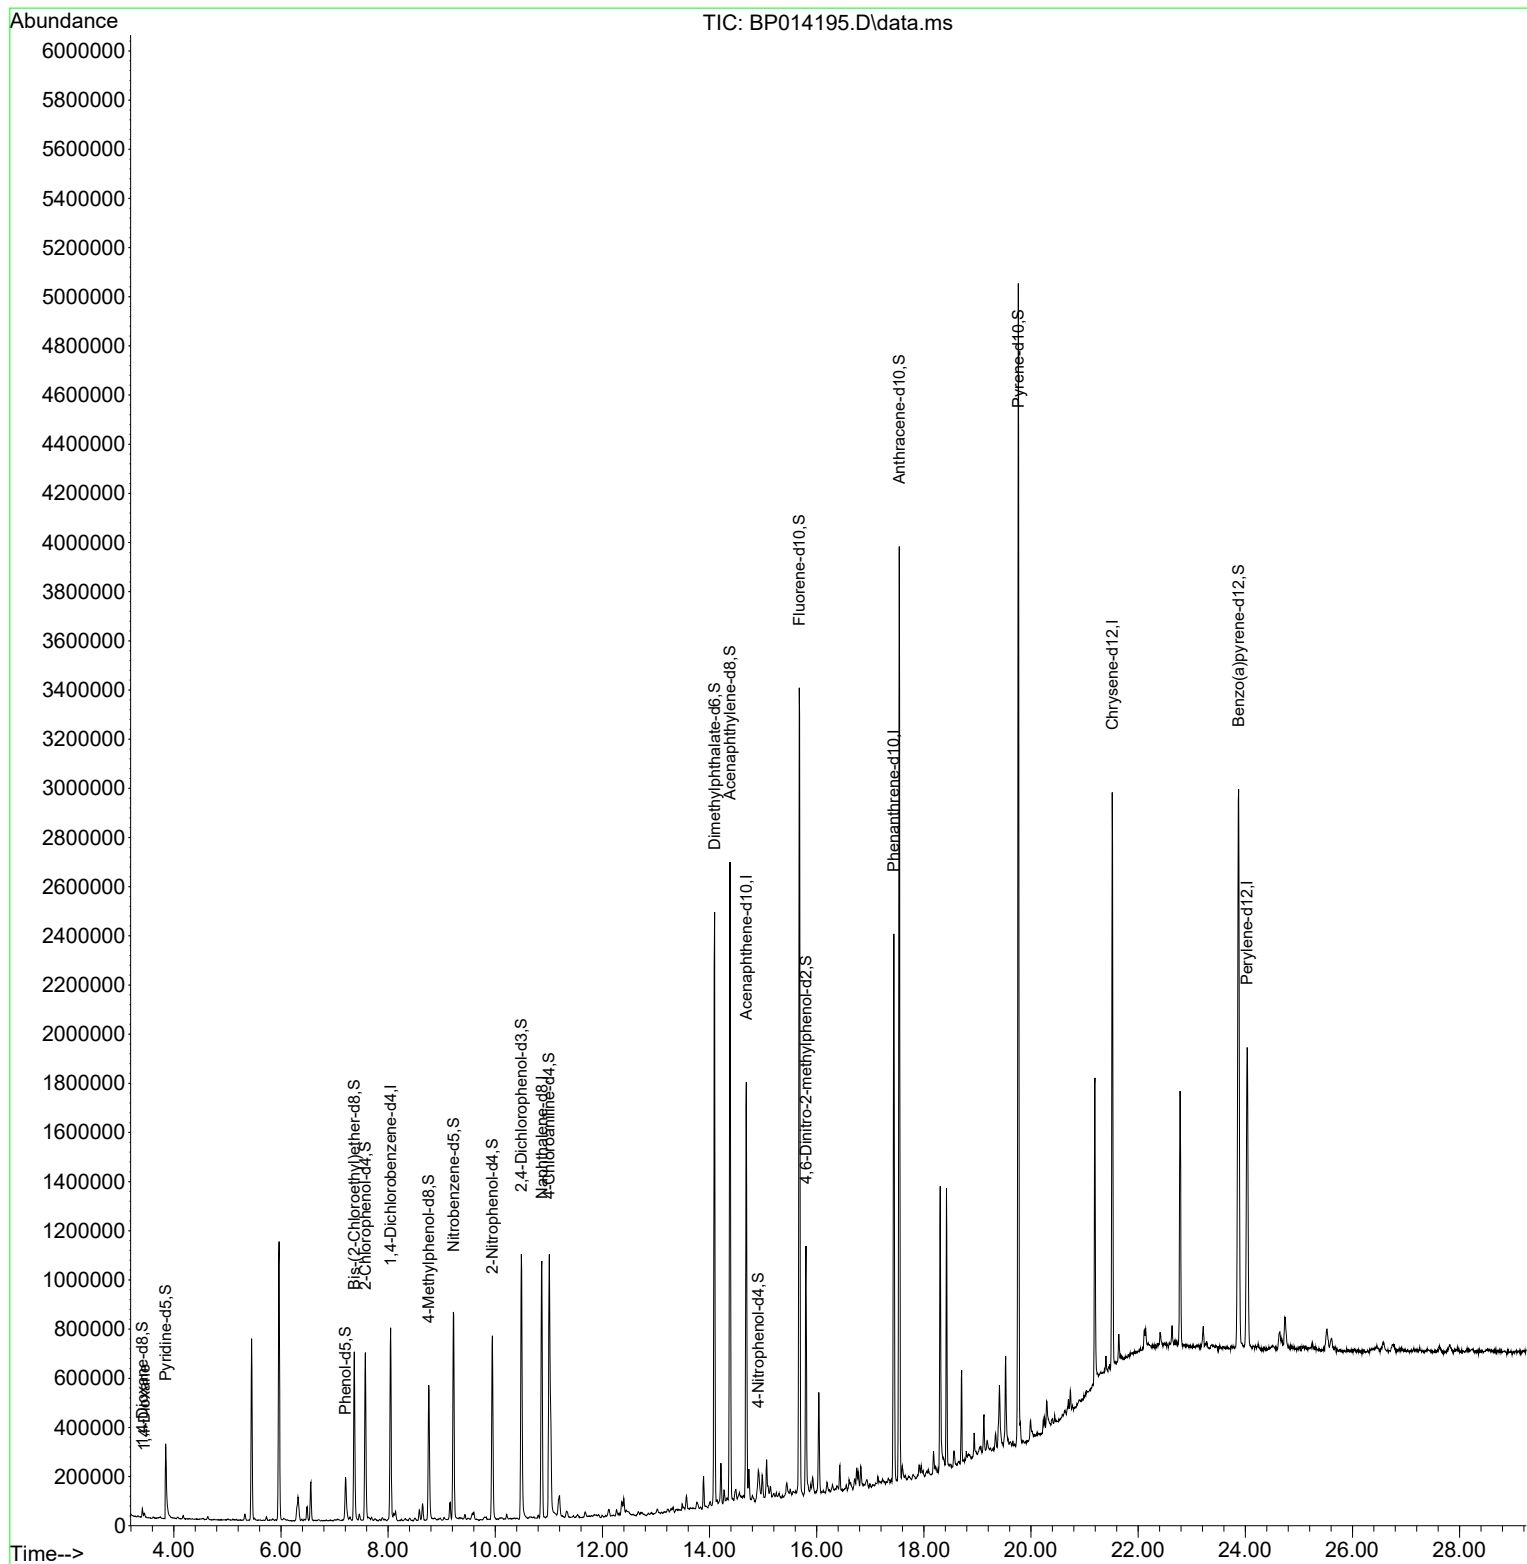

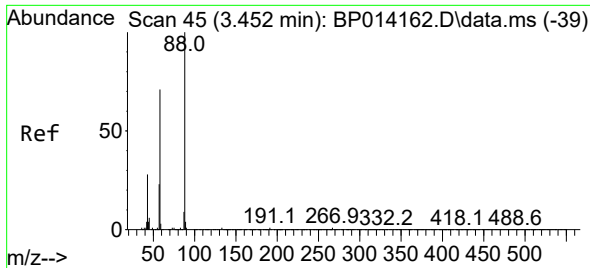

#2
 1,4-Dioxane
 Concen: 1.460 ng/uL
 RT: 3.446 min Scan# 44
 Delta R.T. -0.006 min
 Lab File: BP014195.D
 Acq: 21 Mar 2023 23:28

Instrument :
 BNA_P
 ClientSampleId :
 CB935

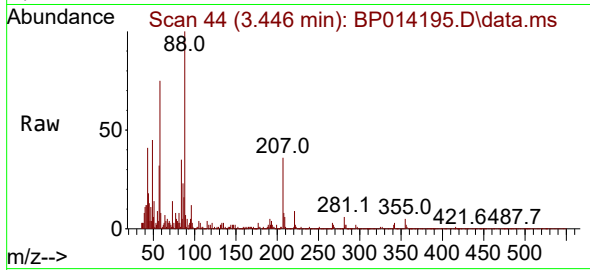

Tgt Ion: 88 Resp: 8339
 Ion Ratio Lower Upper
 88 100
 43 41.4 23.9 35.9#
 58 75.2 50.2 75.2

