

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014220.D
 Acq On : 22 Mar 2023 15:14
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 23 00:59:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 22 03:05:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	216366	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	956849	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.686	164	653677	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	1520637	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.527	240	1443689	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	1300506	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	668	0.117	ng/uL	0.05
4) Pyridine-d5	3.846	84	302722	19.093	ng/ul	0.00
7) Phenol-d5	7.210	99	407015	21.317	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	248468	22.313	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	303884	20.890	ng/ul	0.00
15) 4-Methylphenol-d8	8.763	113	333810	21.403	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	155269	20.337	ng/ul	0.00
24) 2-Nitrophenol-d4	9.951	143	182295	19.947	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	333434	19.390	ng/ul	0.00
31) 4-Chloroaniline-d4	11.010	131	446081	19.602	ng/ul	0.00
46) Dimethylphthalate-d6	14.092	166	1044580	18.829	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1181685	20.108	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	177204	18.126	ng/ul	0.00
60) Fluorene-d10	15.681	176	894237	19.020	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	195043	16.971	ng/ul	0.00
73) Anthracene-d10	17.545	188	1452628	19.678	ng/ul	0.00
81) Pyrene-d10	19.769	212	1760660	22.112	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1383108	19.994	ng/ul	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.446	88	45845	7.416	ng/uL	93
5) Pyridine	3.864	79	316776	19.701	ng/ul	93
6) Benzaldehyde	7.187	77	239042	25.161	ng/ul	100
8) Phenol	7.234	94	417922	21.224	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.469	93	327979	21.741	ng/ul	98
12) 2-Chlorophenol	7.610	128	310916	21.213	ng/ul	96
13) 2-Methylphenol	8.499	108	313517	21.413	ng/ul	96
14) 2,2'-oxybis(1-Chloropr...	8.581	45	413671	25.392	ng/ul	97
16) Acetophenone	8.881	105	534019	21.195	ng/ul	100
17) N-Nitroso-di-n-propyla...	8.863	70	286487	22.226	ng/ul	97
18) 4-Methylphenol	8.828	108	348575	21.644	ng/ul	99
19) Hexachloroethane	9.134	117	135695	21.139	ng/ul	96
22) Nitrobenzene	9.269	77	430207	21.065	ng/ul	98
23) Isophorone	9.793	82	798558	20.304	ng/ul	98
25) 2-Nitrophenol	9.981	139	190456	20.220	ng/ul	95
26) 2,4-Dimethylphenol	10.040	107	412309	19.999	ng/ul	99
27) Bis(2-Chloroethoxy)met...	10.275	93	468705	20.603	ng/ul	100
29) 2,4-Dichlorophenol	10.522	162	326814	19.267	ng/ul	96
30) Naphthalene	10.922	128	1054560	20.070	ng/ul	99
32) 4-Chloroaniline	11.040	127	448828	19.600	ng/ul	100
33) Hexachlorobutadiene	11.198	225	241301	17.877	ng/ul	98
34) Caprolactam	11.828	113	72980	13.250	ng/ul	92
35) 4-Chloro-3-methylphenol	12.157	107	397688	20.275	ng/ul	96
36) 2-Methylnaphthalene	12.522	142	722931	19.616	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014220.D
 Acq On : 22 Mar 2023 15:14
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 23 00:59:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 22 03:05:29 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.740	142	719669	19.428	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.887	216	443978	18.782	ng/ul	98
40) Hexachlorocyclopentadiene	12.857	237	233625	13.802	ng/ul	96
41) 2,4,6-Trichlorophenol	13.128	196	288206	19.409	ng/ul	100
42) 2,4,5-Trichlorophenol	13.204	196	318312	19.533	ng/ul	99
43) 1,1'-Biphenyl	13.522	154	1003381	19.938	ng/ul	99
44) 2-Chloronaphthalene	13.569	162	806063	20.167	ng/ul	98
45) 2-Nitroaniline	13.781	65	263971	22.330	ng/ul	95
47) Dimethylphthalate	14.139	163	1046743	19.062	ng/ul	100
48) 2,6-Dinitrotoluene	14.269	165	217370	20.023	ng/ul	98
50) Acenaphthylene	14.416	152	1252433	20.307	ng/ul	99
51) 3-Nitroaniline	14.604	138	206876	21.522	ng/ul	93
52) Acenaphthene	14.751	153	868523	20.144	ng/ul	100
53) 2,4-Dinitrophenol	14.810	184	116122	14.323	ng/ul	96
55) 4-Nitrophenol	14.916	109	165006	15.625	ng/ul	87
56) Dibenzofuran	15.086	168	1218400	19.425	ng/ul	100
57) 2,4-Dinitrotoluene	15.057	165	319669	19.708	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.316	232	292408	18.755	ng/ul	98
59) Diethylphthalate	15.498	149	1073871	19.281	ng/ul	99
61) Fluorene	15.739	166	1016996	19.560	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.728	204	536540	18.697	ng/ul	99
63) 4-Nitroaniline	15.769	138	221084	22.376	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.822	198	192972	17.599	ng/ul	99
67) N-Nitrosodiphenylamine	15.945	169	869567	20.247	ng/ul	99
68) 4-Bromophenyl-phenylether	16.628	248	346094	18.827	ng/ul	99
69) Hexachlorobenzene	16.745	284	400631	18.494	ng/ul	98
70) Atrazine	16.898	200	352150	19.011	ng/ul	98
71) Pentachlorophenol	17.092	266	234055	16.529	ng/ul	98
72) Phenanthrene	17.486	178	1647756	19.867	ng/ul	99
74) Anthracene	17.580	178	1694302	20.147	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.492	216	454800	19.488	ng/ul	98
76) Pentachlorobenzene	15.004	250	462438	19.076	ng/ul	99
77) Carbazole	17.851	167	1501333	20.240	ng/ul	99
78) Di-n-butylphthalate	18.375	149	1931157	20.831	ng/ul	100
80) Fluoranthene	19.445	202	2045404	22.537	ng/ul#	96
82) Pyrene	19.798	202	2097465	22.154	ng/ul#	95
83) Butylbenzylphthalate	20.651	149	918828	24.069	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.433	252	623717	16.876	ng/ul	99
85) Benzo(a)anthracene	21.510	228	2035746	20.048	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.404	149	1364702	23.911	ng/ul	100
87) Chrysene	21.563	228	1902632	19.661	ng/ul	100
89) Di-n-octyl phthalate	22.363	149	2304228	28.080	ng/ul	100
90) Benzo(b)fluoranthene	23.268	252	1796526	20.731	ng/ul	98
91) Benzo(k)fluoranthene	23.321	252	1772666	21.452	ng/ul	99
93) Benzo(a)pyrene	23.933	252	1502576	19.935	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.692	276	1745805	17.496	ng/ul	97
95) Dibenzo(a,h)anthracene	26.709	278	1459348	17.597	ng/ul	99
96) Benzo(g,h,i)perylene	27.509	276	1382362	17.333	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014220.D
 Acq On : 22 Mar 2023 15:14
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :


Quant Time: Mar 23 00:59:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 22 03:05:29 2023
 Response via : Initial Calibration

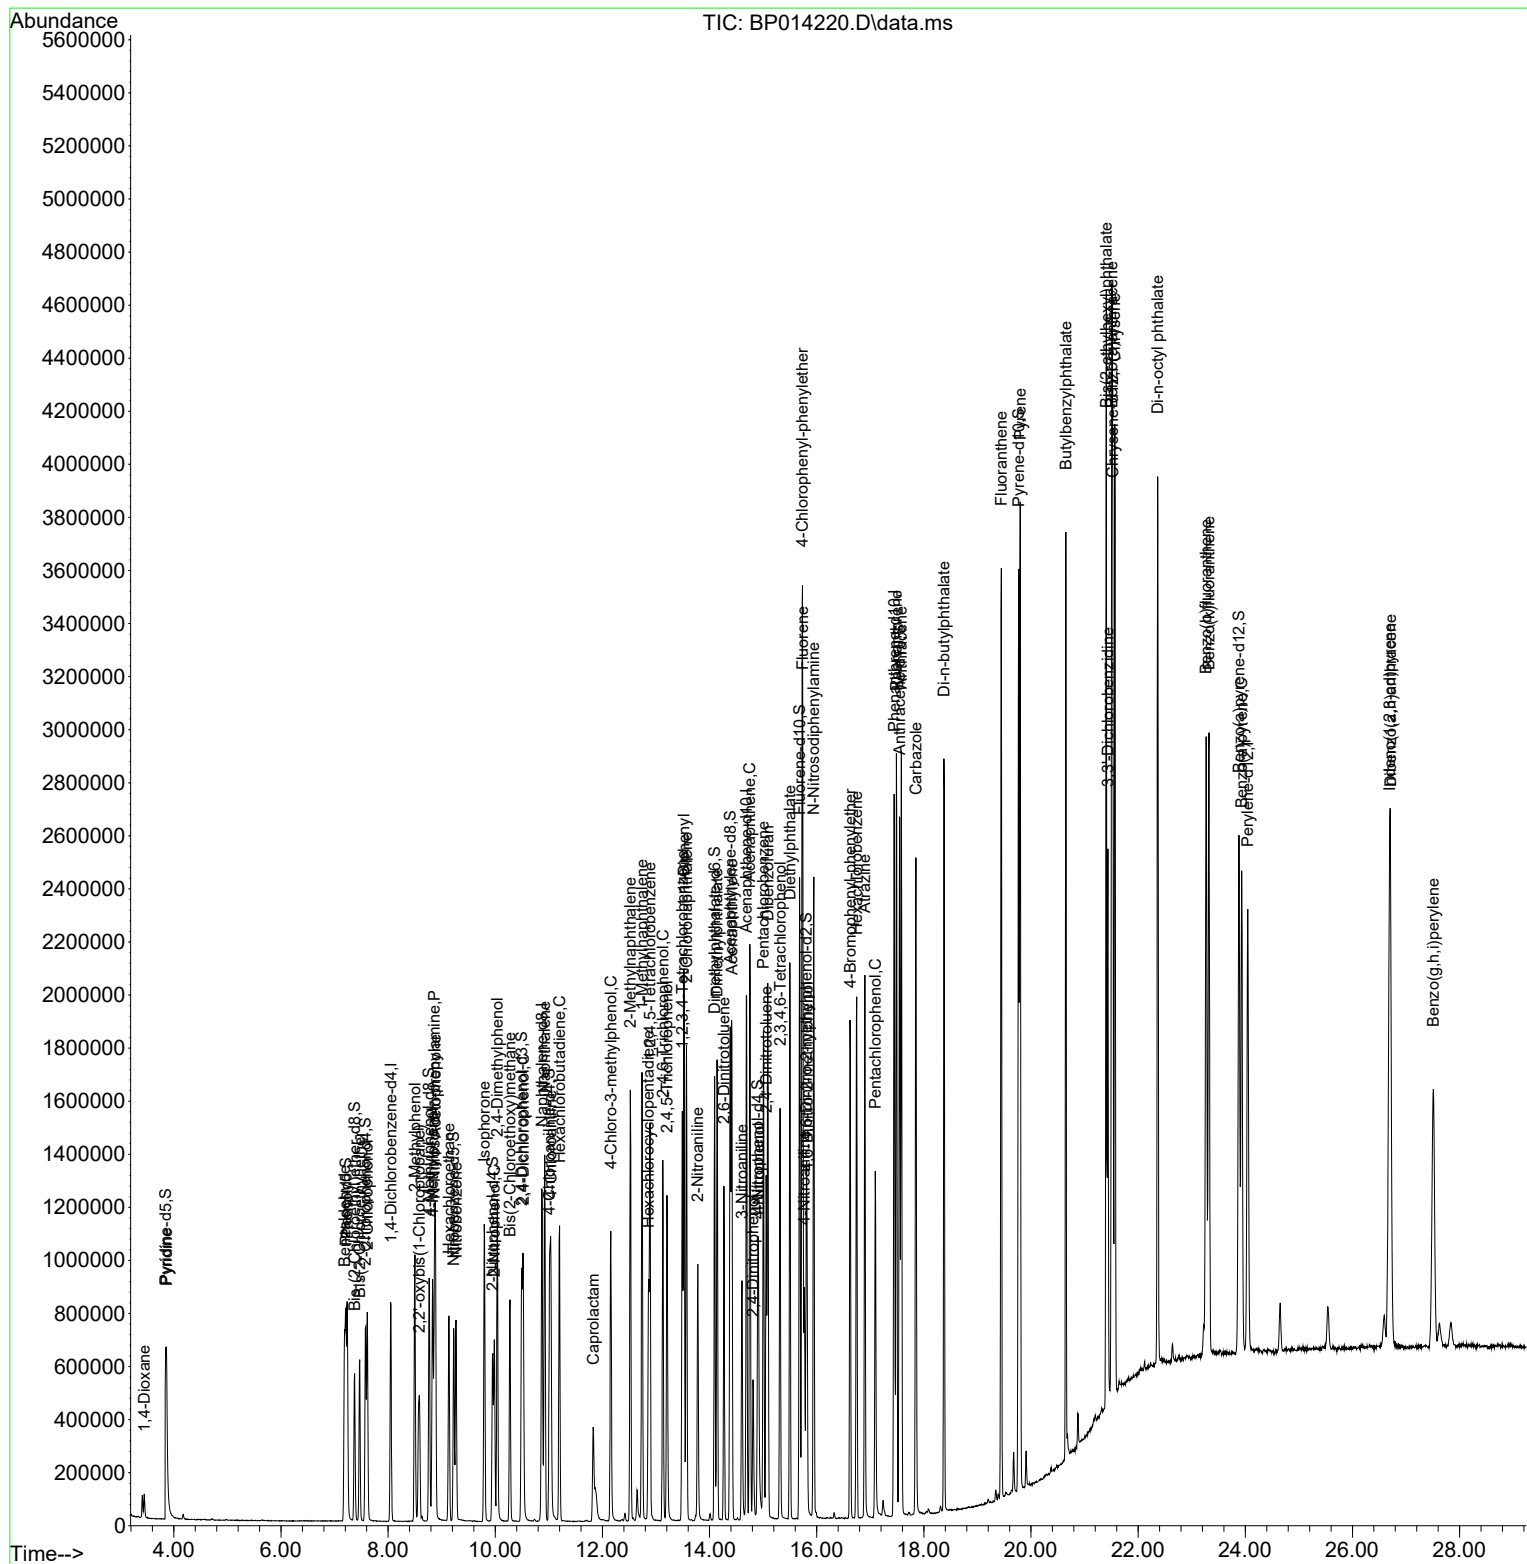



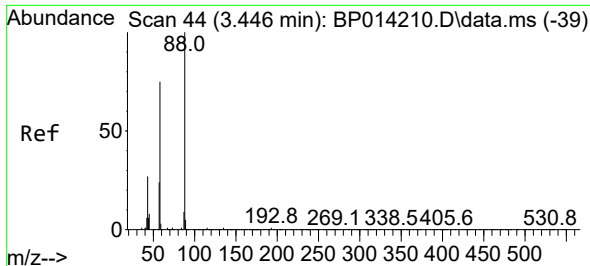


#2
1,4-Dioxane
Concen: 7.416 ng/uL
RT: 3.446 min Scan# 44
Delta R.T. -0.000 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Instrument :
BNA_P
ClientSampleId :



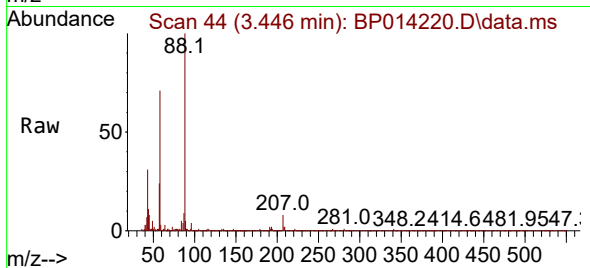



Tgt Ion: 88 Resp: 45845
Ion Ratio Lower Upper
88 100
43 30.8 23.9 35.9
58 70.6 50.2 75.2

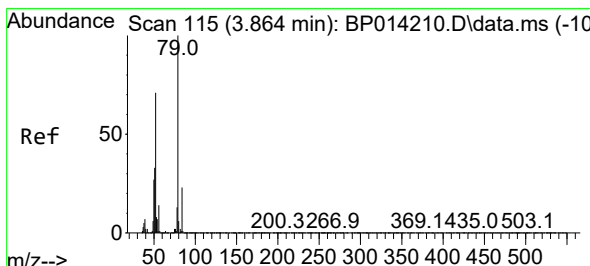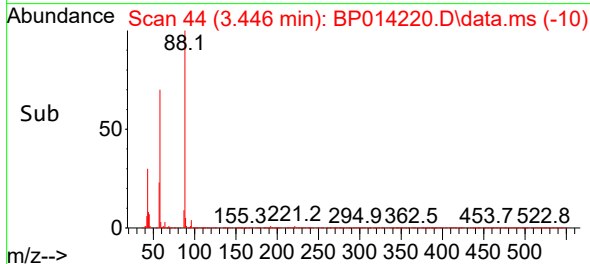

#5
Pyridine
Concen: 19.701 ng/uL
RT: 3.864 min Scan# 115
Delta R.T. -0.000 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion: 79 Resp: 316776
Ion Ratio Lower Upper
79 100
52 76.8 55.1 82.7
51 35.4 28.9 43.3


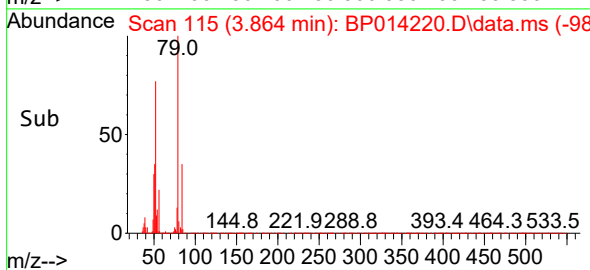

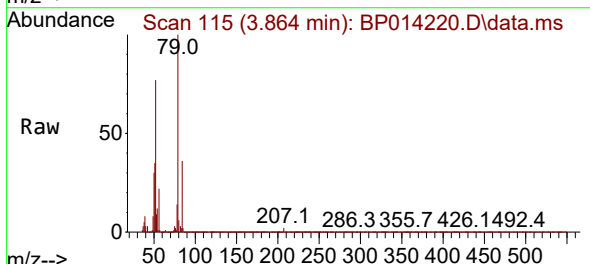




#6
Benzaldehyde
Concen: 25.161 ng/ul
RT: 7.187 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 239042
Ion Ratio Lower Upper
77 100
105 92.6 74.2 111.2
106 87.4 69.8 104.8



#8
Phenol
Concen: 21.224 ng/ul
RT: 7.234 min Scan# 688
Delta R.T. -0.000 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion: 94 Resp: 417922
Ion Ratio Lower Upper
94 100
65 30.4 25.2 37.8
66 44.9 37.2 55.8


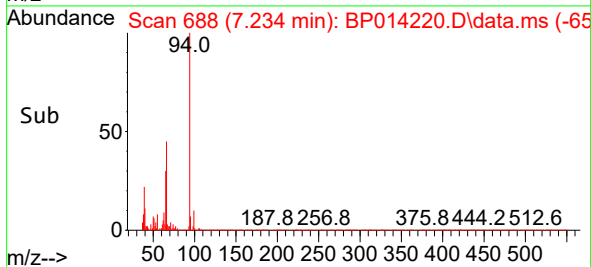

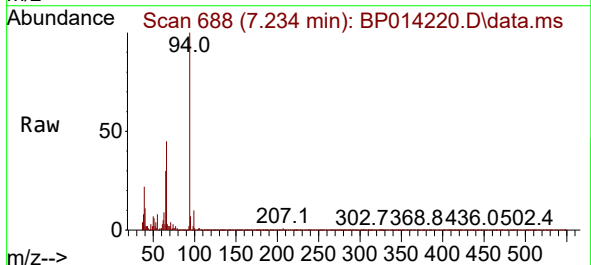




#10
Bis(2-Chloroethyl)ether
Concen: 21.741 ng/ul
RT: 7.469 min Scan# 71
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 93 Resp: 327979
Ion Ratio Lower Upper
93 100
63 76.2 58.8 88.2
95 32.4 25.8 38.6



#12
2-Chlorophenol
Concen: 21.213 ng/ul
RT: 7.610 min Scan# 752
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:128 Resp: 310916
Ion Ratio Lower Upper
128 100
64 52.2 38.3 57.5
130 32.0 25.7 38.5

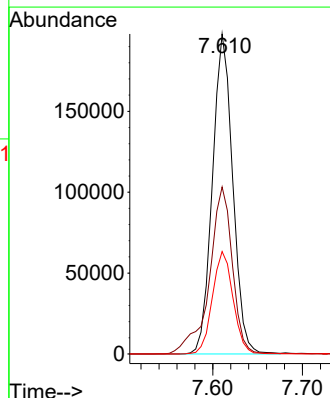



#13

2-Methylphenol

Concen: 21.413 ng/ul

RT: 8.499 min Scan# 902

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P





ClientSampleId :

Tgt Ion:108 Resp: 313517

Ion Ratio Lower Upper

108 100

107 91.4 70.5 105.7

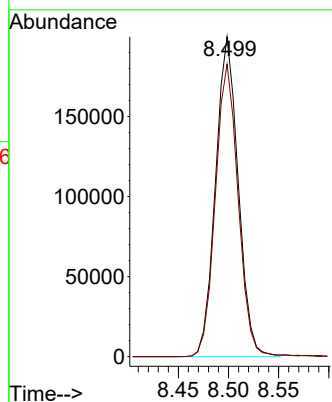

#14

2,2'-oxybis(1-Chloropropane)

Concen: 25.392 ng/ul

RT: 8.581 min Scan# 917

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion: 45 Resp: 413671


Ion Ratio Lower Upper

45 100

77 16.0 14.2 21.2


79 12.3 10.6 15.8








#16
 Acetophenone
 Concen: 21.195 ng/ul
 RT: 8.881 min Scan# 968
 Delta R.T. -0.000 min
 Lab File: BP014220.D
 Acq: 22 Mar 2023 15:14

Instrument :
 BNA_P
 ClientSampleId :







Tgt Ion:105 Resp: 534019
 Ion Ratio Lower Upper
 105 100
 77 81.5 65.4 98.2
 51 27.6 21.8 32.8



#17
 N-Nitroso-di-n-propylamine
 Concen: 22.226 ng/ul
 RT: 8.863 min Scan# 965
 Delta R.T. 0.006 min
 Lab File: BP014220.D
 Acq: 22 Mar 2023 15:14

Tgt Ion: 70 Resp: 286487
 Ion Ratio Lower Upper
 70 100
 42 52.5 40.9 61.3
 101 9.4 7.9 11.9
 130 18.3 16.6 25.0


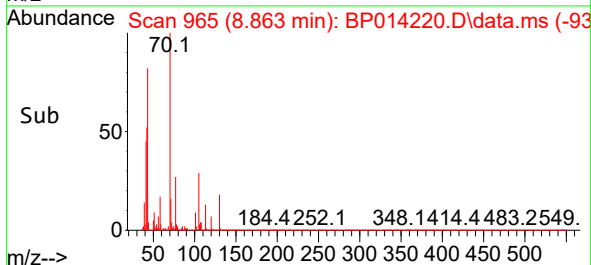
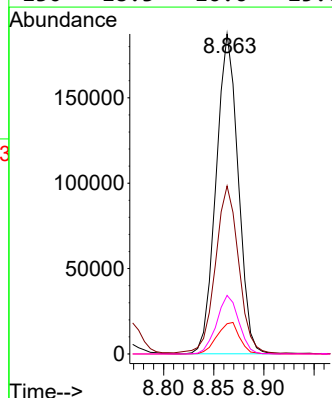
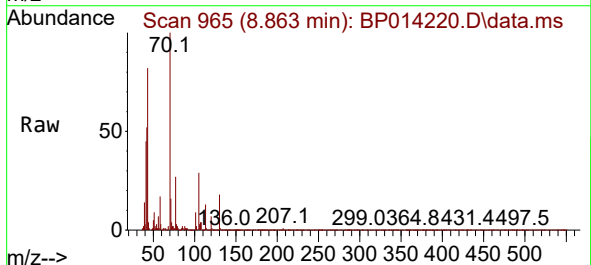




#18
4-Methylphenol
Concen: 21.644 ng/ul
RT: 8.828 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:108 Resp: 348575
Ion Ratio Lower Upper
108 100
107 113.7 89.8 134.6

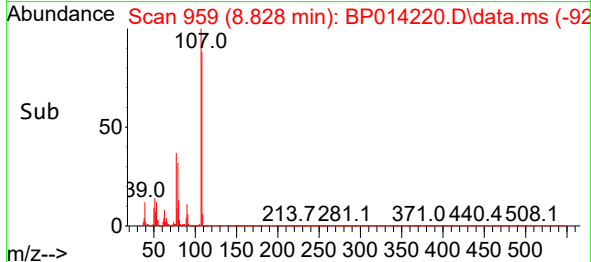

#19
Hexachloroethane
Concen: 21.139 ng/ul
RT: 9.134 min Scan# 1011
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:117 Resp: 135695
Ion Ratio Lower Upper
117 100
201 110.8 91.7 137.5
199 70.8 59.1 88.7


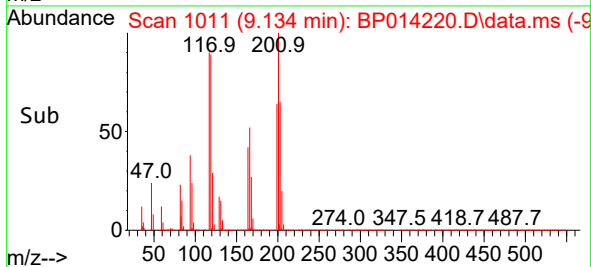

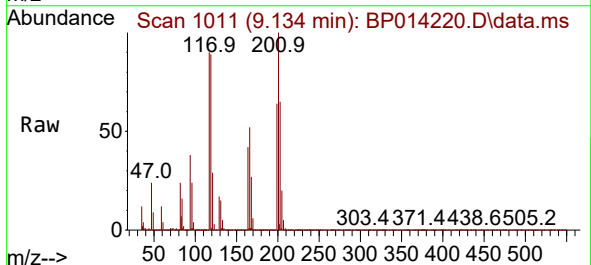




#22
Nitrobenzene
Concen: 21.065 ng/ul
RT: 9.269 min Scan# 1034
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 430207
Ion Ratio Lower Upper
77 100
123 39.5 32.6 48.8
65 13.4 11.2 16.8



#23
Isophorone
Concen: 20.304 ng/ul
RT: 9.793 min Scan# 1123
Delta R.T. -0.000 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion: 82 Resp: 798558
Ion Ratio Lower Upper
82 100
95 8.1 7.1 10.7
138 15.5 13.3 19.9

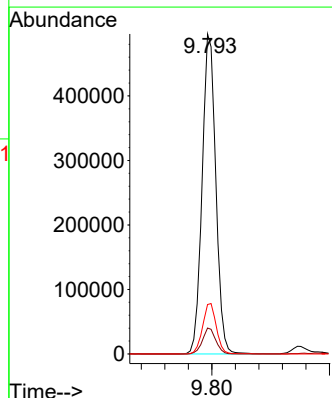



#25

2-Nitrophenol

Concen: 20.220 ng/ul

RT: 9.981 min Scan# 1154

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:139 Resp: 190456

Ion Ratio Lower Upper

139 100

65 59.9 46.6 70.0

109 37.7 34.5 51.7



#26

2,4-Dimethylphenol

Concen: 19.999 ng/ul

RT: 10.040 min Scan# 1165

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:107 Resp: 412309


Ion Ratio Lower Upper

107 100

121 45.8 37.1 55.7

122 77.7 61.2 91.8



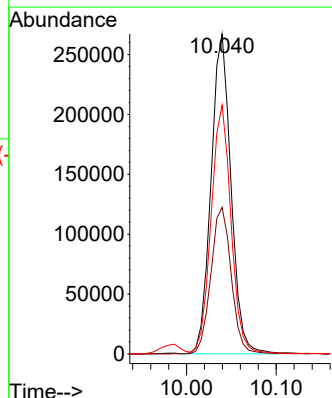





#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.603 ng/ul
 RT: 10.275 min Scan# 1205
 Delta R.T. 0.006 min
 Lab File: BP014220.D
 Acq: 22 Mar 2023 15:14




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 93 Resp: 468705
 Ion Ratio Lower Upper
 93 100
 95 32.0 25.6 38.4
 123 10.4 8.5 12.7



#29
 2,4-Dichlorophenol
 Concen: 19.267 ng/ul
 RT: 10.522 min Scan# 1247
 Delta R.T. 0.006 min
 Lab File: BP014220.D
 Acq: 22 Mar 2023 15:14

Tgt Ion: 162 Resp: 326814
 Ion Ratio Lower Upper
 162 100
 164 67.3 52.0 78.0
 98 39.2 29.1 43.7




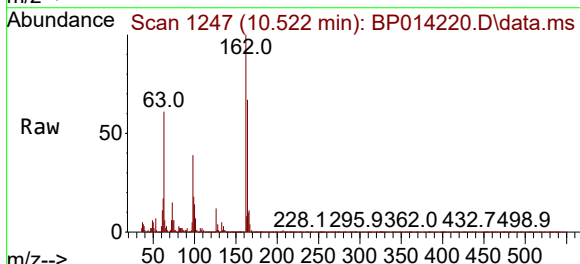




#30
Naphthalene
Concen: 20.070 ng/ul
RT: 10.922 min Scan# 1315
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:128 Resp: 1054560
Ion Ratio Lower Upper
128 100
129 10.9 8.5 12.7
127 13.5 11.0 16.4



#32
4-Chloroaniline
Concen: 19.600 ng/ul
RT: 11.040 min Scan# 1335
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:127 Resp: 448828
Ion Ratio Lower Upper
127 100
129 31.1 24.9 37.3

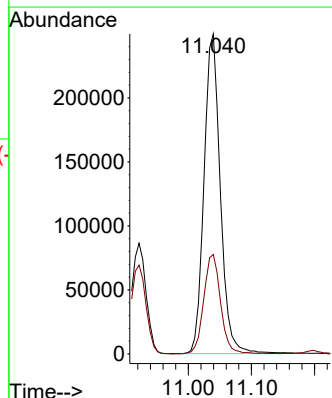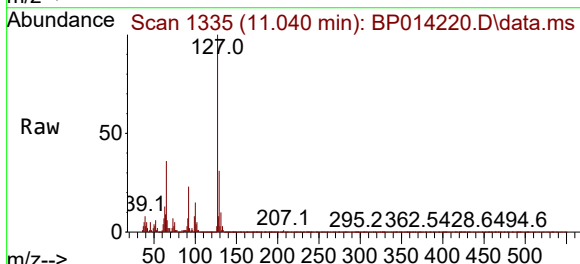



#33

Hexachlorobutadiene

Concen: 17.877 ng/ul

RT: 11.198 min Scan# 11

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:225 Resp: 241301

Ion Ratio Lower Upper

225 100

223 61.9 48.0 72.0

227 64.4 50.3 75.5

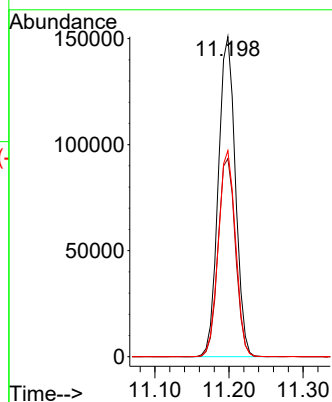

#34

Caprolactam

Concen: 13.250 ng/ul

RT: 11.828 min Scan# 1469

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:113 Resp: 72980


Ion Ratio Lower Upper

113 100

55 172.1 124.0 186.0

56 128.5 102.0 153.0









#35
4-Chloro-3-methylphenol
Concen: 20.275 ng/ul
RT: 12.157 min Scan# 1525
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:107 Resp: 397688
Ion Ratio Lower Upper
107 100
144 22.4 19.4 29.0
142 70.5 59.6 89.4



#36
2-Methylnaphthalene
Concen: 19.616 ng/ul
RT: 12.522 min Scan# 1587
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:142 Resp: 722931
Ion Ratio Lower Upper
142 100
141 90.4 71.7 107.5

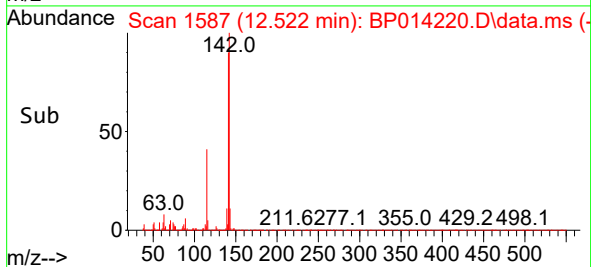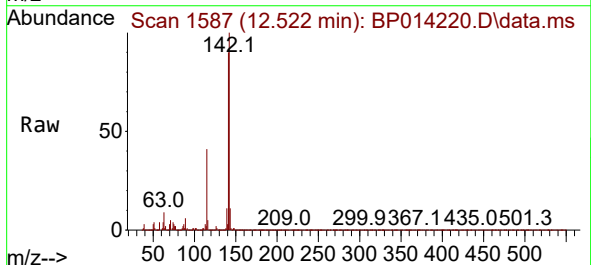



#37

1-Methylnaphthalene

Concen: 19.428 ng/ul

RT: 12.740 min Scan# 1623

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:142 Resp: 719669

Ion Ratio Lower Upper

142 100

141 93.0 73.8 110.6

116 4.3 3.7 5.5



#39

1,2,4,5-Tetrachlorobenzene

Concen: 18.782 ng/ul

RT: 12.887 min Scan# 1649

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Tgt Ion:216 Resp: 443978




Ion Ratio Lower Upper


216 100

214 78.8 61.7 92.5

179 19.9 16.2 24.4

108 16.8 13.2 19.8

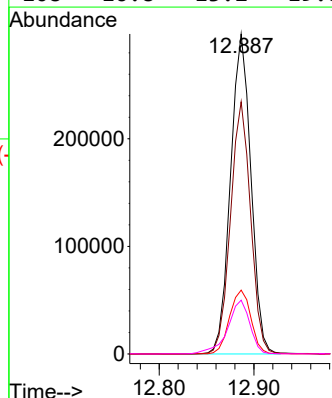



#40

Hexachlorocyclopentadiene

Concen: 13.802 ng/ul

RT: 12.857 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:237 Resp: 233625

Ion Ratio Lower Upper

237 100

235 64.2 49.0 73.6

272 13.5 9.6 14.4

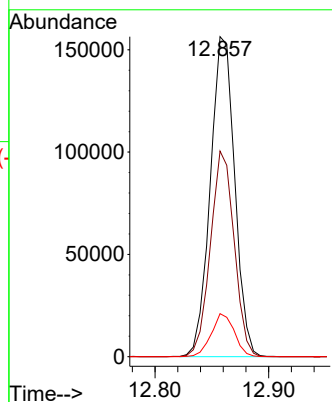

#41

2,4,6-Trichlorophenol

Concen: 19.409 ng/ul

RT: 13.128 min Scan# 1690

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:196 Resp: 288206


Ion Ratio Lower Upper

196 100

198 98.7 78.5 117.7

200 31.7 25.4 38.0





#42

2,4,5-Trichlorophenol

Concen: 19.533 ng/ul

RT: 13.204 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:196 Resp: 318312

Ion Ratio Lower Upper

196 100

198 97.4 77.6 116.4

200 30.7 25.3 37.9

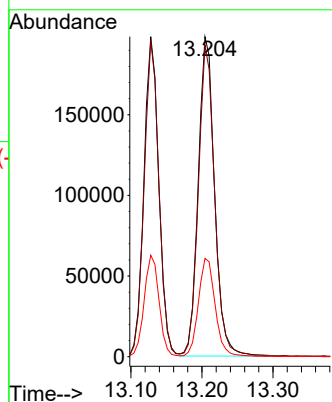

#43

1,1'-Biphenyl

Concen: 19.938 ng/ul

RT: 13.522 min Scan# 1757

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:154 Resp: 1003381


Ion Ratio Lower Upper

154 100

153 40.9 32.6 49.0

76 13.8 9.4 14.0





#44

2-Chloronaphthalene

Concen: 20.167 ng/ul

RT: 13.569 min Scan# 1764

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:162 Resp: 806063

Ion Ratio Lower Upper

162 100

164 33.1 26.0 39.0

127 40.6 31.3 46.9

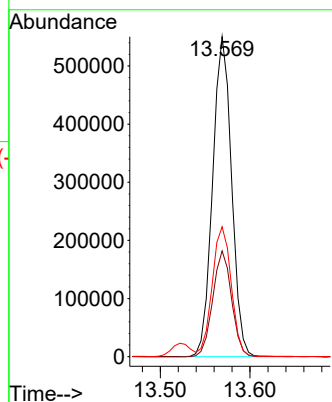

#45

2-Nitroaniline

Concen: 22.330 ng/ul

RT: 13.781 min Scan# 1801

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion: 65 Resp: 263971


Ion Ratio Lower Upper

65 100

92 70.1 56.3 84.5

138 92.7 81.4 122.2









#47
Dimethylphthalate
Concen: 19.062 ng/ul
RT: 14.139 min Scan# 1861
Delta R.T. -0.000 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:163 Resp: 1046743
Ion Ratio Lower Upper
163 100
194 4.0 3.6 5.4
164 10.3 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 20.023 ng/ul
RT: 14.269 min Scan# 1884
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:165 Resp: 217370
Ion Ratio Lower Upper
165 100
89 62.9 51.7 77.5
121 21.6 17.5 26.3





#50

Acenaphthylene

Concen: 20.307 ng/ul

RT: 14.416 min Scan# 1909

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:152 Resp: 1252433

Ion Ratio Lower Upper

152 100

151 19.8 16.2 24.2

153 13.2 10.4 15.6



#51

3-Nitroaniline

Concen: 21.522 ng/ul

RT: 14.604 min Scan# 1941

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:138 Resp: 206876


Ion Ratio Lower Upper

138 100

108 12.7 10.5 15.7


92 132.2 98.5 147.7

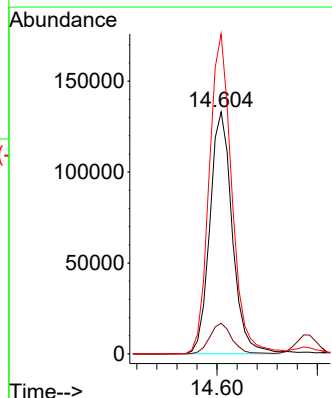






#52
Acenaphthene
Concen: 20.144 ng/ul
RT: 14.751 min Scan# 1966
Delta R.T. -0.000 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:153 Resp: 868523
Ion Ratio Lower Upper
153 100
152 47.2 37.7 56.5
154 88.5 70.4 105.6



#53
2,4-Dinitrophenol
Concen: 14.323 ng/ul
RT: 14.810 min Scan# 1976
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:184 Resp: 116122
Ion Ratio Lower Upper
184 100
63 70.0 51.9 77.9
154 72.7 58.8 88.2




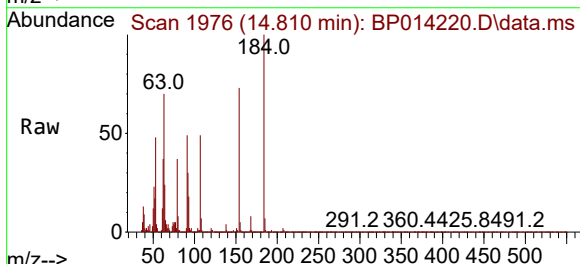




#55
4-Nitrophenol
Concen: 15.625 ng/ul
RT: 14.916 min Scan# 1994
Delta R.T. 0.012 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:109 Resp: 165006
Ion Ratio Lower Upper
109 100
139 107.3 74.5 111.7
65 119.9 86.6 130.0



#56
Dibenzofuran
Concen: 19.425 ng/ul
RT: 15.086 min Scan# 2023
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:168 Resp: 1218400
Ion Ratio Lower Upper
168 100
139 39.7 31.8 47.6





#57

2,4-Dinitrotoluene

Concen: 19.708 ng/ul

RT: 15.057 min Scan# 2017

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:165 Resp: 319669

Ion Ratio Lower Upper

165 100

63 49.0 34.6 52.0

182 3.1 2.2 3.2



#58

2,3,4,6-Tetrachlorophenol

Concen: 18.755 ng/ul

RT: 15.316 min Scan# 2062

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Tgt Ion:232 Resp: 292408




Ion Ratio Lower Upper


232 100

131 40.6 34.1 51.1

130 2.4 2.1 3.1

166 28.9 23.0 34.6



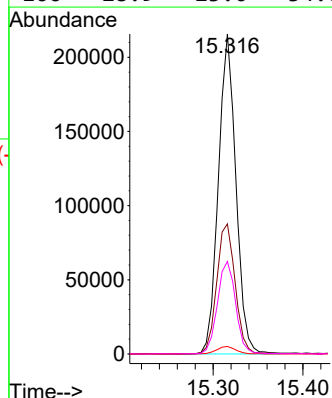





#59
Diethylphthalate
Concen: 19.281 ng/ul
RT: 15.498 min Scan# 2092
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:149 Resp: 1073871
Ion Ratio Lower Upper
149 100
177 22.2 18.2 27.2
150 12.9 10.0 15.0

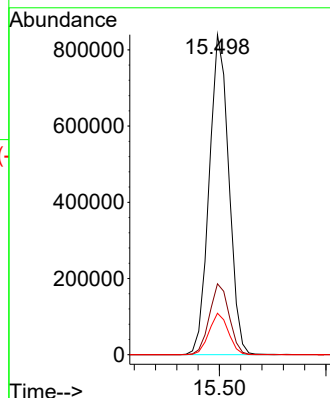

#61
Fluorene
Concen: 19.560 ng/ul
RT: 15.739 min Scan# 2134
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:166 Resp: 1016996
Ion Ratio Lower Upper
166 100
165 97.4 78.9 118.3
167 12.8 11.0 16.6



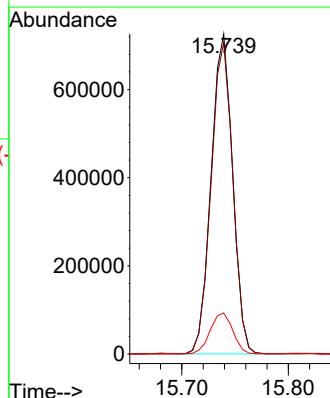
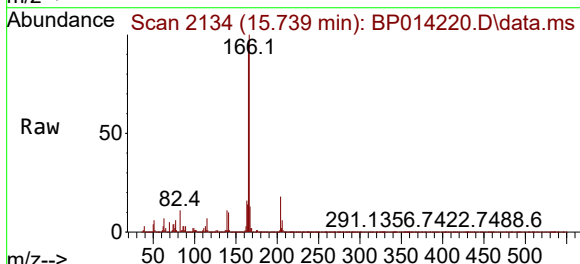




#62
4-Chlorophenyl-phenylether
Concen: 18.697 ng/ul
RT: 15.728 min Scan# 2131
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:204 Resp: 536540
Ion Ratio Lower Upper
204 100
206 33.6 26.6 39.8
141 61.1 49.2 73.8



#63
4-Nitroaniline
Concen: 22.376 ng/ul
RT: 15.769 min Scan# 2139
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:138 Resp: 221084
Ion Ratio Lower Upper
138 100
92 57.7 44.5 66.7
108 99.8 87.2 130.8




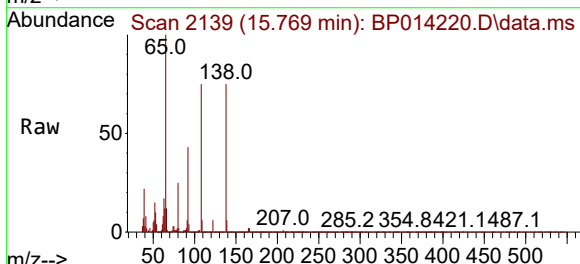




#66
4,6-Dinitro-2-methylphenol
Concen: 17.599 ng/ul
RT: 15.822 min Scan# 2148
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:198 Resp: 192972
Ion Ratio Lower Upper
198 100
182 3.9 3.0 4.6
77 25.9 20.3 30.5

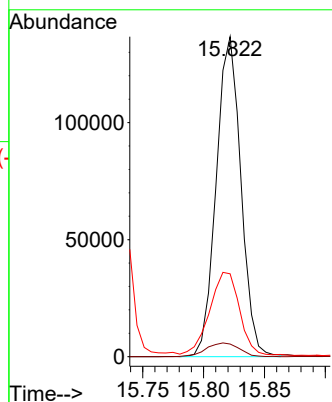

#67
N-Nitrosodiphenylamine
Concen: 20.247 ng/ul
RT: 15.945 min Scan# 2169
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:169 Resp: 869567
Ion Ratio Lower Upper
169 100
168 66.5 53.7 80.5
167 36.1 28.6 43.0


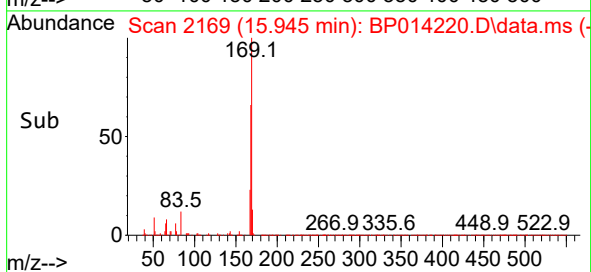
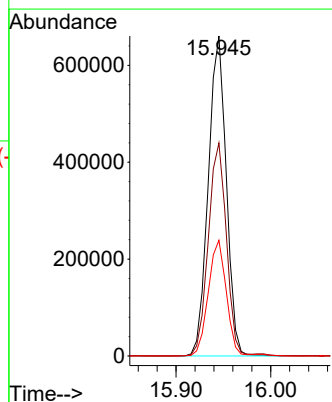





#68
4-Bromophenyl-phenylether
Concen: 18.827 ng/ul
RT: 16.628 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:248 Resp: 346094
Ion Ratio Lower Upper
248 100
250 98.3 78.8 118.2
141 74.7 60.8 91.2



#69
Hexachlorobenzene
Concen: 18.494 ng/ul
RT: 16.745 min Scan# 2305
Delta R.T. 0.006 min
Lab File: BP014220.D
Acq: 22 Mar 2023 15:14

Tgt Ion:284 Resp: 400631
Ion Ratio Lower Upper
284 100
142 30.9 23.2 34.8
249 31.8 25.7 38.5





#70

Atrazine

Concen: 19.011 ng/ul

RT: 16.898 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:200 Resp: 352150

Ion Ratio Lower Upper

200 100

173 25.8 19.0 28.4

215 47.4 38.5 57.7



#71

Pentachlorophenol

Concen: 16.529 ng/ul

RT: 17.092 min Scan# 2364

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:266 Resp: 234055


Ion Ratio Lower Upper

266 100

264 63.8 48.4 72.6

268 63.5 50.4 75.6

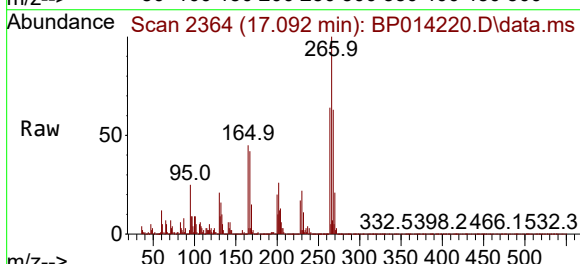



#72

Phenanthrene

Concen: 19.867 ng/ul

RT: 17.486 min Scan# 2430

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:178 Resp: 1647756

Ion Ratio Lower Upper

178 100

179 15.4 12.2 18.4

176 19.7 15.4 23.0



#74

Anthracene

Concen: 20.147 ng/ul

RT: 17.580 min Scan# 2447

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:178 Resp: 1694302


Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7

176 19.0 15.1 22.7

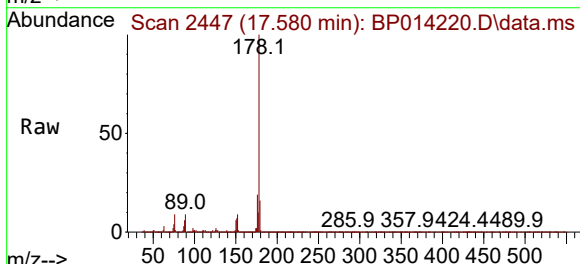



#75

1,2,3,4-Tetrachlorobenzene

Concen: 19.488 ng/uL

RT: 13.492 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:216 Resp: 454800

Ion Ratio Lower Upper

216 100

214 79.0 61.4 92.2

218 49.8 39.1 58.7

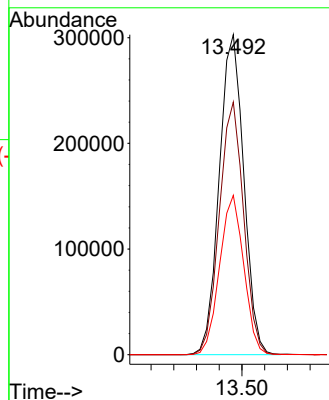

#76

Pentachlorobenzene

Concen: 19.076 ng/uL

RT: 15.004 min Scan# 2009

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:250 Resp: 462438


Ion Ratio Lower Upper

250 100

248 63.1 51.0 76.4

252 63.2 50.8 76.2

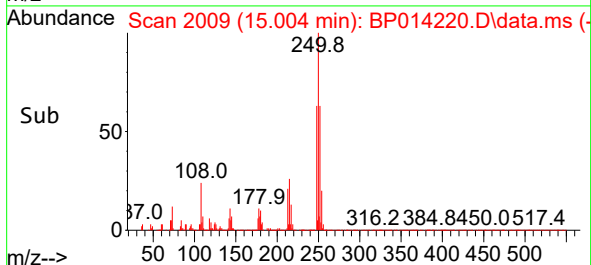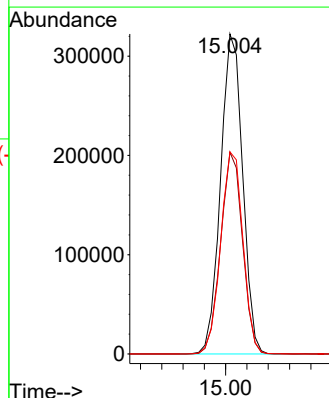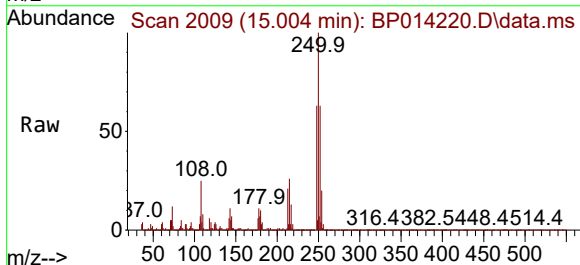



#77

Carbazole

Concen: 20.240 ng/ul

RT: 17.851 min Scan# 2491

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:167 Resp: 1501333

Ion Ratio Lower Upper

167 100

166 21.5 17.5 26.3

139 13.1 10.5 15.7



#78

Di-n-butylphthalate

Concen: 20.831 ng/ul

RT: 18.375 min Scan# 2582

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:149 Resp: 1931157


Ion Ratio Lower Upper

149 100

150 9.2 7.4 11.2

104 5.5 4.6 6.8

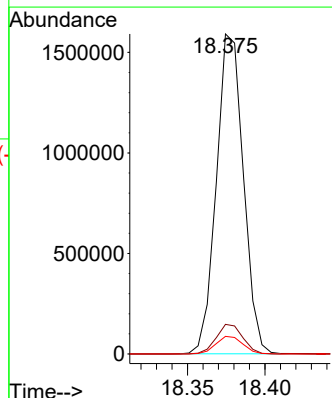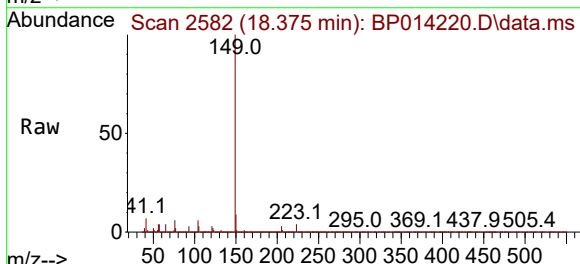



#80

Fluoranthene

Concen: 22.537 ng/ul

RT: 19.445 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:202 Resp: 2045404

Ion Ratio Lower Upper

202 100

101 9.7 6.6 10.0

100 7.6 5.0 7.4#

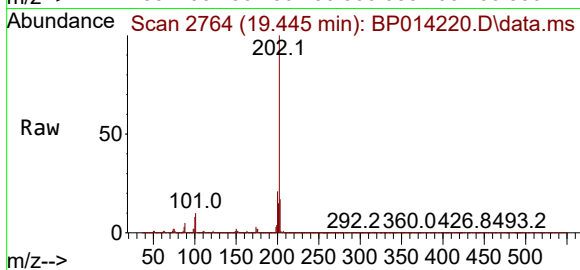

#82

Pyrene

Concen: 22.154 ng/ul

RT: 19.798 min Scan# 2824

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:202 Resp: 2097465


Ion Ratio Lower Upper

202 100

101 12.1 7.8 11.8#

100 9.5 6.5 9.7





#83

Butylbenzylphthalate

Concen: 24.069 ng/ul

RT: 20.651 min Scan# 2969

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 918828

Ion Ratio Lower Upper

149 100

91 74.5 57.9 86.9

206 22.6 17.9 26.9

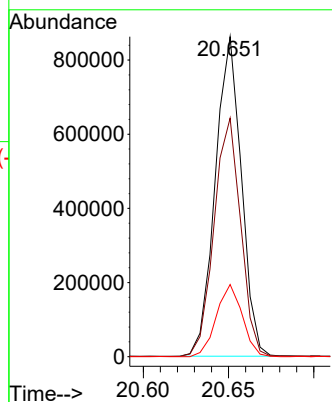

#84

3,3'-Dichlorobenzidine

Concen: 16.876 ng/ul

RT: 21.433 min Scan# 3102

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:252 Resp: 623717


Ion Ratio Lower Upper

252 100

254 63.9 51.3 76.9

126 9.7 6.9 10.3





#85

Benzo(a)anthracene

Concen: 20.048 ng/ul

RT: 21.510 min Scan# 3113

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 2035746

Ion Ratio Lower Upper

228 100

229 19.7 15.5 23.3

226 27.2 22.1 33.1

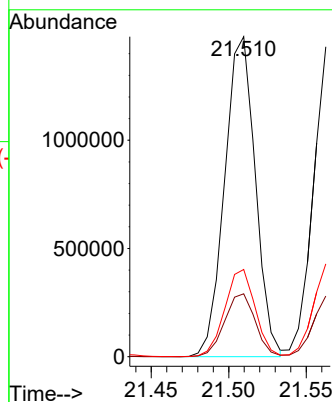

#86

Bis(2-ethylhexyl)phthalate

Concen: 23.911 ng/ul

RT: 21.404 min Scan# 3097

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:149 Resp: 1364702


Ion Ratio Lower Upper

149 100

167 27.8 22.3 33.5

279 5.0 4.3 6.5





#87

Chrysene

Concen: 19.661 ng/ul

RT: 21.563 min Scan# 31

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 1902632

Ion Ratio Lower Upper

228 100

226 30.0 24.2 36.2

229 19.6 15.7 23.5

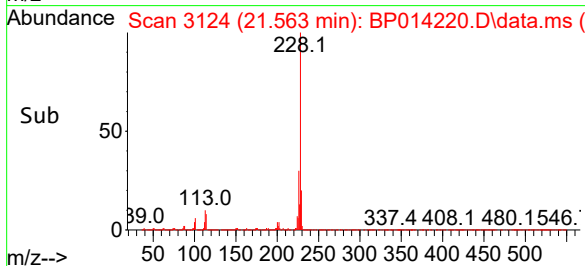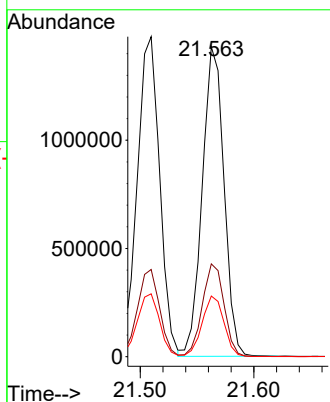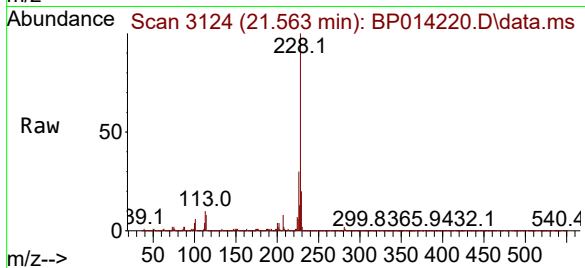

#89

Di-n-octyl phthalate

Concen: 28.080 ng/ul




RT: 22.363 min Scan# 3260


Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Tgt Ion:149 Resp: 2304228

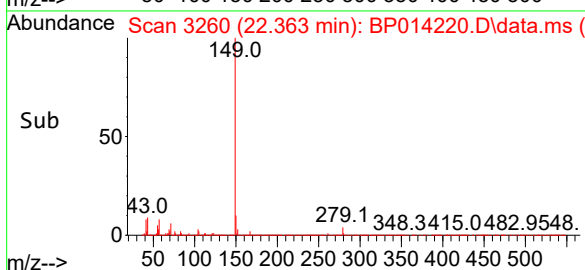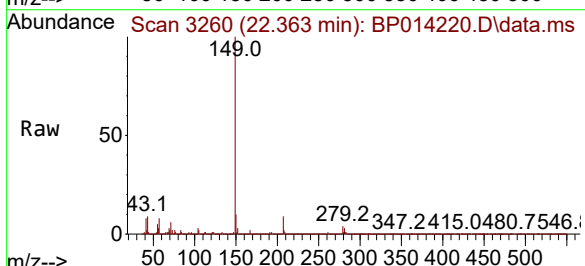



#90

Benzo(b)fluoranthene

Concen: 20.731 ng/ul

RT: 23.268 min Scan# 3412

Delta R.T. 0.006 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 1796526

Ion Ratio Lower Upper

252 100

253 22.4 17.3 25.9

125 7.7 5.4 8.2



#91

Benzo(k)fluoranthene

Concen: 21.452 ng/ul

RT: 23.321 min Scan# 3423

Delta R.T. 0.012 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:252 Resp: 1772666


Ion Ratio Lower Upper

252 100

253 21.8 17.4 26.0

125 7.9 5.5 8.3





#93

Benzo(a)pyrene

Concen: 19.935 ng/ul

RT: 23.933 min Scan# 3

Delta R.T. 0.012 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 1502576

Ion Ratio Lower Upper

252 100

253 22.0 17.4 26.2

125 8.7 6.2 9.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 17.496 ng/ul

RT: 26.692 min Scan# 3996

Delta R.T. 0.018 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14




Tgt Ion:276 Resp: 1745805


Ion Ratio Lower Upper

276 100

138 19.5 13.1 19.7

277 25.2 20.2 30.2

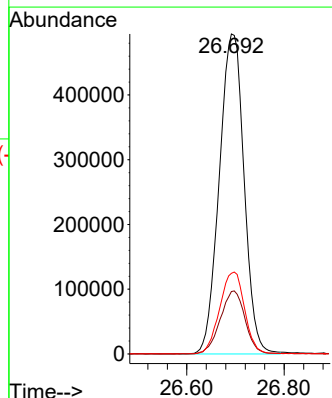



#95

Dibenzo(a,h)anthracene

Concen: 17.597 ng/ul

RT: 26.709 min Scan# 3999

Delta R.T. 0.018 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:278 Resp: 1459348

Ion Ratio Lower Upper

278 100

139 12.2 8.7 13.1

279 23.5 19.0 28.4



#96

Benzo(g,h,i)perylene

Concen: 17.333 ng/ul

RT: 27.509 min Scan# 4135

Delta R.T. 0.018 min

Lab File: BP014220.D

Acq: 22 Mar 2023 15:14

Tgt Ion:276 Resp: 1382362

Ion Ratio Lower Upper

276 100

138 16.6 11.9 17.9

277 24.7 18.7 28.1

