

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014143.D
 Acq On : 20 Mar 2023 16:44
 Operator : CG/JU
 Sample : 01927-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAQ4

Quant Time: Mar 21 00:47:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	179412	20.000	ng/u1	0.00
20) Naphthalene-d8	10.875	136	735346	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.692	164	494354	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.451	188	1156218	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1057964	20.000	ng/u1	0.00
88) Perylene-d12	24.057	264	948801	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	15279	3.218	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.210	99	306237	19.342	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	191244	20.712	ng/u1	0.00
11) 2-Chlorophenol-d4	7.581	132	246794	20.459	ng/u1	0.00
15) 4-Methylphenol-d8	8.763	113	243528	18.830	ng/u1	0.00
21) Nitrobenzene-d5	9.228	128	120191	20.485	ng/u1	0.00
24) 2-Nitrophenol-d4	9.951	143	144686	20.600	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.499	165	257588	19.492	ng/u1	0.00
31) 4-Chloroaniline-d4	11.022	131	53910	3.083	ng/u1	0.00
46) Dimethylphthalate-d6	14.098	166	844528	20.130	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	925538	20.825	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	113926	15.409	ng/u1	0.00
60) Fluorene-d10	15.686	176	727407	20.458	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	146160	16.726	ng/u1	0.00
73) Anthracene-d10	17.551	188	1174723	20.929	ng/u1	0.00
81) Pyrene-d10	19.774	212	1499993	25.707	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.892	264	1123398	22.259	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.887	105	37150	1.778	ng/u1	98
86) Bis(2-ethylhexyl)phtha...	21.410	149	158583	3.792	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014143.D
Acq On : 20 Mar 2023 16:44
Operator : CG/JU
Sample : 01927-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAQ4

Quant Time: Mar 21 00:47:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 20 13:12:59 2023
Response via : Initial Calibration




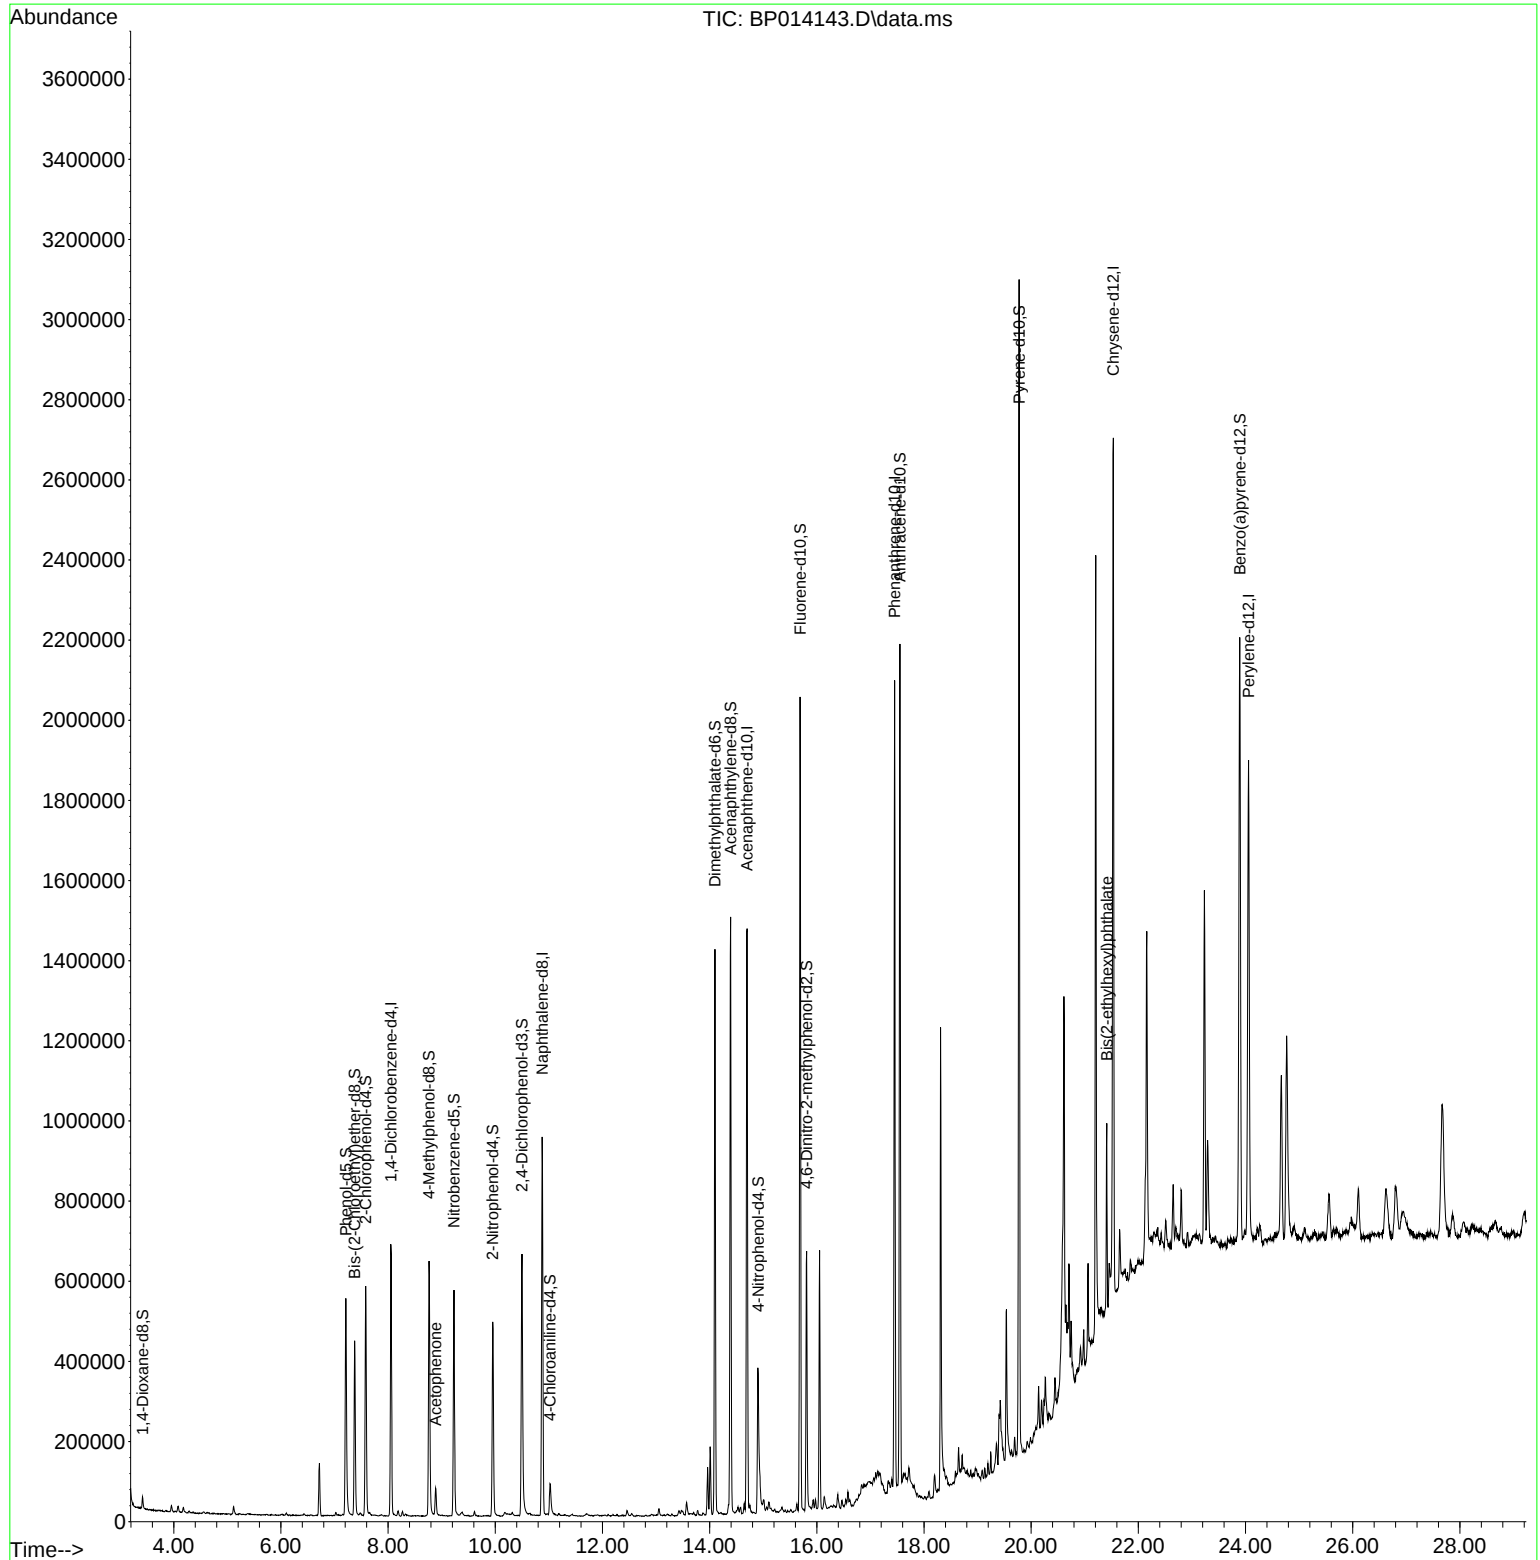


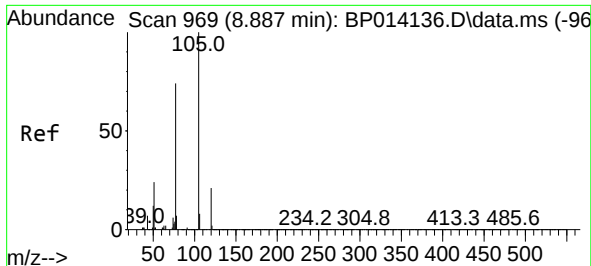

#16
Acetophenone
Concen: 1.778 ng/ul
RT: 8.887 min Scan# 969
Delta R.T. 0.000 min
Lab File: BP014143.D
Acq: 20 Mar 2023 16:44

Instrument :
BNA_P
ClientSampleId :
DCAQ4

Tgt Ion:	105	Resp:	37150
Ion Ratio	Lower	Upper	
105	100		
77	83.6	65.4	98.2
51	28.4	21.8	32.8

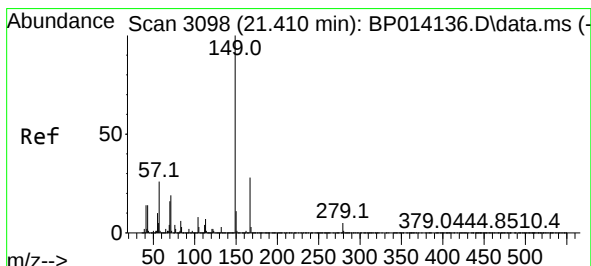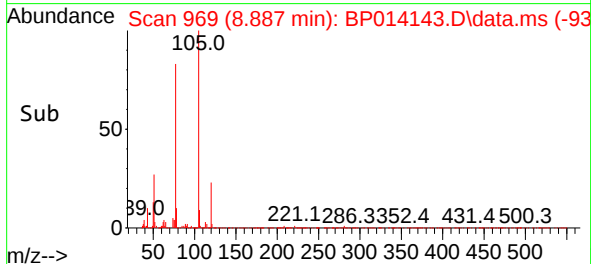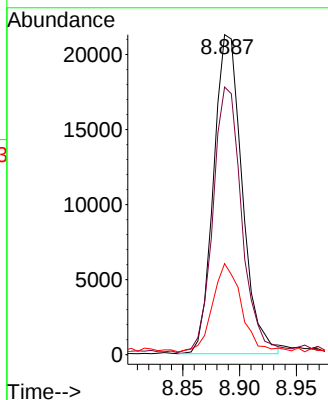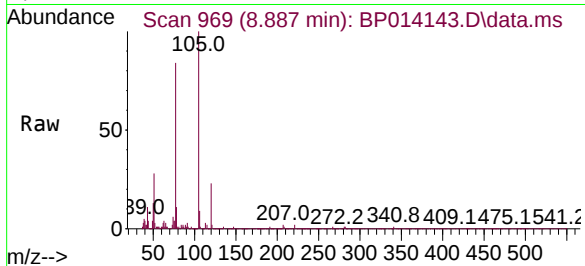

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.792 ng/ul
RT: 21.410 min Scan# 3098
Delta R.T. 0.000 min
Lab File: BP014143.D
Acq: 20 Mar 2023 16:44

Tgt Ion:	149	Resp:	158583
Ion Ratio	Lower	Upper	
149	100		
167	28.0	22.3	33.5
279	5.3	4.3	6.5

