

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014160.D
 Acq On : 21 Mar 2023 02:27
 Operator : CG/JU
 Sample : 01885-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB919

Quant Time: Mar 21 03:03:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:12:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	210228	20.000	ng/u1	0.00
20) Naphthalene-d8	10.875	136	882640	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.692	164	586587	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1328043	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.521	240	1177376	20.000	ng/u1	#-0.01
88) Perylene-d12	24.045	264	1021423	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	20343	3.656	ng/uL	0.00
4) Pyridine-d5	3.852	84	123883	8.041	ng/u1	0.00
7) Phenol-d5	7.210	99	121189	6.532	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	397253	36.716	ng/u1	0.00
11) 2-Chlorophenol-d4	7.581	132	345438	24.439	ng/u1	0.00
15) 4-Methylphenol-d8	8.763	113	267376	17.644	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	257239	36.526	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.951	143	274058	32.509	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.492	165	458394	28.898	ng/u1	0.00
31) 4-Chloroaniline-d4	11.016	131	301836	14.379	ng/u1	0.00
46) Dimethylphthalate-d6	14.098	166	1842560	37.012	ng/u1	0.00
49) Acenaphthylene-d8	14.386	160	2007624	38.069	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	44967	5.126	ng/u1	0.01
60) Fluorene-d10	15.680	176	1539115	36.480	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.804	200	293131	29.204	ng/u1	0.00
73) Anthracene-d10	17.545	188	2419508	37.529	ng/u1	-0.01
81) Pyrene-d10	19.768	212	2857791	44.009	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	2072924	38.153	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.452	88	60972	10.151	ng/uL	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014160.D
Acq On : 21 Mar 2023 02:27
Operator : CG/JU
Sample : 01885-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB919


Quant Time: Mar 21 03:03:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 20 13:12:59 2023
Response via : Initial Calibration

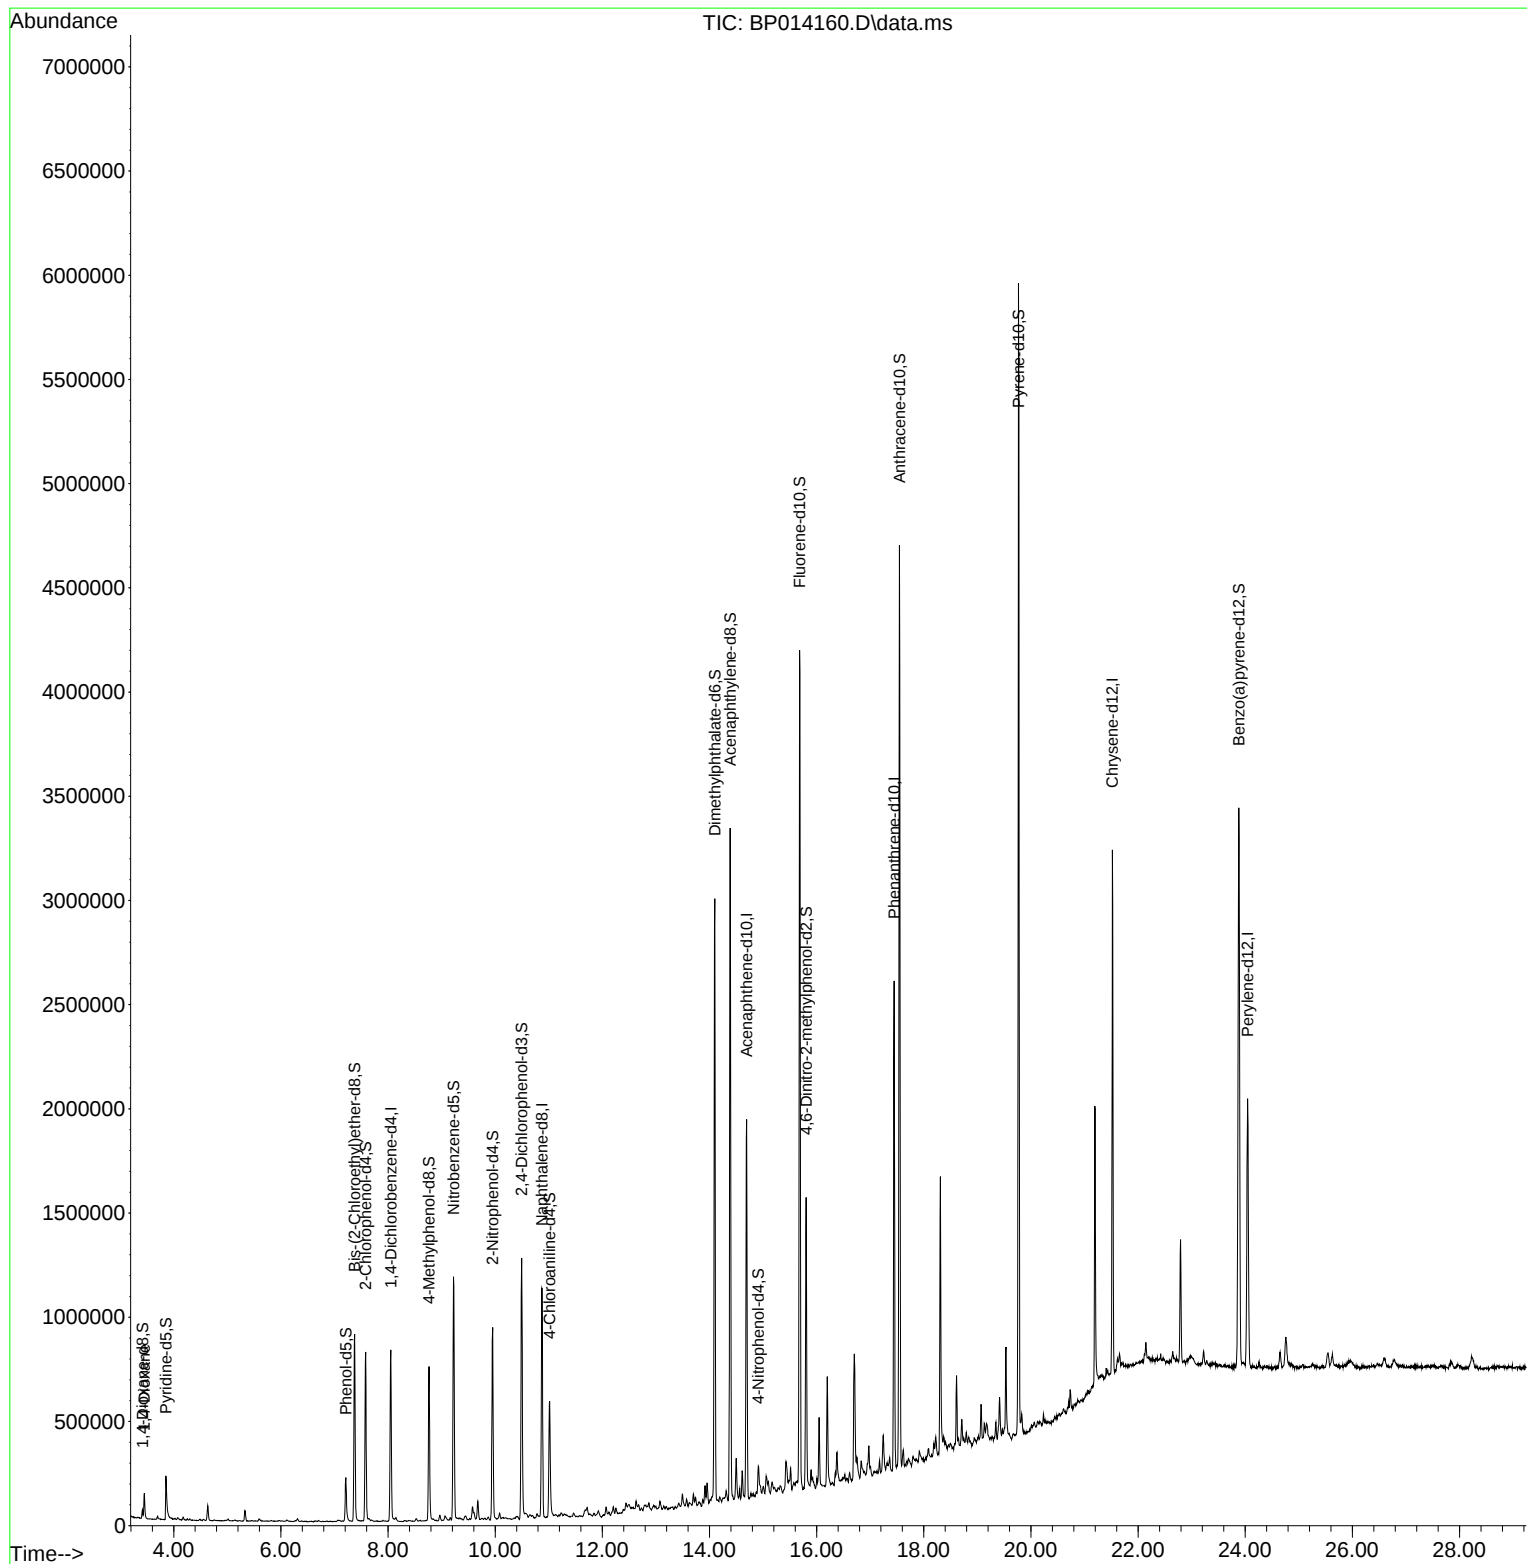

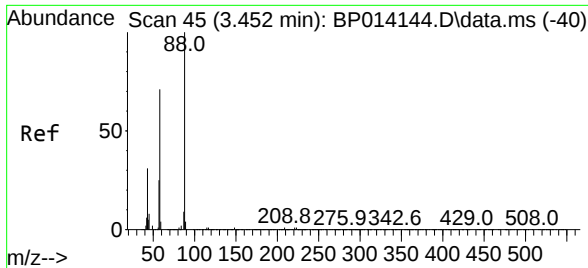

#2
 1,4-Dioxane
 Concen: 10.151 ng/uL
 RT: 3.452 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP014160.D
 Acq: 21 Mar 2023 02:27

Instrument :
 BNA_P
 ClientSampleId :
 CB919

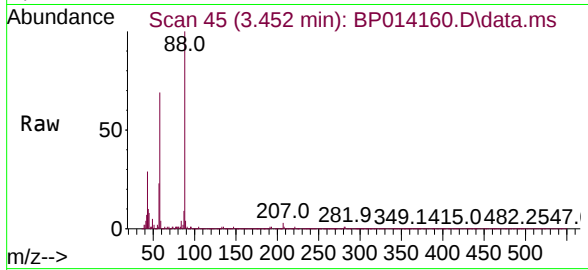

Tgt Ion: 88 Resp: 60972
 Ion Ratio Lower Upper
 88 100
 43 28.8 23.9 35.9
 58 68.8 50.2 75.2

