

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014177.D
 Acq On : 21 Mar 2023 12:41
 Operator : CG/JU
 Sample : 01996-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A29

Quant Time: Mar 22 01:18:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 21 04:47:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	180193	20.000	ng/u1	0.00
20) Naphthalene-d8	10.869	136	778554	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.687	164	517027	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.440	188	1181962	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.522	240	1002553	20.000	ng/u1	# 0.00
88) Perylene-d12	24.039	264	866085	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	31446	6.594	ng/uL	0.00
4) Pyridine-d5	3.864	84	31726	2.403	ng/u1	0.02
7) Phenol-d5	7.205	99	267635	16.831	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	361579	38.989	ng/u1	0.00
11) 2-Chlorophenol-d4	7.575	132	397934	32.846	ng/u1	0.00
15) 4-Methylphenol-d8	8.764	113	306054	23.563	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	230895	37.169	ng/u1	0.00
24) 2-Nitrophenol-d4	9.946	143	268090	36.052	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	465948	33.302	ng/u1	0.00
31) 4-Chloroaniline-d4	11.022	131	42152	2.276	ng/u1	0.01
46) Dimethylphthalate-d6	14.093	166	1638534	37.342	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	1770736	38.095	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	110817	14.331	ng/u1	0.00
60) Fluorene-d10	15.681	176	1404943	37.780	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	301725	33.775	ng/u1	0.00
73) Anthracene-d10	17.545	188	2219174	38.676	ng/u1	0.00
81) Pyrene-d10	19.769	212	2622182	47.423	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.874	264	1801433	39.103	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.446	88	244529	47.495	ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014177.D
Acq On : 21 Mar 2023 12:41
Operator : CG/JU
Sample : 01996-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A29


Quant Time: Mar 22 01:18:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 21 04:47:07 2023
Response via : Initial Calibration

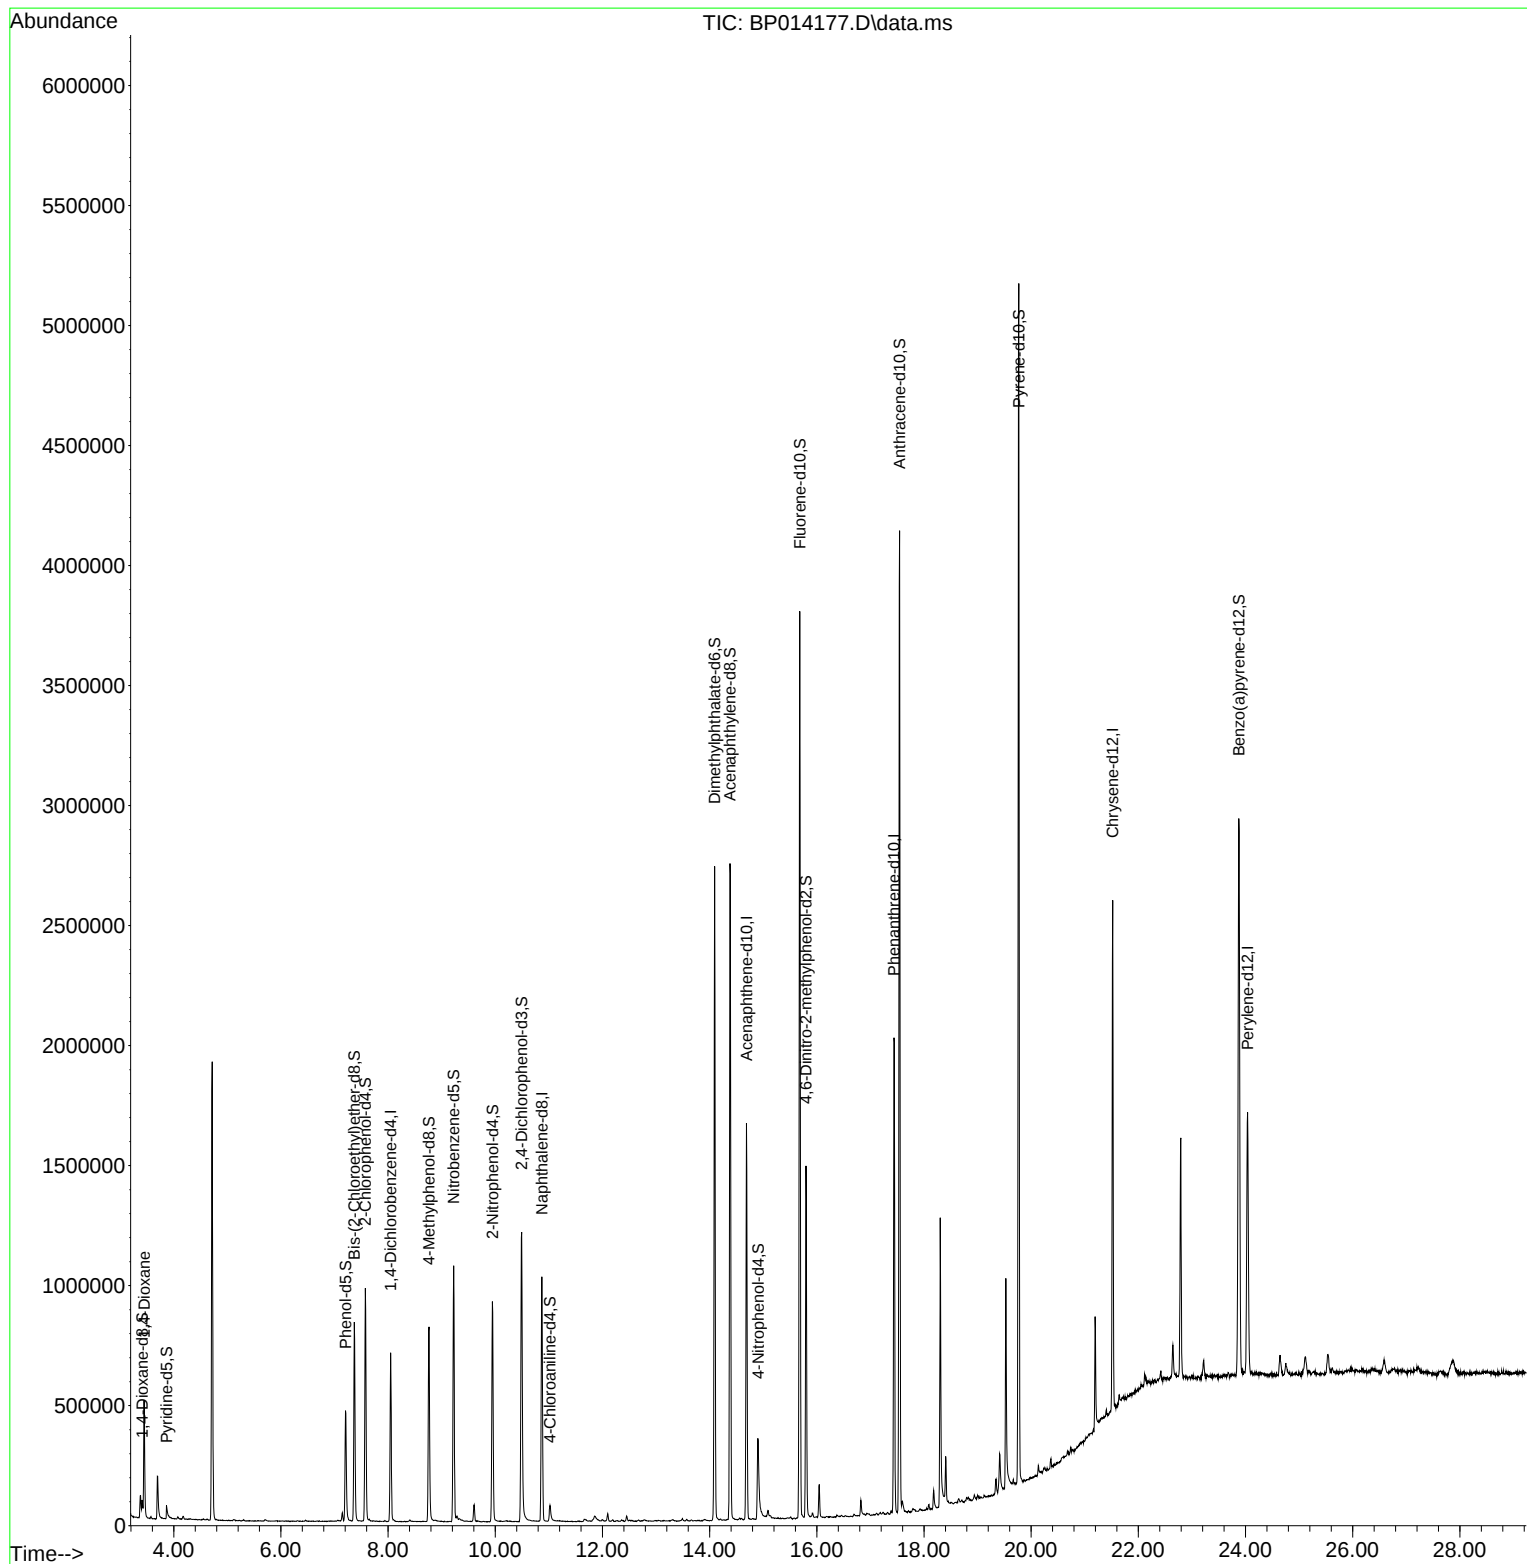

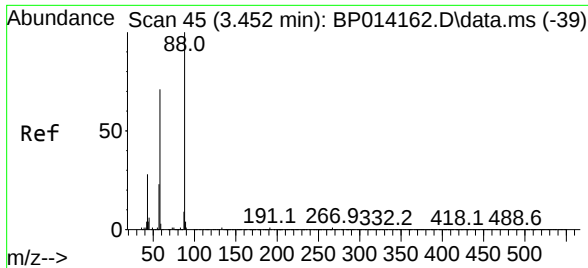

#2
 1,4-Dioxane
 Concen: 47.495 ng/uL
 RT: 3.446 min Scan# 44
 Delta R.T. -0.006 min
 Lab File: BP014177.D
 Acq: 21 Mar 2023 12:41

Instrument :
 BNA_P
 ClientSampleId :
 H0A29

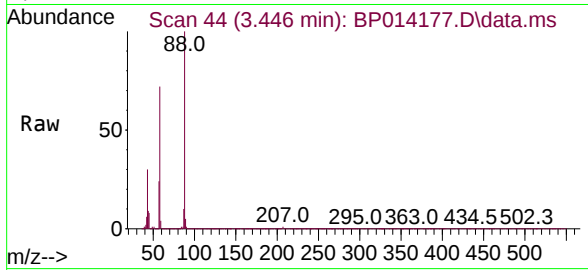

Tgt Ion:	88	Resp:	244529
Ion	Ratio	Lower	Upper
88	100		
43	29.5	23.9	35.9
58	72.0	50.2	75.2

