

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014189.D
 Acq On : 21 Mar 2023 20:02
 Operator : CG/JU
 Sample : 01949-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB929

Quant Time: Mar 22 01:22:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 21 04:47:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	195733	20.000	ng/u1	0.00
20) Naphthalene-d8	10.869	136	815502	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.686	164	547355	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1211011	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.521	240	952717	20.000	ng/u1	# 0.00
88) Perylene-d12	24.051	264	984460	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	20270	3.913	ng/uL	0.00
4) Pyridine-d5	3.852	84	214161	14.931	ng/u1	0.00
7) Phenol-d5	7.205	99	124513	7.209	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	280369	27.832	ng/u1	0.00
11) 2-Chlorophenol-d4	7.575	132	260191	19.772	ng/u1	0.00
15) 4-Methylphenol-d8	8.763	113	240322	17.033	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	174344	26.794	ng/u1	0.00
24) 2-Nitrophenol-d4	9.946	143	188453	24.195	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	315325	21.515	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	477467	24.618	ng/u1	0.00
46) Dimethylphthalate-d6	14.092	166	1195537	25.737	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	1336090	27.151	ng/u1	0.00
54) 4-Nitrophenol-d4	14.916	143	30298	3.701	ng/u1	0.02
60) Fluorene-d10	15.681	176	1033833	26.260	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	126542	13.825	ng/u1	0.00
73) Anthracene-d10	17.545	188	1638297	27.867	ng/u1	0.00
81) Pyrene-d10	19.769	212	1755920	33.417	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.886	264	1449779	27.686	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.446	88	245251	43.853	ng/uL	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014189.D
Acq On : 21 Mar 2023 20:02
Operator : CG/JU
Sample : 01949-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB929

Quant Time: Mar 22 01:22:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 21 04:47:07 2023
Response via : Initial Calibration

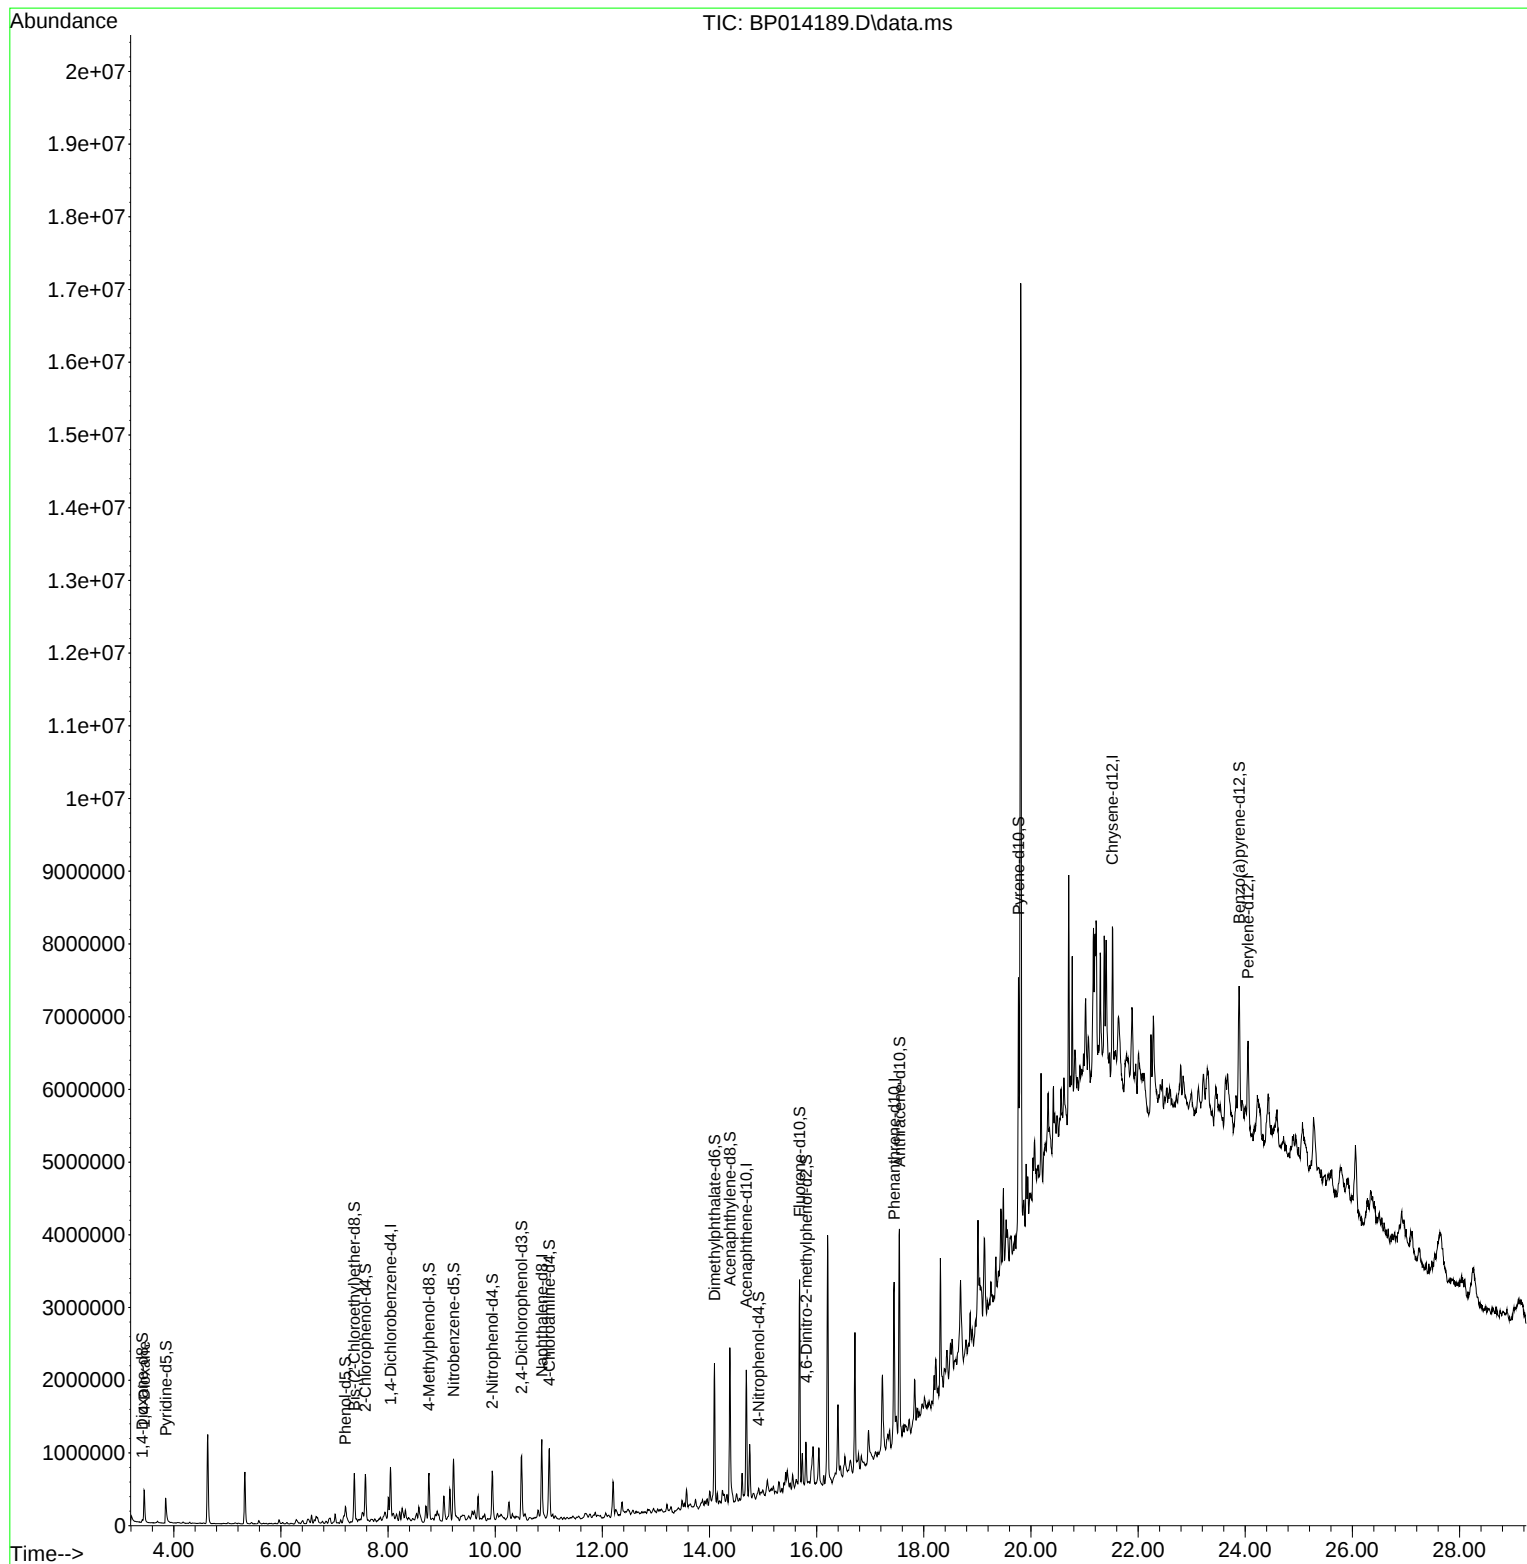

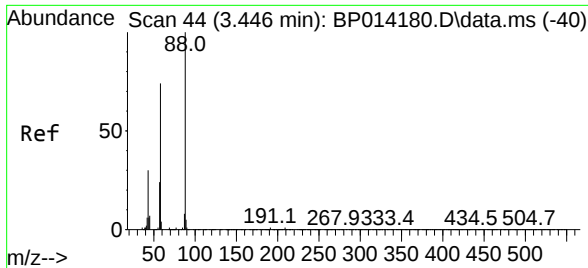

#2
 1,4-Dioxane
 Concen: 43.853 ng/uL
 RT: 3.446 min Scan# 44
 Delta R.T. -0.006 min
 Lab File: BP014189.D
 Acq: 21 Mar 2023 20:02

Instrument :
 BNA_P
 ClientSampleId :
 CB929

Tgt Ion: 88 Resp: 245251

Ion	Ratio	Lower	Upper
88	100		
43	28.6	23.9	35.9
58	71.4	50.2	75.2

