

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014205.D
 Acq On : 22 Mar 2023 05:43
 Operator : CG/JU
 Sample : 01949-02
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB931

Quant Time: Mar 22 06:08:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 22 03:05:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	188486	20.000	ng/u1	0.00
20) Naphthalene-d8	10.863	136	806110	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.681	164	537916	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.439	188	1223613	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.516	240	1115025	20.000	ng/u1	# 0.00
88) Perylene-d12	24.027	264	980441	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	18611	3.731	ng/uL	0.00
4) Pyridine-d5	3.846	84	178019	12.888	ng/u1	0.00
7) Phenol-d5	7.205	99	99496	5.982	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	261621	26.969	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	259831	20.503	ng/u1	0.00
15) 4-Methylphenol-d8	8.757	113	194108	14.286	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	163858	25.476	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	189255	24.581	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	340189	23.482	ng/u1	0.00
31) 4-Chloroaniline-d4	11.004	131	448433	23.390	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	1243964	27.249	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	1305634	26.998	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	34958	4.345	ng/u1	0.02
60) Fluorene-d10	15.675	176	1032882	26.697	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	167667	18.130	ng/u1	0.00
73) Anthracene-d10	17.533	188	1710597	28.798	ng/u1	0.00
81) Pyrene-d10	19.757	212	2006461	32.627	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.868	264	1501012	28.781	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.446	88	240170	44.596	ng/uL	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014205.D
Acq On : 22 Mar 2023 05:43
Operator : CG/JU
Sample : 01949-02
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB931

Quant Time: Mar 22 06:08:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 22 03:05:29 2023
Response via : Initial Calibration

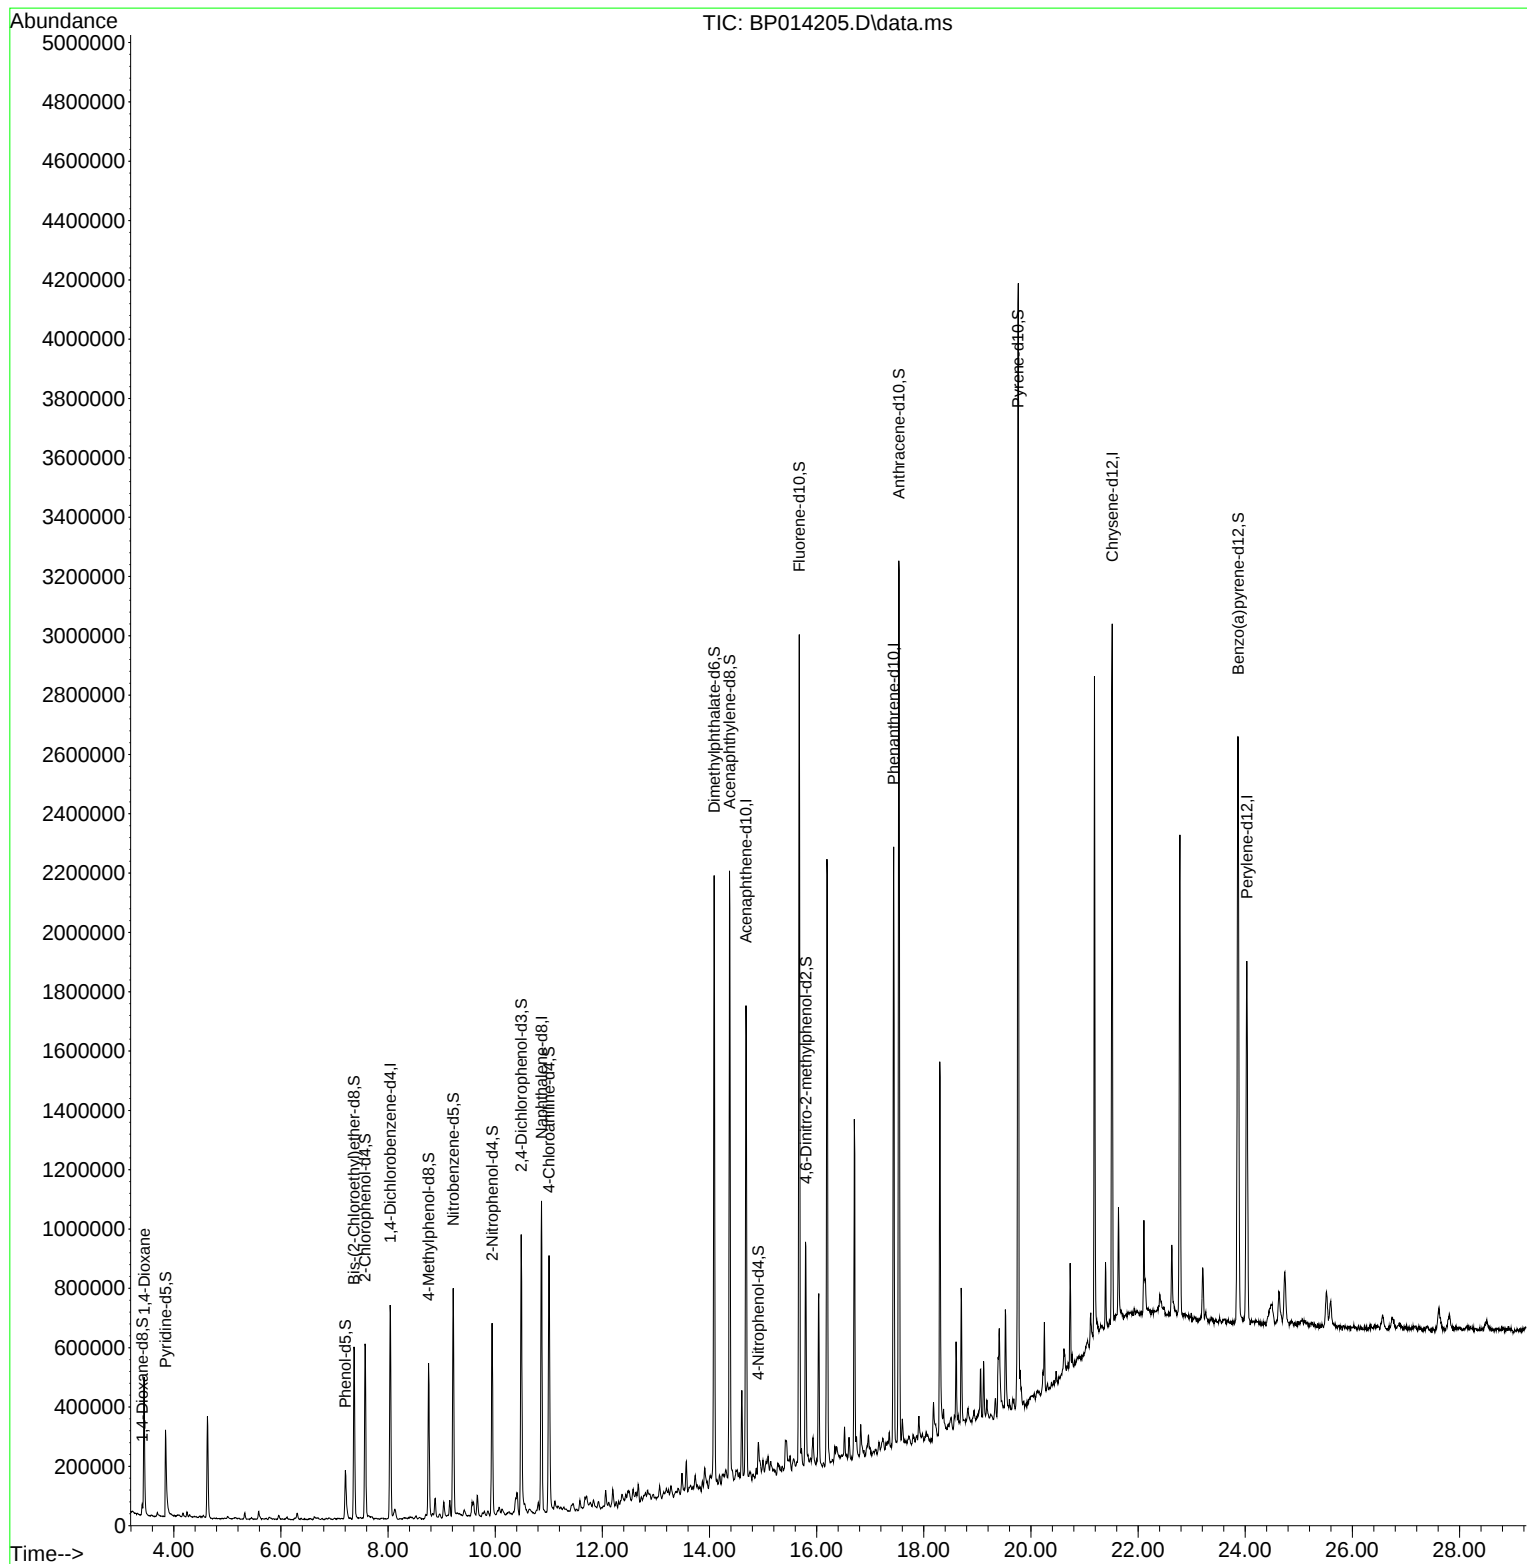

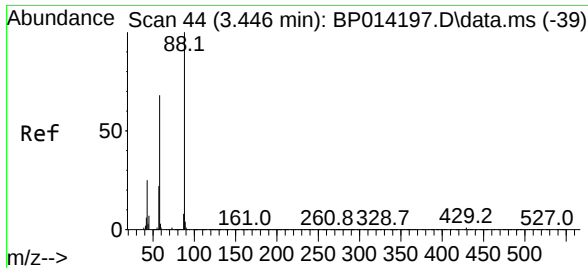

#2
 1,4-Dioxane
 Concen: 44.596 ng/uL
 RT: 3.446 min Scan# 44
 Delta R.T. 0.000 min
 Lab File: BP014205.D
 Acq: 22 Mar 2023 05:43

Instrument :
 BNA_P
 ClientSampleId :
 CB931

Tgt Ion: 88 Resp: 240170
 Ion Ratio Lower Upper
 88 100
 43 27.7 23.9 35.9
 58 69.4 50.2 75.2

