

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014209.D
 Acq On : 22 Mar 2023 07:59
 Operator : CG/JU
 Sample : 01996-10
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A31

Quant Time: Mar 22 08:27:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 22 03:05:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	197561	20.000	ng/u1	0.00
20) Naphthalene-d8	10.863	136	836067	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.681	164	571280	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.434	188	1288887	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.516	240	1071302	20.000	ng/u1	# 0.00
88) Perylene-d12	24.027	264	928980	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	25576	4.891	ng/uL	0.00
4) Pyridine-d5	3.852	84	105590	7.293	ng/u1	0.00
7) Phenol-d5	7.205	99	133133	7.636	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	319197	31.393	ng/u1	0.00
11) 2-Chlorophenol-d4	7.575	132	311975	23.487	ng/u1	0.00
15) 4-Methylphenol-d8	8.758	113	228380	16.037	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	198469	29.751	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	223471	27.985	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	401268	26.706	ng/u1	0.00
31) 4-Chloroaniline-d4	11.005	131	311928	15.687	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	1561590	32.209	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	1600476	31.162	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	55094	6.448	ng/u1	0.00
60) Fluorene-d10	15.675	176	1332916	32.439	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	270157	27.733	ng/u1	0.00
73) Anthracene-d10	17.539	188	2179542	34.834	ng/u1	0.00
81) Pyrene-d10	19.757	212	2549299	43.146	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.863	264	1748308	35.380	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.446	88	389396	68.983	ng/uL 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014209.D
Acq On : 22 Mar 2023 07:59
Operator : CG/JU
Sample : 01996-10
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A31

Quant Time: Mar 22 08:27:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 22 03:05:29 2023
Response via : Initial Calibration

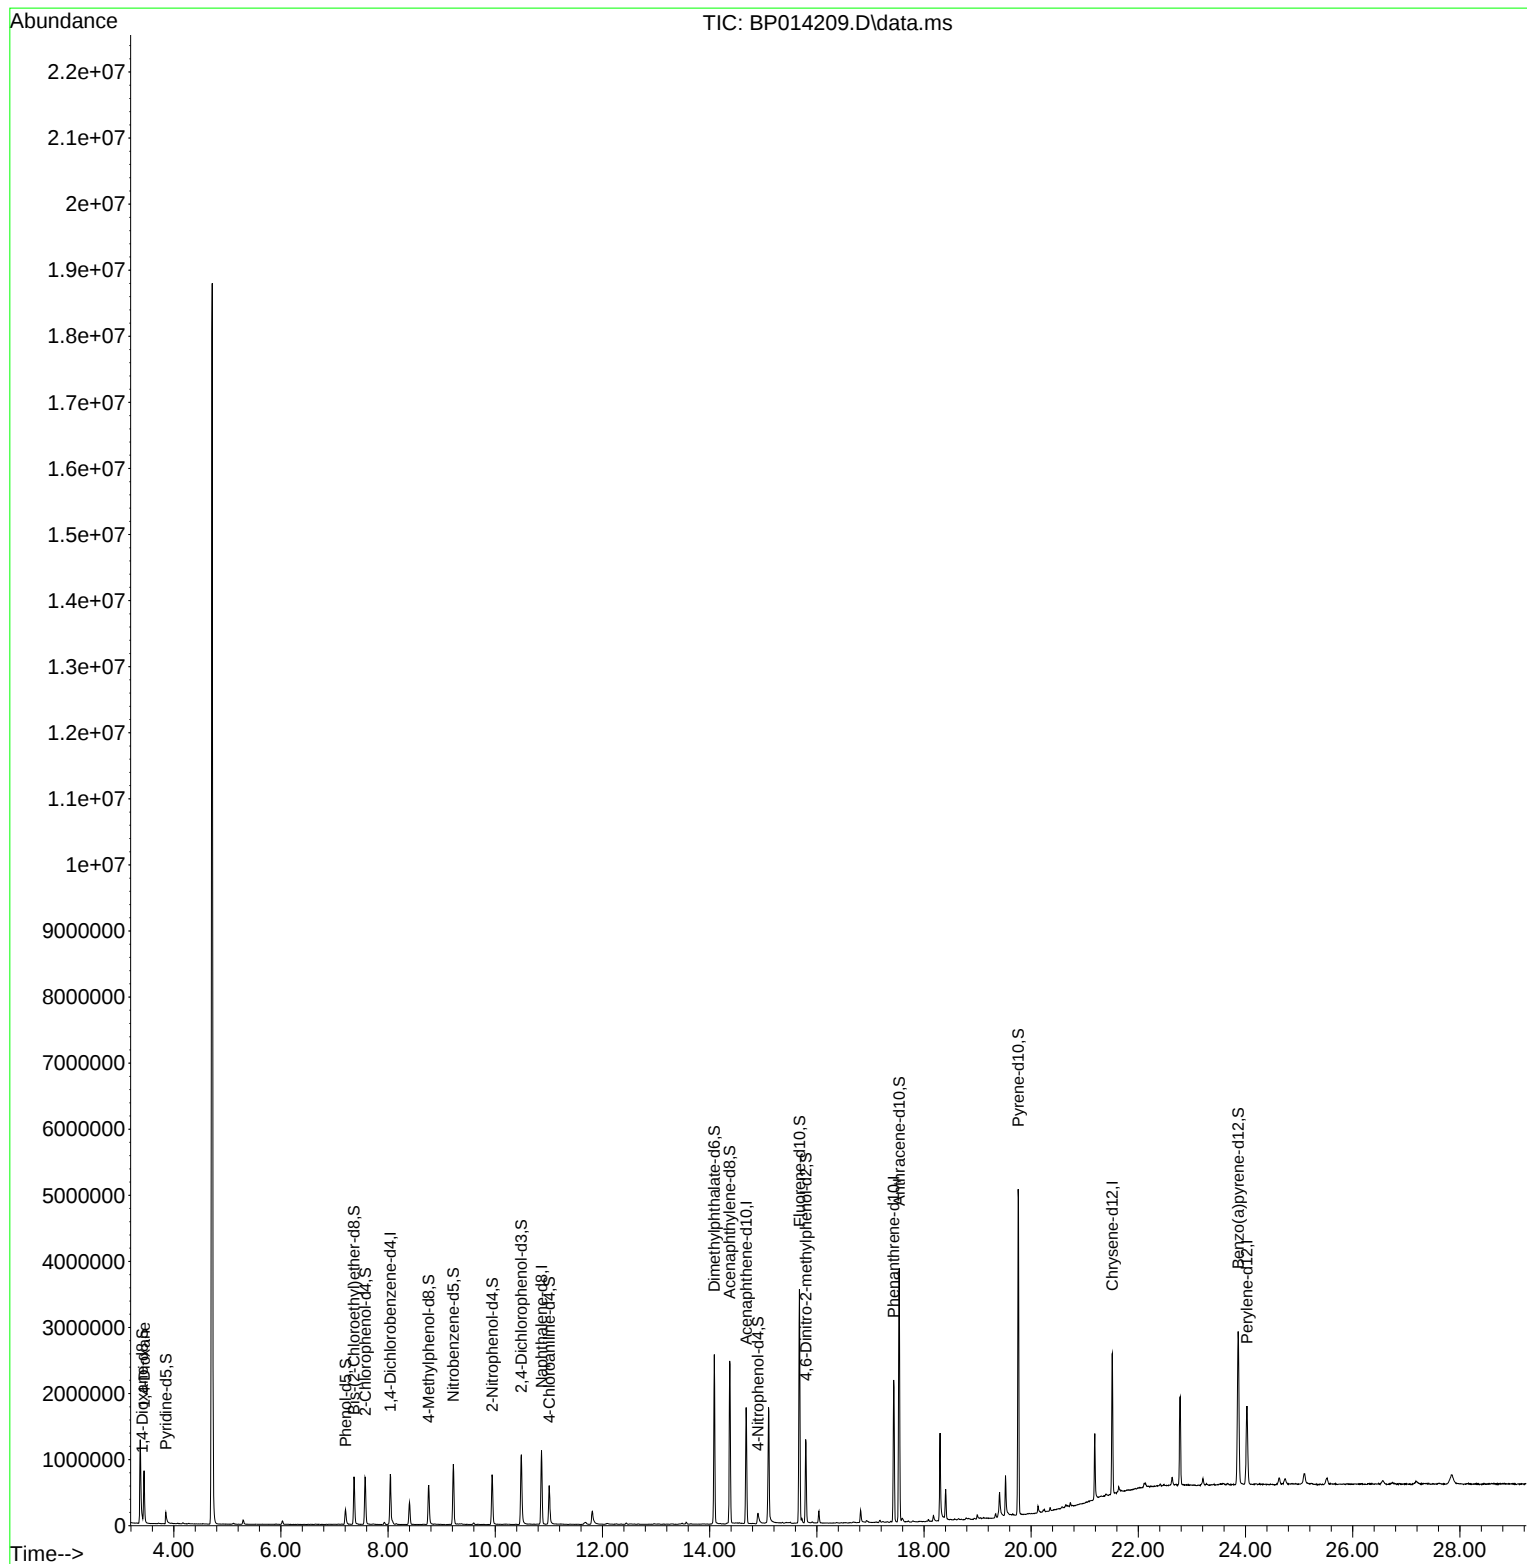

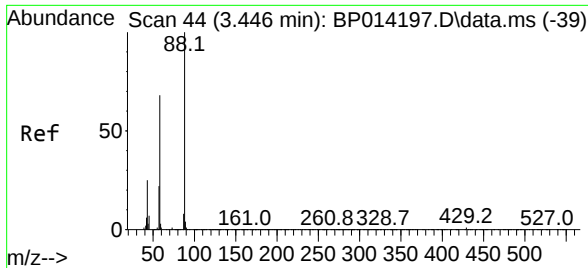

#2
 1,4-Dioxane
 Concen: 68.983 ng/uL
 RT: 3.446 min Scan# 44
 Delta R.T. 0.000 min
 Lab File: BP014209.D
 Acq: 22 Mar 2023 07:59

Instrument :
 BNA_P
 ClientSampleId :
 H0A31

Tgt Ion: 88 Resp: 389396
 Ion Ratio Lower Upper
 88 100
 43 28.7 23.9 35.9
 58 71.6 50.2 75.2

