

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014137.D
 Acq On : 20 Mar 2023 12:46
 Operator : CG/JU
 Sample : PB151502BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	6	9	15	rVB2	9867	13770	0.26%	0.029%
2	3.417	35	39	48	rVB	41310	57273	1.10%	0.120%
3	3.852	111	113	130	rBV	290917	489562	9.38%	1.029%
4	4.175	165	168	174	rVB	9469	13854	0.27%	0.029%
5	7.211	677	684	696	rBV	655285	1089963	20.88%	2.292%
6	7.375	705	712	726	rBV	509726	820413	15.72%	1.725%
7	7.581	740	747	758	rBV	660896	1093440	20.95%	2.299%
8	8.052	820	827	836	rBV	534748	868351	16.64%	1.826%
9	8.763	940	948	964	rBV	825610	1424730	27.30%	2.996%
10	9.228	1018	1027	1043	rBV	671443	1120186	21.46%	2.356%
11	9.952	1143	1150	1165	rBV	581499	1017258	19.49%	2.139%
12	10.499	1235	1243	1259	rBV	781604	1484971	28.45%	3.123%
13	10.875	1299	1307	1319	rVB	739471	1268298	24.30%	2.667%
14	11.016	1324	1331	1350	rBV	570228	1099693	21.07%	2.313%
15	12.463	1571	1577	1585	rBV2	11547	24449	0.47%	0.051%
16	13.581	1761	1767	1773	rVB3	13593	24598	0.47%	0.052%
17	13.669	1773	1782	1784	rBV9	3238	6258	0.12%	0.013%
18	14.098	1848	1855	1868	rBV	1812405	2519463	48.27%	5.298%
19	14.393	1897	1905	1915	rBV	1892957	2833252	54.29%	5.958%
20	14.698	1950	1957	1964	rBV	1285848	1937366	37.12%	4.074%
21	14.898	1985	1991	2013	rBV	550903	1237550	23.71%	2.602%
22	15.687	2118	2125	2134	rBV	2465718	3662898	70.18%	7.703%
23	15.810	2140	2146	2160	rBV	888988	1347647	25.82%	2.834%
24	15.928	2163	2166	2173	rVB5	13968	24695	0.47%	0.052%
25	16.475	2253	2259	2263	rBV9	4028	8709	0.17%	0.018%
26	17.128	2365	2370	2373	rBV7	6664	11396	0.22%	0.024%
27	17.451	2419	2425	2433	rBV	1858418	2546235	48.79%	5.354%
28	17.551	2435	2442	2453	rBV	3035415	4286602	82.13%	9.014%
29	18.092	2532	2534	2540	rVB7	5159	6840	0.13%	0.014%
30	18.316	2568	2572	2581	rBV4	46572	110627	2.12%	0.233%
31	19.351	2744	2748	2754	rBV4	45556	67831	1.30%	0.143%
32	19.422	2757	2760	2767	rVB	35739	55124	1.06%	0.116%
33	19.775	2814	2820	2830	rBV	3977228	5219021	100.00%	10.975%
34	21.533	3114	3119	3126	rBV	2109759	2849186	54.59%	5.991%
35	23.892	3513	3520	3531	rVB2	2118393	4432151	84.92%	9.320%
36	24.057	3542	3548	3556	rVB2	1207061	2480495	47.53%	5.216%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014137.D
Acq On : 20 Mar 2023 12:46
Operator : CG/JU
Sample : PB151502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47554155

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014137.D
Acq On : 20 Mar 2023 12:46
Operator : CG/JU
Sample : PB151502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

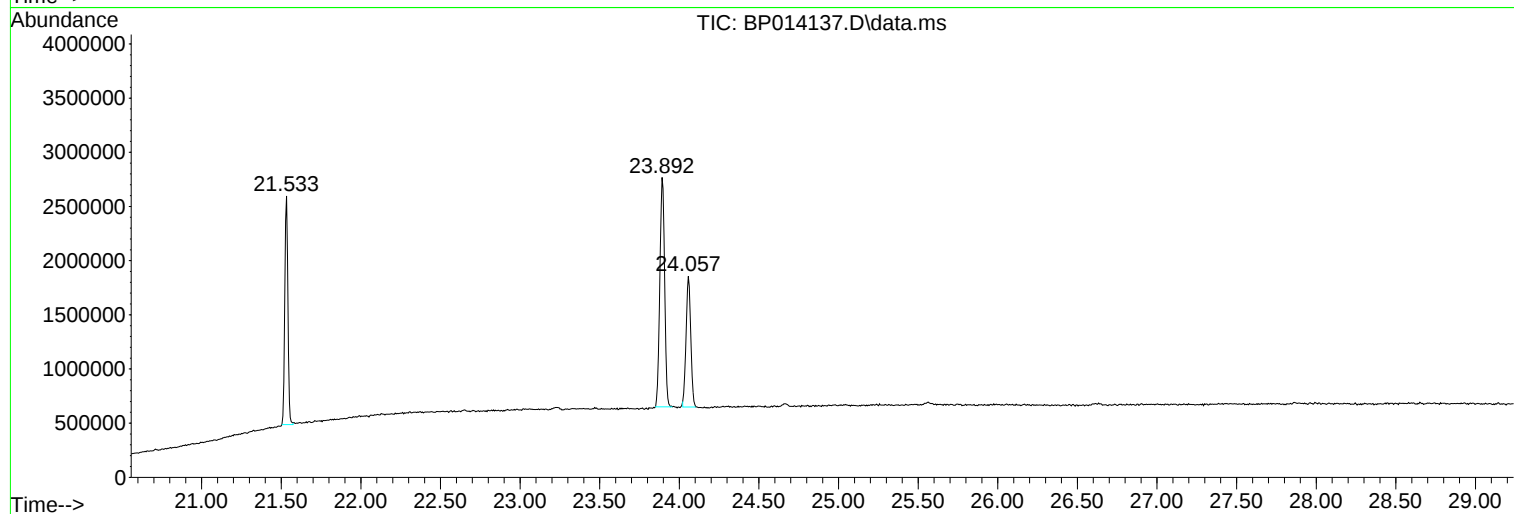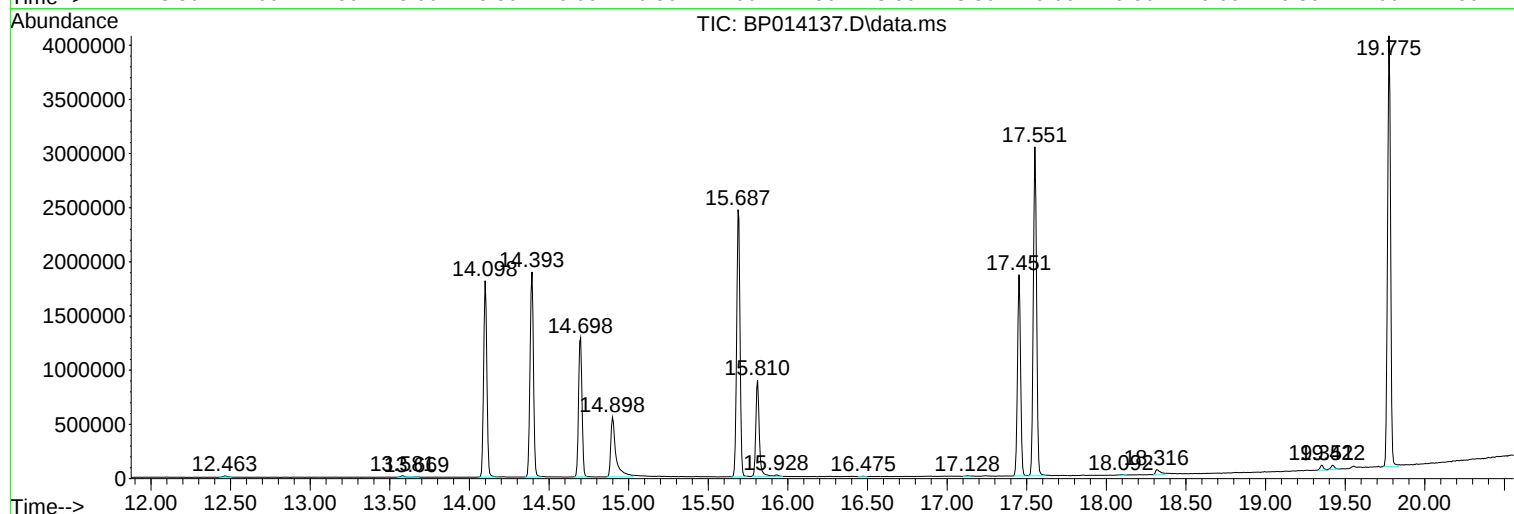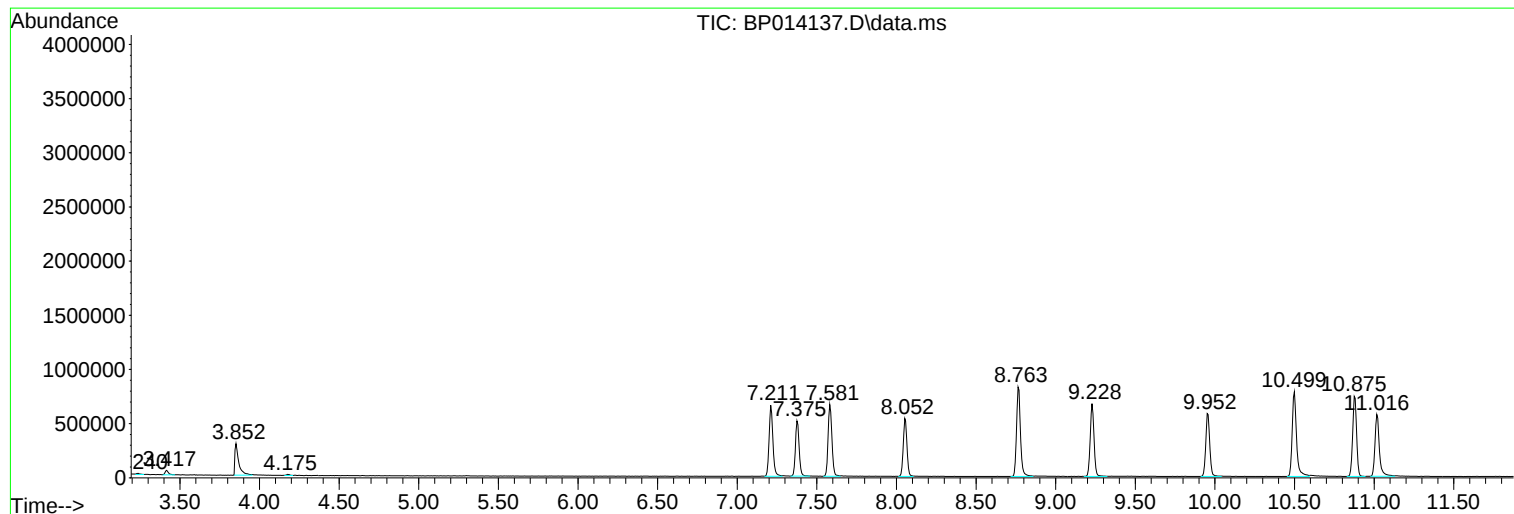

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014137.D
Acq On : 20 Mar 2023 12:46
Operator : CG/JU
Sample : PB151502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014137.D
Acq On : 20 Mar 2023 12:46
Operator : CG/JU
Sample : PB151502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc