

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014145.D
 Acq On : 20 Mar 2023 17:53
 Operator : CG/JU
 Sample : PB151507BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK507

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	35	39	45	rVB	39665	55278	1.11%	0.110%
2	3.852	110	113	129	rBV	358385	595953	11.93%	1.190%
3	4.181	164	169	174	rVB	11703	17389	0.35%	0.035%
4	4.634	245	246	255	rVB9	3579	5174	0.10%	0.010%
5	7.210	677	684	698	rBV	695262	1150354	23.03%	2.297%
6	7.375	705	712	722	rBV	548828	870294	17.42%	1.737%
7	7.581	740	747	760	rBV	696727	1145460	22.93%	2.287%
8	8.051	819	827	836	rBV	611863	976893	19.55%	1.950%
9	8.763	940	948	966	rBV	866379	1493566	29.90%	2.982%
10	9.228	1020	1027	1041	rBV	695744	1189405	23.81%	2.374%
11	9.951	1141	1150	1161	rBV	610171	1074395	21.51%	2.145%
12	10.498	1235	1243	1264	rBV	843243	1576587	31.56%	3.147%
13	10.875	1300	1307	1315	rBV	885011	1448738	29.00%	2.892%
14	11.016	1321	1331	1349	rBV	1359955	2482814	49.70%	4.957%
15	12.463	1570	1577	1590	rVB3	14301	30162	0.60%	0.060%
16	13.575	1759	1766	1771	rBV2	11318	19927	0.40%	0.040%
17	13.663	1776	1781	1786	rBV8	3747	5967	0.12%	0.012%
18	14.098	1848	1855	1872	rBV	1820288	2532043	50.68%	5.055%
19	14.392	1897	1905	1916	rBV	1911517	2875023	57.55%	5.740%
20	14.692	1949	1956	1965	rBV	1375757	2112946	42.29%	4.218%
21	14.898	1984	1991	2014	rBV	552610	1231498	24.65%	2.458%
22	15.686	2118	2125	2138	rBV	2574864	3664645	73.35%	7.316%
23	15.804	2139	2145	2162	rVV	914660	1403928	28.10%	2.803%
24	15.922	2162	2165	2174	rVB3	14162	28545	0.57%	0.057%
25	16.480	2254	2260	2263	rBV8	3158	5864	0.12%	0.012%
26	17.121	2364	2369	2374	rBV9	3548	8388	0.17%	0.017%
27	17.239	2385	2389	2391	rBV5	4900	7014	0.14%	0.014%
28	17.451	2418	2425	2434	rBV	1896127	2713937	54.32%	5.418%
29	17.551	2435	2442	2457	rVV	2956774	4149515	83.06%	8.284%
30	17.927	2504	2506	2511	rBV6	3873	5442	0.11%	0.011%
31	18.321	2568	2573	2582	rBV7	26536	68408	1.37%	0.137%
32	19.351	2744	2748	2754	rBV2	42719	57806	1.16%	0.115%
33	19.421	2756	2760	2764	rBV	37773	52154	1.04%	0.104%
34	19.774	2814	2820	2829	rBV	3841405	4995914	100.00%	9.974%
35	21.533	3113	3119	3127	rBV	2233421	3121603	62.48%	6.232%
36	23.892	3513	3520	3532	rVB2	2079282	4280839	85.69%	8.546%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014145.D
Acq On : 20 Mar 2023 17:53
Operator : CG/JU
Sample : PB151507BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK507

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION

37	24.056	3541	3548	3557	rVB2	1262352	2637663	52.80%	5.266%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 50091531

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014145.D
Acq On : 20 Mar 2023 17:53
Operator : CG/JU
Sample : PB151507BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK507

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

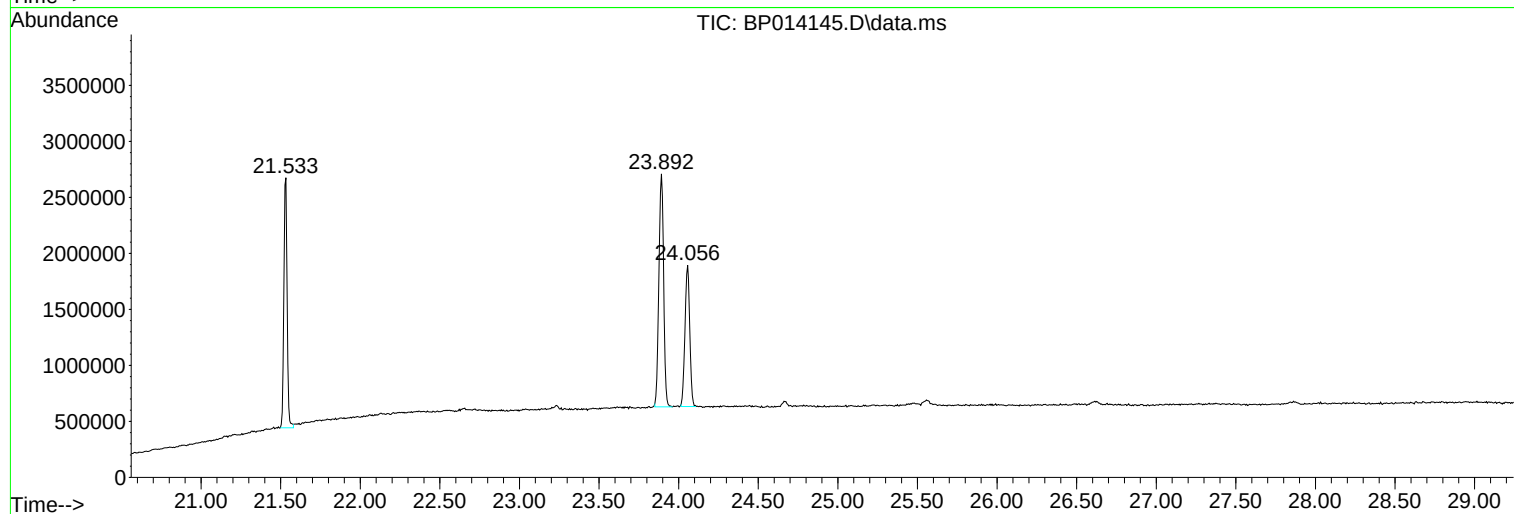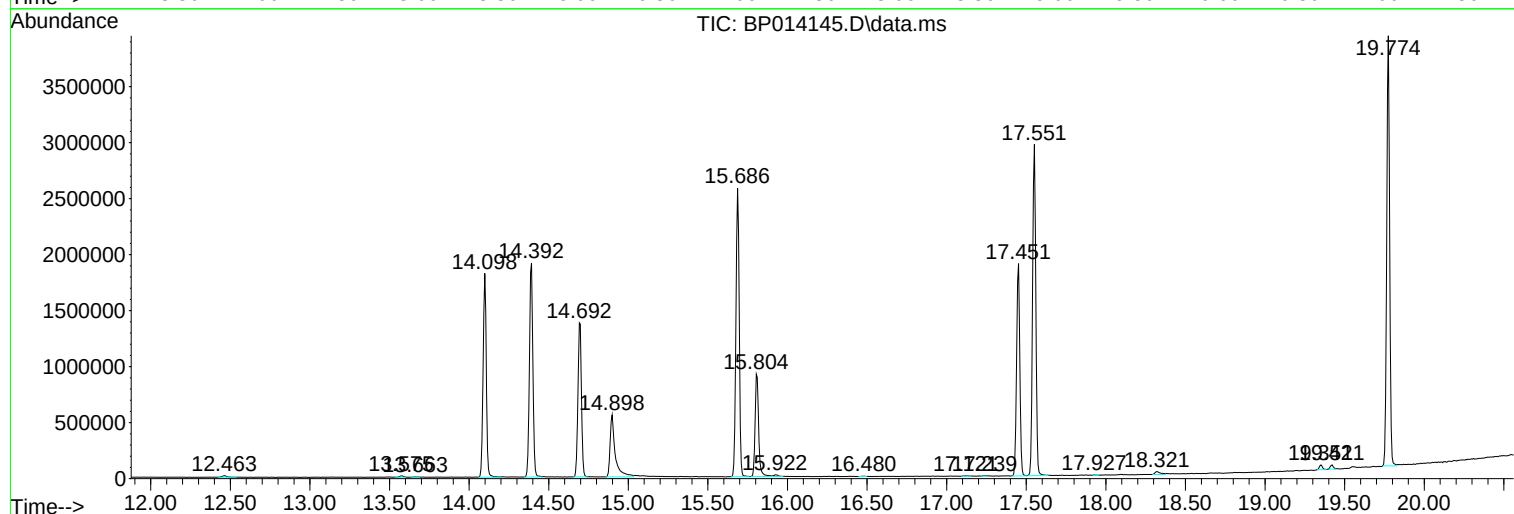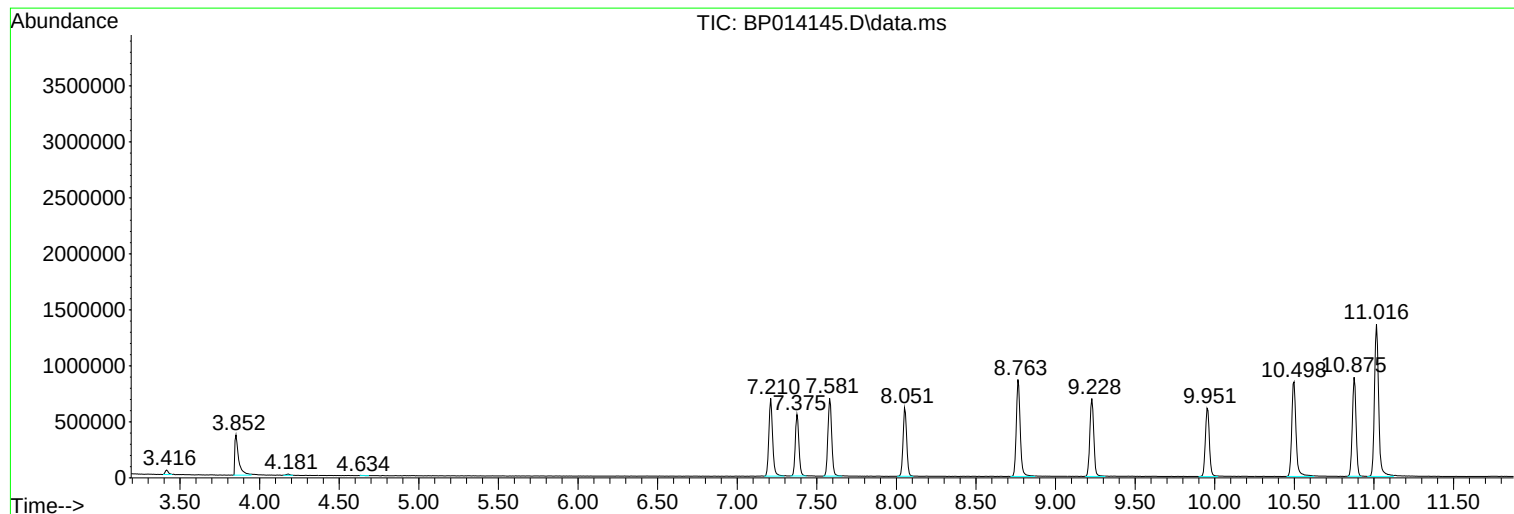

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014145.D
Acq On : 20 Mar 2023 17:53
Operator : CG/JU
Sample : PB151507BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK507

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014145.D
Acq On : 20 Mar 2023 17:53
Operator : CG/JU
Sample : PB151507BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK507

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc